
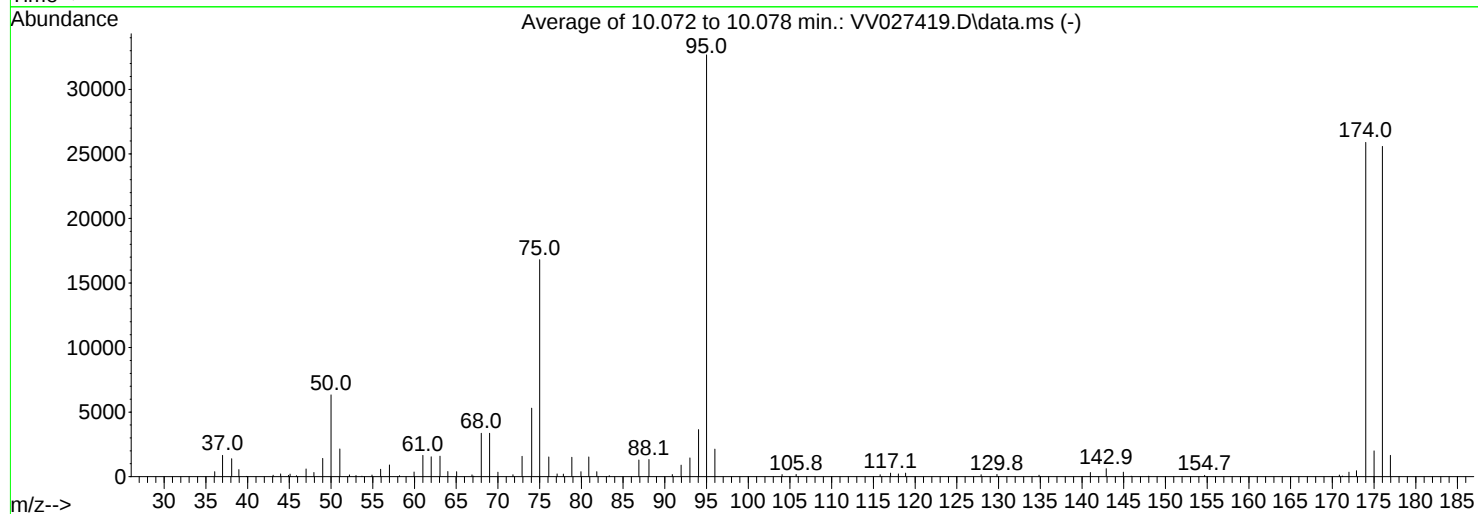


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
 Data File : VV027419.D
 Acq On : 17 Aug 2022 13:53
 Operator : SY/MD
 Sample : BFB309
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB309

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 18 02:23:52 2022

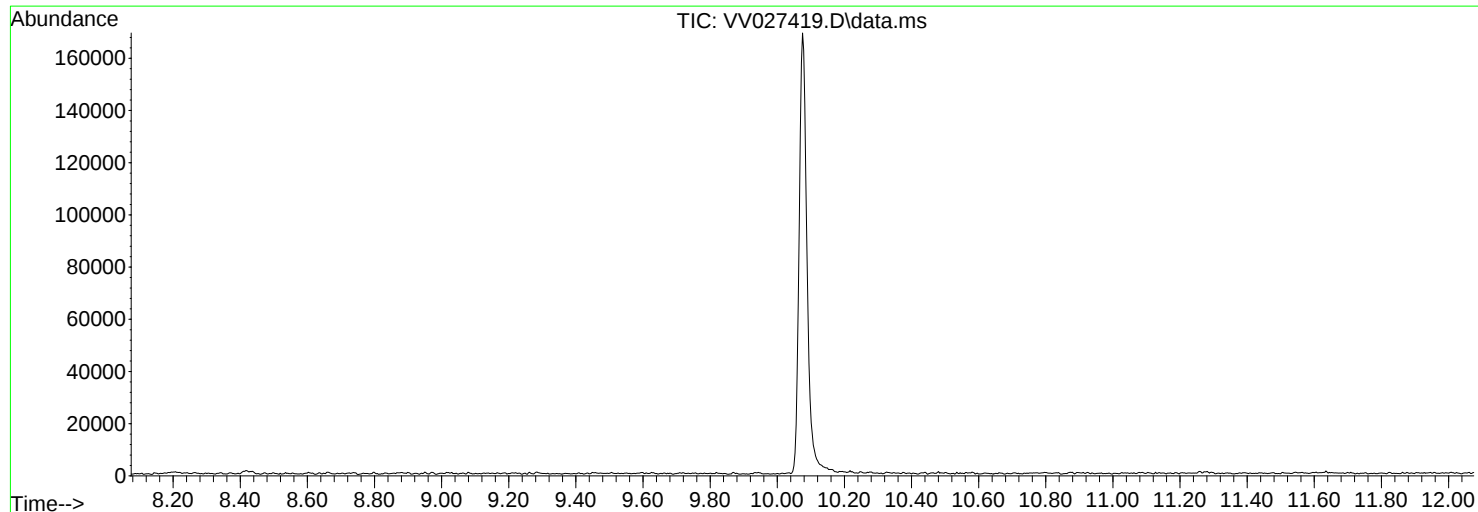

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	6338	PASS
75	95	30	80	51.4	16811	PASS
95	95	100	100	100.0	32675	PASS
96	95	5	9	6.5	2135	PASS
173	174	0.00	2	1.8	464	PASS
174	95	50	120	79.3	25899	PASS
175	174	5	9	7.7	1996	PASS
176	174	95	105	98.8	25587	PASS
177	176	5	10	6.4	1646	PASS

m/z	Abundance
37.90	162.0
39.90	354.0
44.10	339.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.00	363.0
37.00	1538.0
38.10	1396.0
38.90	586.0
39.90	378.0
43.00	105.0
43.90	537.0
44.90	288.0
45.90	106.0
47.00	517.0
47.90	281.0
49.00	1405.0
50.00	6093.0
51.00	2142.0
52.20	112.0
53.70	109.0
55.00	124.0
56.00	554.0
57.00	839.0
58.20	121.0
59.90	291.0
61.00	1703.0
62.00	1452.0
63.10	1534.0
64.00	393.0
65.00	361.0
66.90	115.0
67.10	114.0
68.00	3365.0
69.00	3392.0
70.00	324.0
71.80	163.0
72.90	1544.0
74.10	5120.0
75.00	16768.0
76.10	1514.0
77.10	207.0
77.90	232.0
78.90	1432.0
79.90	398.0
80.90	1447.0
81.90	419.0
83.30	115.0
86.90	1228.0
88.10	1327.0
90.90	163.0
92.00	896.0
93.00	1453.0
94.00	3668.0
95.00	31456.0
96.00	2173.0
104.00	148.0
105.70	164.0
115.80	125.0
117.10	275.0
118.00	178.0
118.90	283.0
127.90	179.0
129.80	121.0
134.90	122.0
141.10	296.0
143.00	583.0
145.00	358.0
148.00	109.0
154.70	158.0
171.20	151.0
172.00	299.0
172.90	500.0
174.00	24672.0
175.00	1898.0
176.00	24000.0
177.00	1444.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.10	390.0
37.00	1701.0
38.10	1439.0
39.00	551.0
39.90	396.0
43.00	106.0
43.90	539.0
45.10	305.0
47.00	634.0
47.90	332.0
49.00	1498.0
50.00	6649.0
51.10	2207.0
52.20	140.0
53.00	113.0
54.90	120.0
55.90	585.0
57.00	950.0
58.20	115.0
59.90	380.0
61.00	1676.0
62.00	1571.0
63.10	1647.0
64.00	386.0
65.10	399.0
66.90	157.0
68.00	3465.0
69.00	3472.0
70.00	367.0
71.80	162.0
72.90	1622.0
74.10	5515.0
75.00	17512.0
76.10	1612.0
77.10	197.0
77.80	205.0
78.90	1533.0
80.00	393.0
80.90	1591.0
81.90	391.0
83.40	118.0
86.90	1338.0
88.10	1354.0
90.90	176.0
92.00	915.0
93.00	1494.0
94.10	3803.0
95.00	33968.0
96.00	2208.0
104.10	162.0
105.80	180.0
115.80	158.0
117.10	281.0
118.00	235.0
118.80	291.0
127.90	155.0
129.80	177.0
134.90	112.0
141.00	311.0
142.90	615.0
144.90	347.0
154.70	144.0
170.90	167.0
172.00	380.0
172.90	483.0
174.00	26640.0
175.00	2108.0
176.00	26632.0
177.00	1695.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.10	392.0
37.00	1712.0
38.10	1321.0
39.00	501.0
39.90	380.0
43.10	116.0
43.90	586.0
45.10	276.0
45.80	118.0
47.00	631.0
48.00	341.0
49.00	1333.0
50.00	6271.0
51.10	2088.0
52.20	154.0
53.00	133.0
54.80	116.0
55.90	570.0
57.00	914.0
60.00	405.0
61.00	1565.0
62.00	1572.0
63.00	1587.0
64.00	396.0
65.10	379.0
66.90	154.0
68.00	3236.0
69.00	3199.0
70.00	344.0
71.80	125.0
72.90	1561.0
74.00	5298.0
75.00	16152.0
76.10	1466.0
77.10	222.0
77.80	169.0
78.80	1527.0
80.00	364.0
80.90	1550.0
81.80	344.0
86.90	1314.0
88.10	1284.0
90.90	160.0
91.90	854.0
93.00	1391.0
94.00	3479.0
95.00	32600.0
96.00	2023.0
104.10	159.0
105.70	174.0
115.80	167.0
116.90	281.0
118.00	218.0
118.80	255.0
127.90	115.0
129.80	217.0
134.80	103.0
140.90	366.0
142.80	672.0
144.90	335.0
145.90	104.0
170.80	198.0
172.00	363.0
172.90	410.0
174.00	26384.0
175.00	1983.0
176.00	26128.0
176.90	1799.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309