
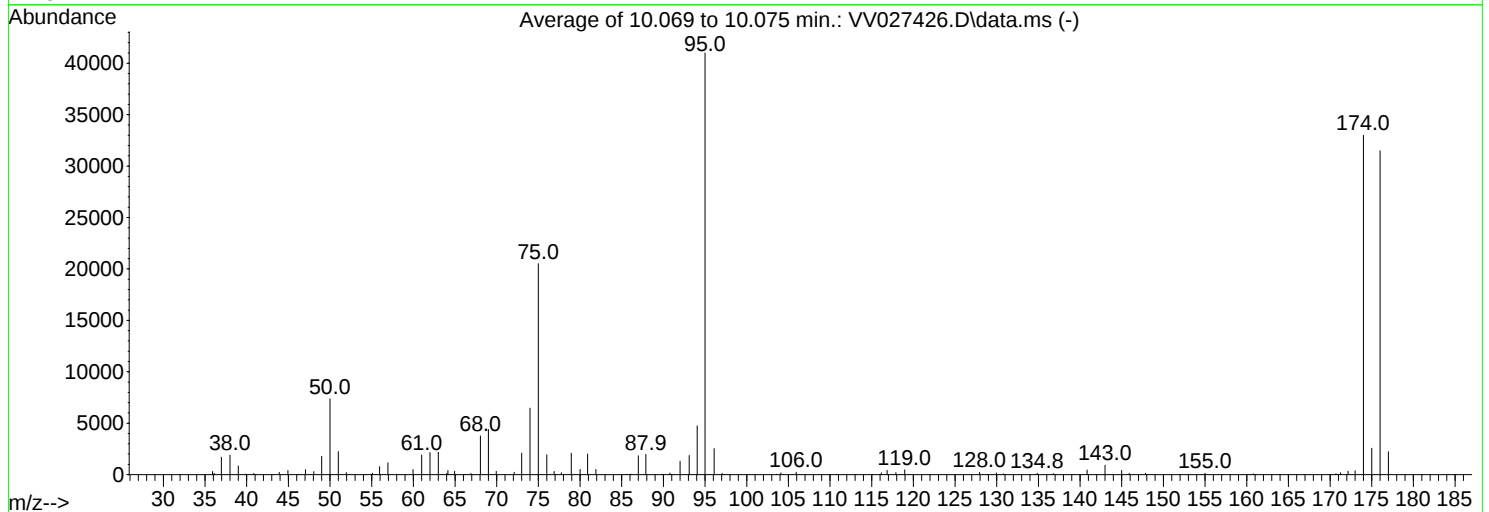


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
 Data File : VV027426.D
 Acq On : 18 Aug 2022 08:54
 Operator : SY/MD
 Sample : BFB310
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB310

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 18 02:23:52 2022

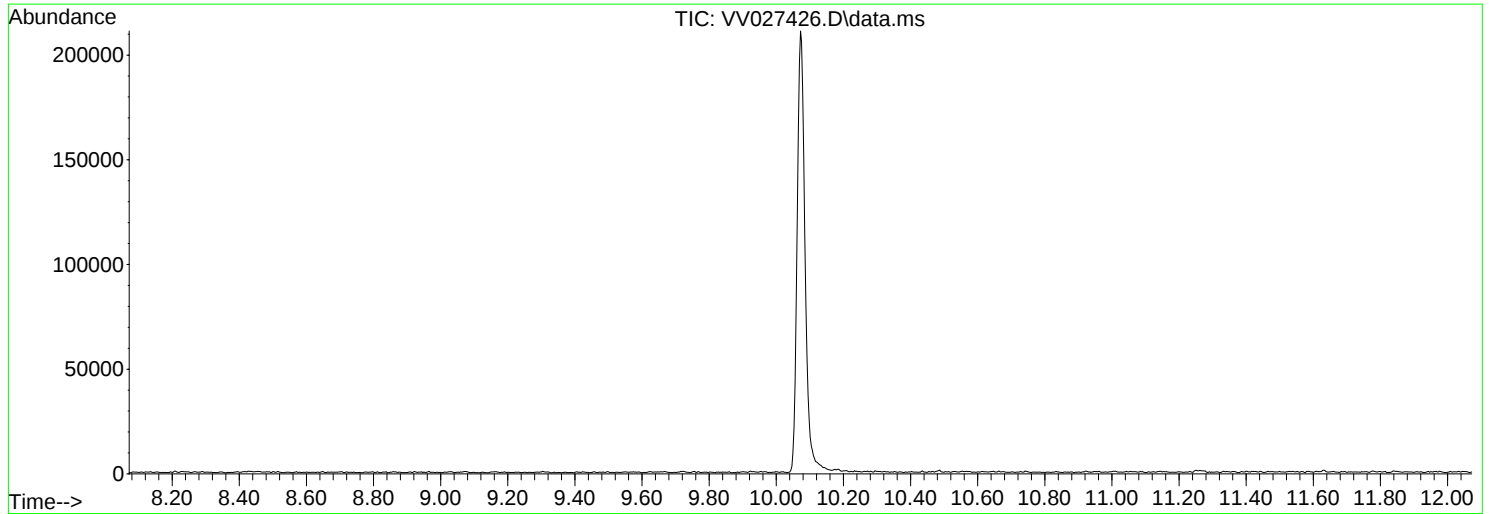

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	7379	PASS
75	95	30	80	50.0	20525	PASS
95	95	100	100	100.0	41011	PASS
96	95	5	9	6.2	2541	PASS
173	174	0.00	2	1.1	368	PASS
174	95	50	120	80.5	33003	PASS
175	174	5	9	7.8	2575	PASS
176	174	95	105	95.4	31485	PASS
177	176	5	10	7.1	2228	PASS

m/z	Abundance
38.40	108.0
39.90	325.0
44.00	316.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310

m/z	Abundance
35.90	480.0
36.90	1642.0
38.00	1886.0
39.00	772.0
40.00	385.0
41.00	131.0
43.90	517.0
44.90	376.0
46.20	106.0
47.10	478.0
48.10	297.0
49.00	1709.0
50.00	6938.0
51.00	2230.0
52.00	170.0
54.20	110.0
54.90	165.0
55.90	825.0
57.00	1223.0
58.00	100.0
60.00	504.0
61.00	2005.0
62.00	2132.0
63.00	2156.0
64.00	363.0
64.20	362.0
64.90	287.0
66.90	177.0
68.00	3769.0
69.00	4222.0
70.00	322.0
72.10	231.0
73.00	1997.0
74.00	6431.0
75.00	19816.0
76.00	1921.0
76.90	272.0
77.70	198.0
78.90	1890.0
80.00	495.0
80.90	1948.0
81.90	517.0
87.00	1723.0
87.90	1907.0
90.80	177.0
92.00	1285.0
93.10	1717.0
94.00	4534.0
95.00	39896.0
96.10	2576.0
97.10	105.0
104.10	189.0
106.00	222.0
116.20	144.0
116.90	396.0
117.90	195.0
119.00	447.0
127.90	214.0
130.00	196.0
130.80	103.0
134.80	142.0
136.70	109.0
140.90	459.0
143.00	936.0
145.00	360.0
146.00	142.0
147.80	131.0
155.00	117.0
160.80	109.0
171.20	157.0
172.20	275.0
174.00	30936.0
175.00	2481.0
176.00	29368.0
177.00	2212.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310

m/z	Abundance
35.90	434.0
36.90	1721.0
38.00	1973.0
39.00	840.0
39.90	389.0
40.80	125.0
43.90	533.0
45.00	409.0
47.00	493.0
48.00	286.0
49.00	1846.0
50.00	7649.0
51.00	2278.0
51.90	210.0
55.10	195.0
56.00	791.0
57.00	1165.0
58.00	104.0
60.00	538.0
61.00	1957.0
62.00	2227.0
63.00	2290.0
64.10	413.0
64.90	339.0
66.90	141.0
68.00	3898.0
69.00	4537.0
69.90	336.0
72.10	240.0
73.00	2149.0
74.00	6654.0
75.00	21280.0
76.00	2001.0
76.90	321.0
77.70	191.0
78.90	2170.0
80.00	530.0
80.90	2090.0
81.90	518.0
87.00	1892.0
87.90	2045.0
90.80	152.0
92.00	1352.0
93.10	1913.0
94.00	4925.0
95.00	42368.0
96.10	2610.0
97.00	107.0
104.10	172.0
105.90	223.0
116.10	182.0
116.90	422.0
117.90	223.0
119.00	489.0
128.00	240.0
129.90	178.0
130.80	129.0
134.80	151.0
136.80	110.0
140.80	463.0
143.00	950.0
143.90	103.0
145.00	437.0
145.90	116.0
147.90	143.0
155.00	166.0
160.80	129.0
170.70	127.0
171.30	201.0
172.10	337.0
173.00	513.0
174.00	34128.0
175.00	2690.0
176.00	32496.0
177.00	2342.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310

m/z	Abundance
36.10	397.0
37.00	1731.0
38.00	1852.0
39.00	922.0
39.90	375.0
40.70	110.0
43.90	538.0
45.00	411.0
47.00	497.0
48.00	294.0
49.00	1783.0
50.00	7550.0
51.00	2194.0
51.90	212.0
55.10	219.0
56.00	713.0
56.90	1062.0
59.90	477.0
61.00	1765.0
62.00	2061.0
63.00	2110.0
64.10	437.0
65.00	356.0
66.10	101.0
68.10	3631.0
69.00	4397.0
69.90	311.0
72.10	250.0
73.00	2104.0
74.00	6327.0
75.00	20480.0
76.00	1876.0
76.90	343.0
77.80	188.0
79.00	2215.0
80.00	533.0
80.90	1961.0
81.90	499.0
85.60	102.0
86.10	174.0
87.00	1876.0
87.90	1950.0
89.90	102.0
90.80	141.0
92.00	1290.0
93.10	1983.0
94.10	4778.0
95.00	40768.0
96.10	2436.0
97.00	118.0
103.60	121.0
104.10	134.0
105.90	262.0
110.80	106.0
116.10	208.0
116.80	443.0
117.90	201.0
118.90	475.0
128.00	215.0
128.90	113.0
129.90	164.0
134.90	124.0
136.90	114.0
140.80	437.0
143.00	861.0
145.00	410.0
145.80	113.0
147.90	128.0
153.00	107.0
155.00	161.0
157.10	116.0
170.70	137.0
171.30	206.0
172.10	388.0
173.00	590.0
174.00	33944.0
175.00	2553.0
176.00	32592.0
177.00	2129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB310