

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081924\
 Data File : VV036968.D
 Acq On : 19 Aug 2024 10:18
 Operator : SY/MD
 Sample : VV0819WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 20 04:43:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 20 04:42:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	693468	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	662661	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	319892	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	211687	38.219	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.440%
7) Chloroethane-d5	1.532	69	177988	40.749	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.500%
11) 1,1-Dichloroethene-d2	2.059	65	93856	39.614	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.220%
21) 2-Butanone-d5	3.796	46	262799	89.550	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.550%
24) Chloroform-d	4.246	84	432196	43.482	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.960%
26) 1,2-Dichloroethane-d4	4.940	65	283416	44.348	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.700%
32) Benzene-d6	4.953	84	853922	42.665	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.320%
36) 1,2-Dichloropropane-d6	5.985	67	288005	44.603	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.200%
41) Toluene-d8	7.239	98	743485	40.495	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.000%
43) trans-1,3-Dichloroprop...	7.551	79	125860	37.453	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.900%
47) 2-Hexanone-d5	8.027	63	148116	79.778	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.780%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	340672	45.950	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.900%
66) 1,2-Dichlorobenzene-d4	11.554	152	289935	44.478	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.960%
Target Compounds						
39) cis-1,3-Dichloropropene	6.911	75	8736	0.972	ug/L	Qvalue # 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081924\
Data File : VV036968.D
Acq On : 19 Aug 2024 10:18
Operator : SY/MD
Sample : VV0819WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 20 04:43:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 20 04:42:25 2024
Response via : Initial Calibration

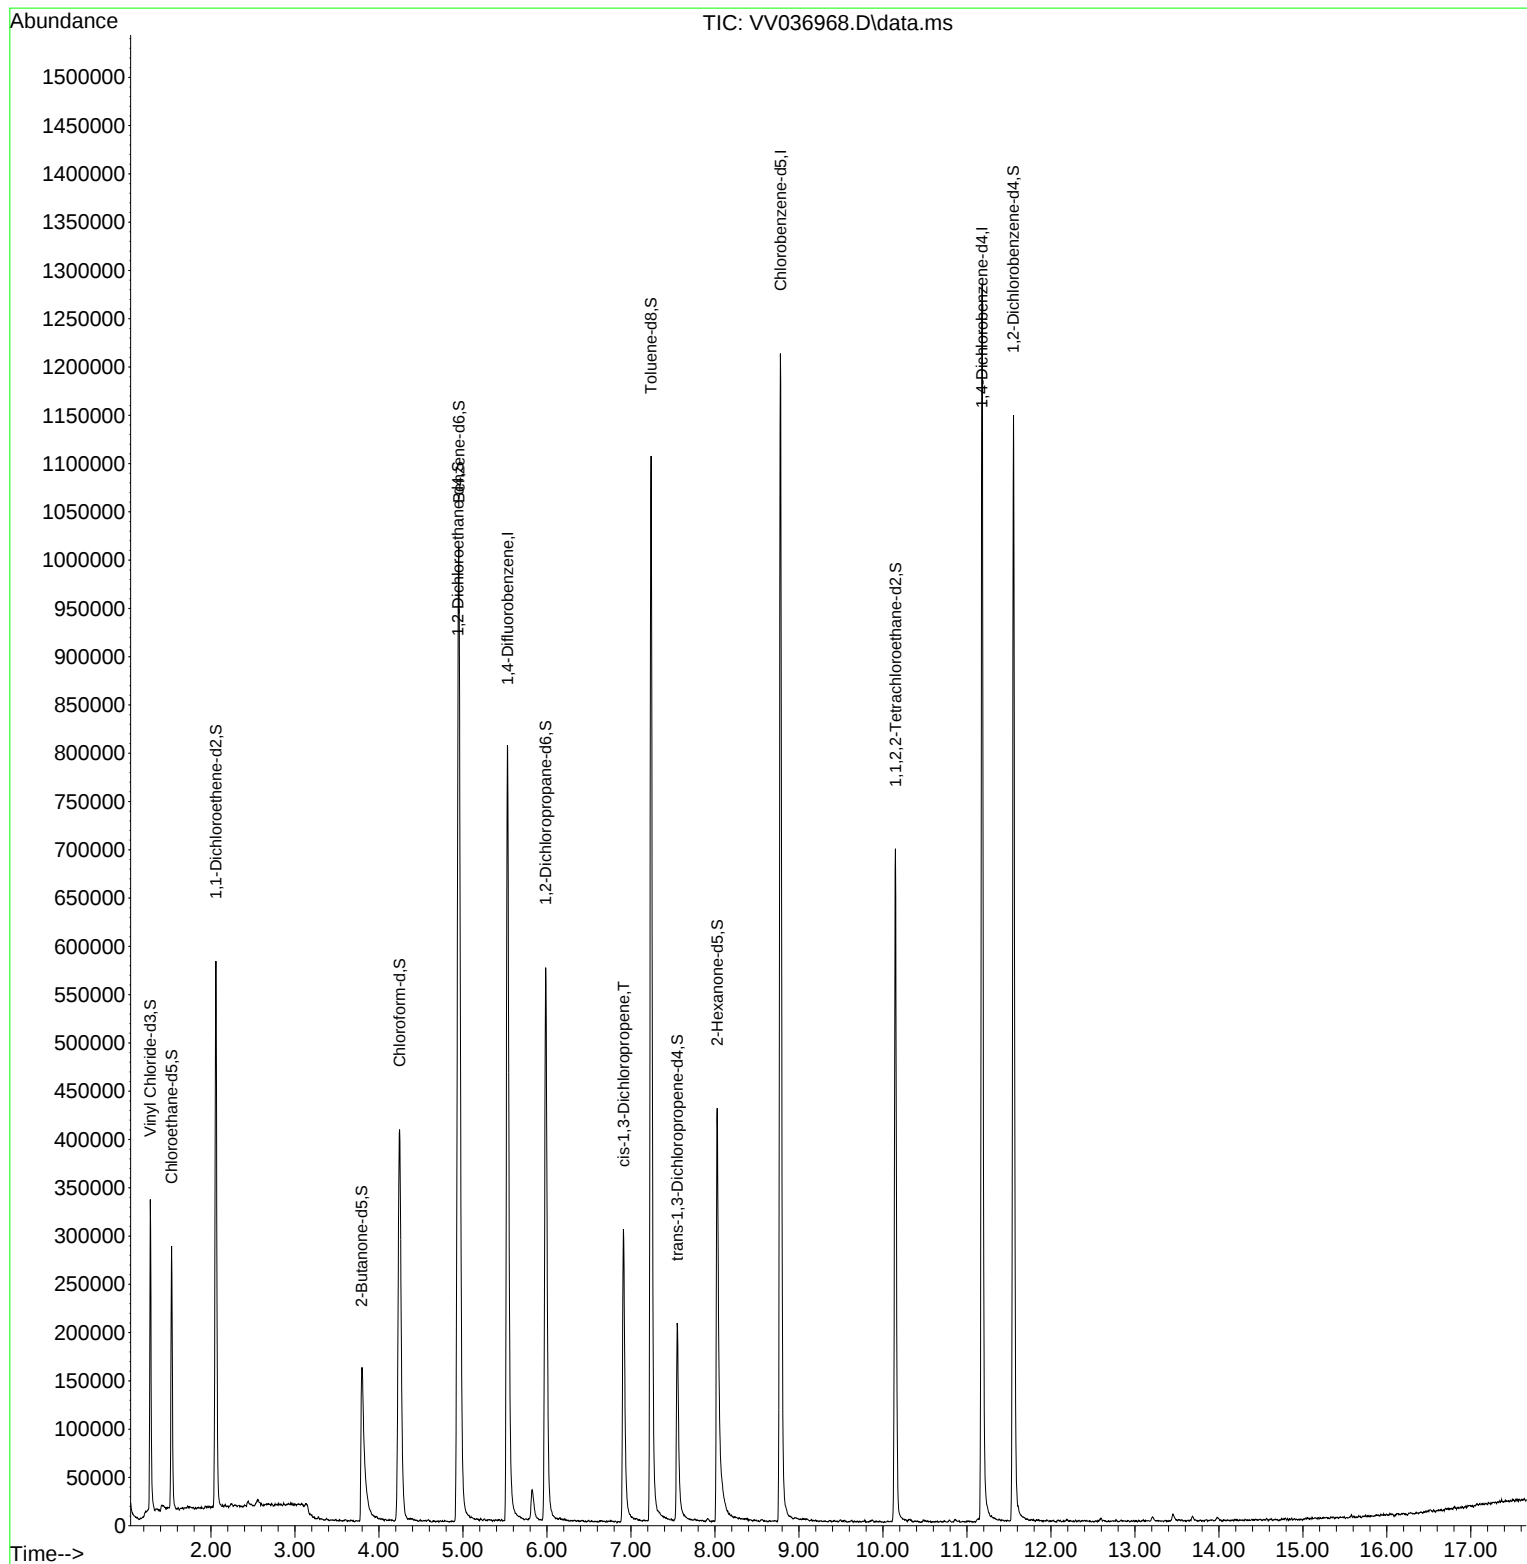

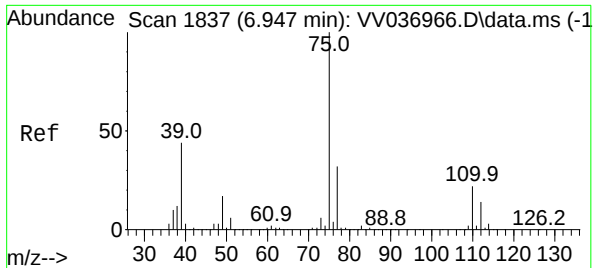

#39
 cis-1,3-Dichloropropene
 Concen: 0.972 ug/L
 RT: 6.911 min Scan# 11
 Delta R.T. -0.035 min
 Lab File: VV036968.D
 Acq: 19 Aug 2024 10:18

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 8736
 Ion Ratio Lower Upper
 75 100
 77 54.6 22.2 41.2#

