
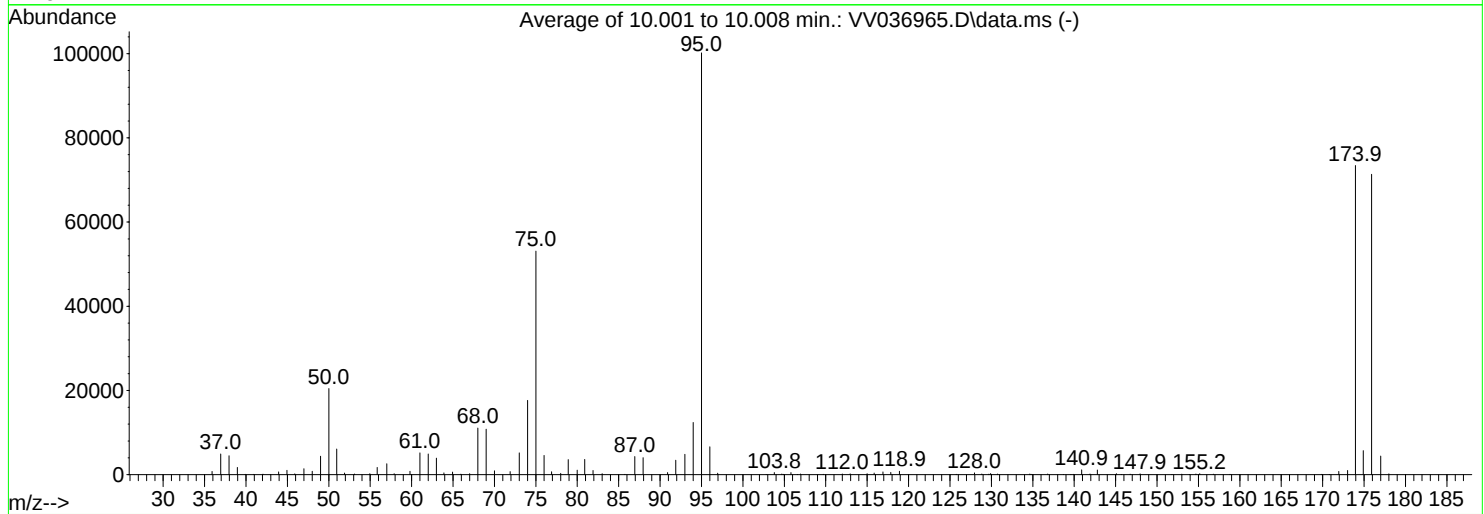


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081924\
Data File : VV036965.D
Acq On : 19 Aug 2024 08:35
Operator : SY/MD
Sample : BFB364
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB364

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis
Last Update : Tue Aug 20 04:42:25 2024

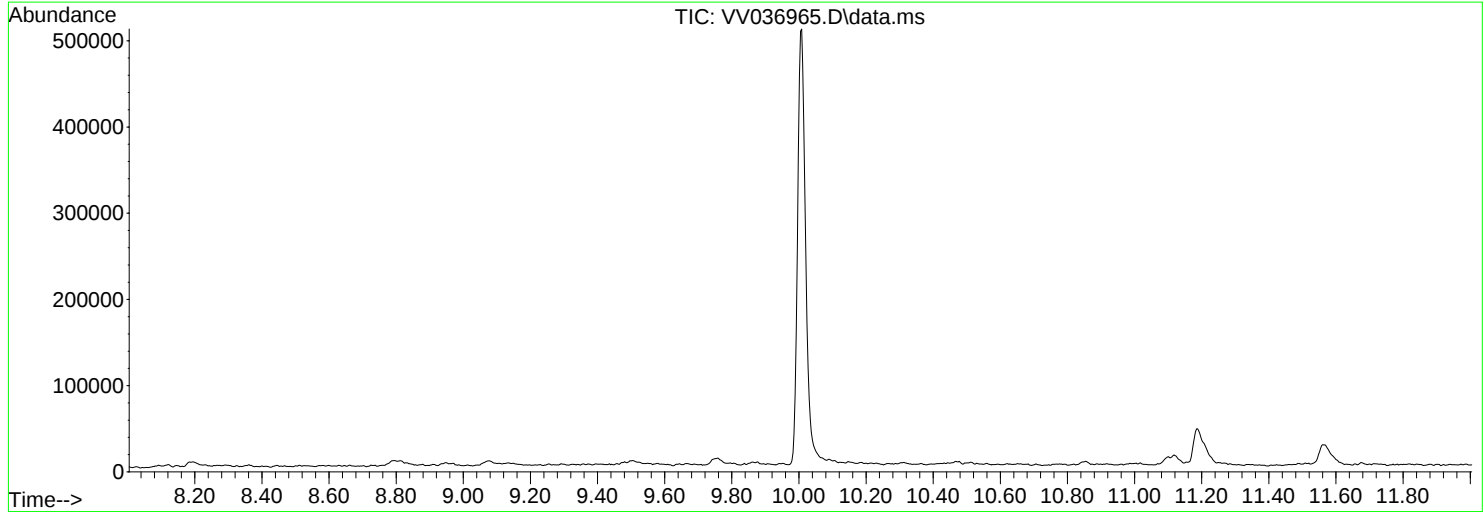

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	20453	PASS
75	95	30	80	53.0	53104	PASS
95	95	100	100	100.0	100189	PASS
96	95	5	9	6.6	6613	PASS
173	174	0.00	2	1.3	990	PASS
174	95	50	120	73.3	73427	PASS
175	174	5	9	7.8	5715	PASS
176	174	95	105	97.2	71344	PASS
177	176	5	10	6.2	4397	PASS

m/z	Abundance
35.90	2423.0
36.90	206.0
37.90	867.0
38.80	203.0
39.90	530.0
41.00	256.0
41.80	260.0
42.90	301.0
43.90	1132.0
45.00	118.0
50.80	105.0
52.00	127.0
54.10	115.0
54.90	192.0
55.80	151.0
56.40	101.0
57.20	114.0
59.80	124.0
63.80	128.0
67.00	140.0
70.00	129.0
76.90	203.0
78.00	159.0
79.00	120.0
94.30	112.0
108.00	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

m/z	Abundance
36.00	3292.0
37.00	5018.0
38.00	5094.0
39.00	1657.0
39.90	685.0
40.90	403.0
41.80	142.0
43.10	327.0
44.00	1740.0
45.00	1042.0
45.90	203.0
47.00	1271.0
48.00	805.0
49.00	4259.0
50.00	19160.0
51.00	6189.0
51.90	463.0
53.20	147.0
55.00	477.0
55.90	1631.0
57.00	2782.0
57.90	216.0
60.00	816.0
61.00	5235.0
62.00	4618.0
63.00	3738.0
63.90	519.0
64.90	554.0
65.90	123.0
67.00	363.0
68.00	10472.0
69.00	10383.0
70.00	985.0
71.90	743.0
73.00	5044.0
74.00	16632.0
75.00	49584.0
76.00	4070.0
76.90	858.0
78.10	471.0
78.90	3502.0
80.00	913.0
80.90	3299.0
81.90	930.0
83.00	272.0
85.80	131.0
87.00	4021.0
87.90	3787.0
90.90	519.0
91.90	3024.0
93.00	4402.0
94.00	11802.0
95.00	94152.0
96.00	6068.0
96.90	359.0
103.80	410.0
104.70	228.0
105.80	421.0
106.60	141.0
109.70	106.0
112.00	137.0
113.00	164.0
115.00	267.0
115.90	403.0
116.90	640.0
117.80	475.0
118.90	823.0
128.00	339.0
129.00	168.0
129.70	352.0
130.70	157.0
134.60	169.0
135.00	152.0
136.70	140.0
138.70	120.0
139.90	110.0
140.90	1054.0
141.90	181.0
142.80	1092.0
145.10	230.0
146.80	106.0
148.00	185.0
153.00	144.0
154.70	221.0
155.20	170.0
170.80	107.0
172.00	750.0
173.00	779.0
173.90	65960.0
174.90	5003.0
175.90	63512.0
177.00	4139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

177.90

138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

m/z	Abundance
36.00	3177.0
37.00	5245.0
38.00	5475.0
39.00	1991.0
39.90	586.0
40.90	355.0
42.10	183.0
43.10	344.0
44.00	1796.0
44.90	1184.0
45.90	200.0
47.00	1469.0
48.00	828.0
49.00	4467.0
50.00	20952.0
51.00	6408.0
51.90	529.0
53.10	132.0
55.00	437.0
55.90	1949.0
57.00	2842.0
57.90	220.0
59.80	942.0
61.00	5364.0
62.00	5057.0
63.00	3932.0
64.00	578.0
64.90	609.0
66.00	122.0
67.00	381.0
68.00	11499.0
69.00	11087.0
70.00	1092.0
71.90	745.0
73.00	5441.0
74.00	18120.0
75.00	54936.0
76.00	4721.0
76.90	951.0
78.00	497.0
78.90	3847.0
80.00	1121.0
80.90	3704.0
81.90	974.0
83.00	228.0
85.70	105.0
86.90	4543.0
88.00	4114.0
90.90	513.0
91.90	3570.0
93.00	5048.0
94.00	12947.0
95.00	103376.0
96.00	6779.0
96.90	358.0
102.80	104.0
103.80	510.0
104.70	209.0
105.80	491.0
106.90	217.0
109.70	117.0
112.00	150.0
112.90	191.0
115.00	272.0
115.90	393.0
116.90	647.0
117.90	543.0
118.90	826.0
125.70	111.0
127.90	416.0
128.80	147.0
129.90	371.0
130.70	187.0
134.70	241.0
136.80	158.0
139.90	109.0
140.90	1209.0
141.90	179.0
142.80	1175.0
145.10	273.0
146.80	130.0
147.90	205.0
151.80	101.0
153.00	121.0
153.90	108.0
154.70	222.0
155.10	246.0
156.80	150.0
158.80	106.0
169.90	104.0
172.00	791.0
173.00	985.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

173.90	76000.0
174.90	6002.0
175.90	73704.0
177.00	4545.0
178.00	178.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

m/z	Abundance
36.00	3084.0
37.00	5073.0
38.00	5538.0
39.00	2155.0
39.90	548.0
41.00	283.0
42.00	208.0
43.00	368.0
44.00	1758.0
44.90	1266.0
45.90	160.0
47.00	1481.0
48.00	782.0
49.00	4368.0
50.00	21248.0
51.00	5927.0
51.90	514.0
53.00	158.0
55.00	416.0
55.90	1971.0
57.00	2505.0
57.90	212.0
59.80	1015.0
61.00	4970.0
62.00	5007.0
63.00	4067.0
64.00	550.0
65.00	627.0
66.00	154.0
67.00	321.0
68.00	11209.0
69.00	10936.0
70.00	1075.0
71.90	685.0
73.00	4981.0
74.00	18168.0
75.00	54792.0
76.00	4954.0
76.90	838.0
78.00	471.0
78.90	3760.0
80.00	1225.0
80.90	3855.0
81.90	1029.0
83.00	182.0
86.90	4381.0
88.00	4187.0
90.90	446.0
91.90	3726.0
93.00	5092.0
94.00	12445.0
95.00	103040.0
96.00	6993.0
97.00	292.0
103.80	587.0
104.90	203.0
105.80	529.0
107.00	245.0
112.00	137.0
112.90	175.0
115.00	186.0
115.80	394.0
116.90	617.0
117.90	556.0
118.90	736.0
125.80	101.0
127.90	468.0
128.80	168.0
129.90	469.0
130.80	171.0
134.80	266.0
136.90	182.0
139.60	116.0
140.90	1148.0
141.90	159.0
142.80	1096.0
145.10	223.0
145.70	105.0
146.70	125.0
147.90	223.0
153.00	108.0
155.10	303.0
156.80	185.0
158.80	112.0
169.90	136.0
171.90	710.0
173.00	1205.0
174.00	78320.0
174.90	6139.0
175.90	76816.0
177.00	4506.0
178.10	237.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364