

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037114.D
 Acq On : 28 Aug 2024 01:58
 Operator : SY/MD
 Sample : P3693-20
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 28 06:16:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 28 05:52:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	614757	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	593532	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	275698	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	151206	26.888	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	53.780%#		
7) Chloroethane-d5	1.532	69	146092	33.614	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	67.220%#		
11) 1,1-Dichloroethene-d2	2.056	65	78650	33.276	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.560%		
21) 2-Butanone-d5	3.796	46	220504	101.255	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.250%		
24) Chloroform-d	4.243	84	367948	41.806	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.620%		
26) 1,2-Dichloroethane-d4	4.937	65	242023	43.666	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.340%		
32) Benzene-d6	4.953	84	721406	40.241	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.480%		
36) 1,2-Dichloropropane-d6	5.985	67	237782	42.348	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	84.700%		
41) Toluene-d8	7.239	98	637525	39.404	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	78.800%#		
43) trans-1,3-Dichloroprop...	7.554	79	87914	33.843	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.680%		
47) 2-Hexanone-d5	8.024	63	133881	87.365	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	87.370%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	305211	44.819	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.640%		
66) 1,2-Dichlorobenzene-d4	11.554	152	244529	44.285	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.580%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	9280	3.973	ug/L	91
48) 2-Hexanone	8.027	43	16496	4.569	ug/L #	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037114.D
Acq On : 28 Aug 2024 01:58
Operator : SY/MD
Sample : P3693-20
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 28 06:16:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 28 05:52:22 2024
Response via : Initial Calibration




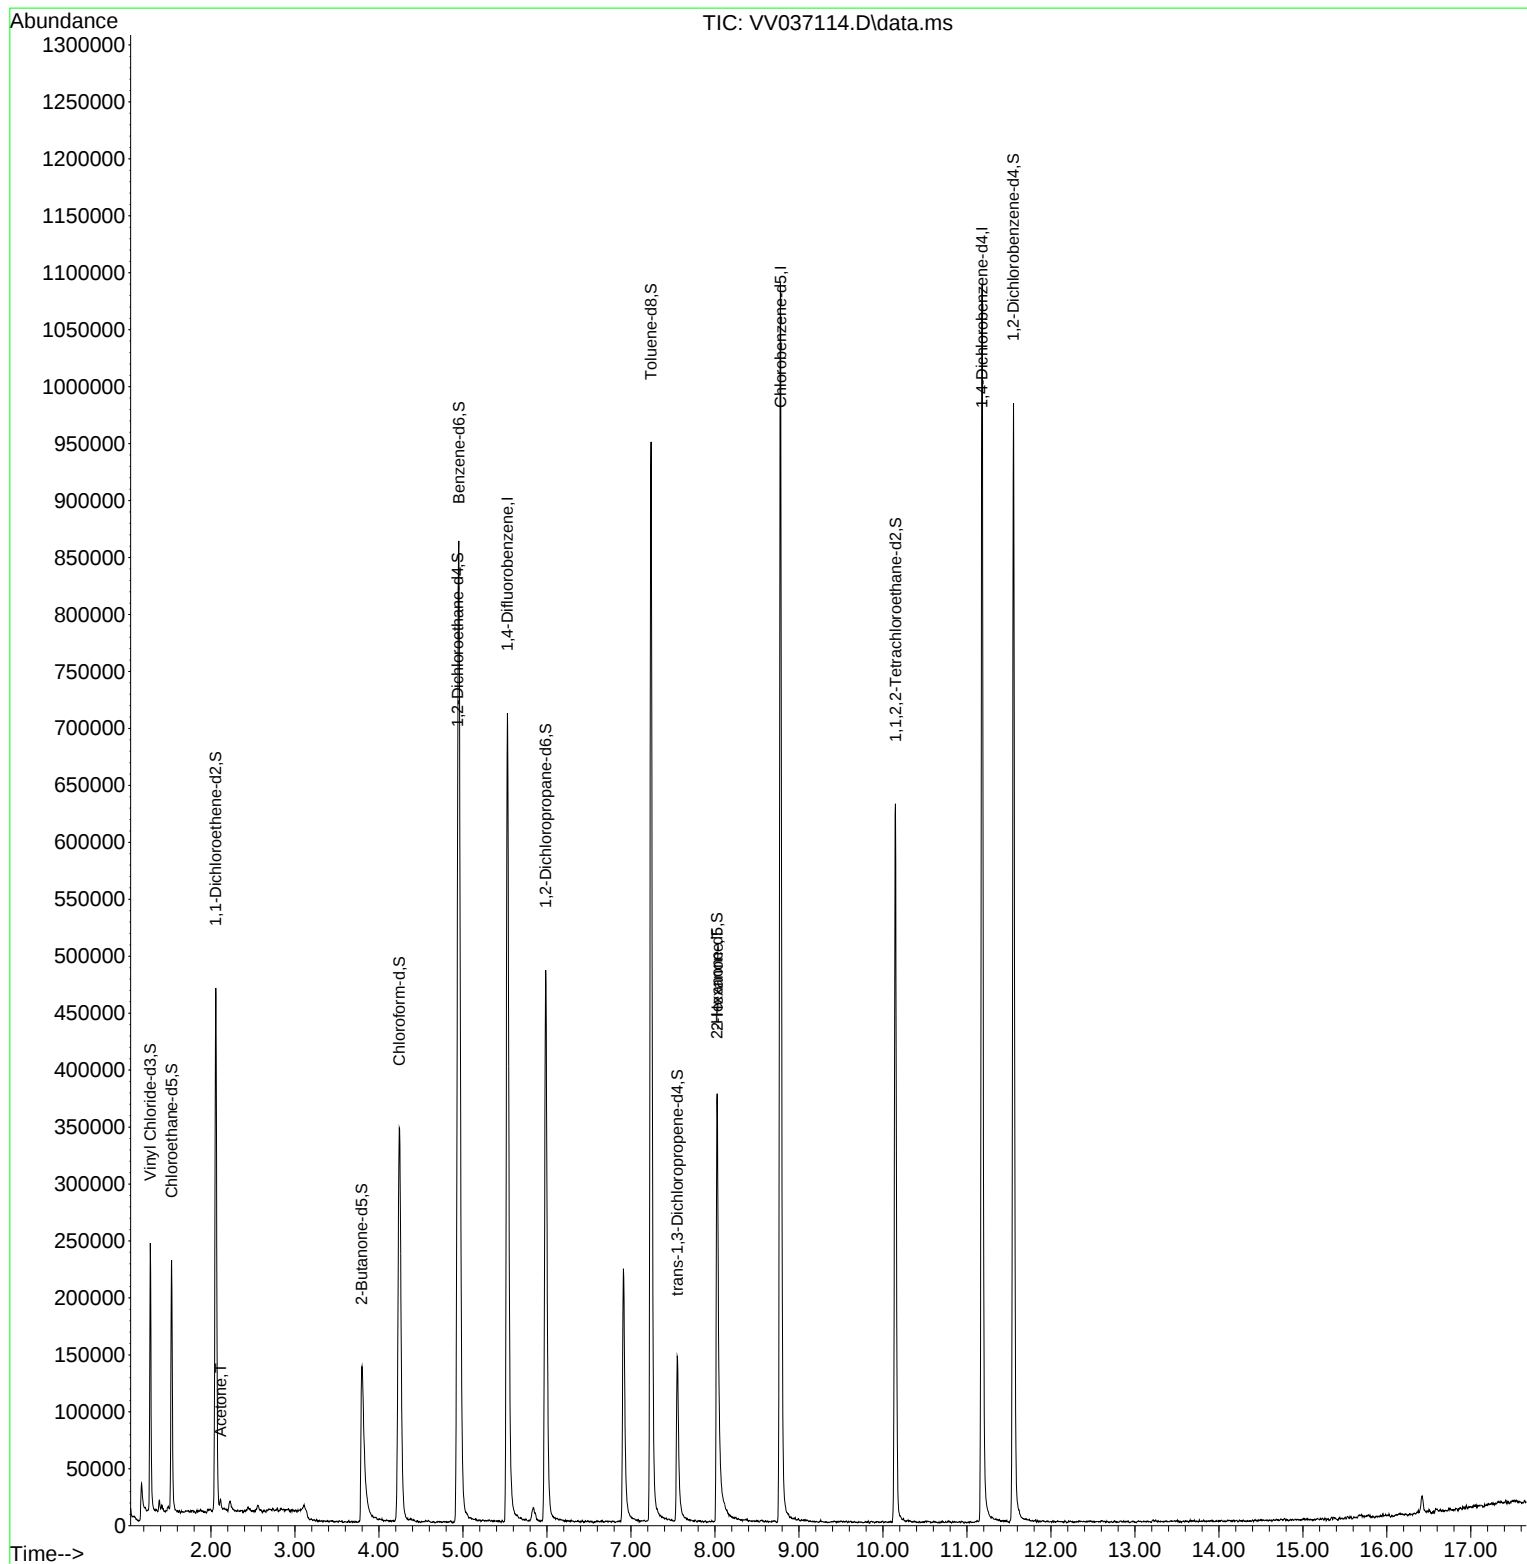


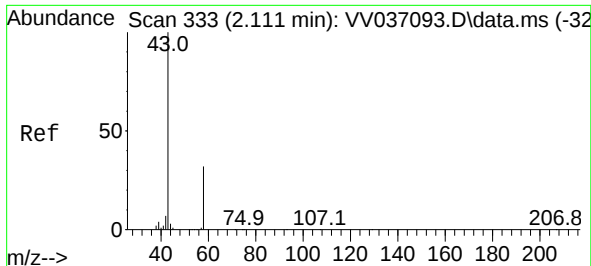

#13
Acetone
Concen: 3.973 ug/L
RT: 2.114 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV037114.D
Acq: 28 Aug 2024 01:58

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 43 Resp: 9280
Ion Ratio Lower Upper
43 100
58 37.2 0.0 64.8

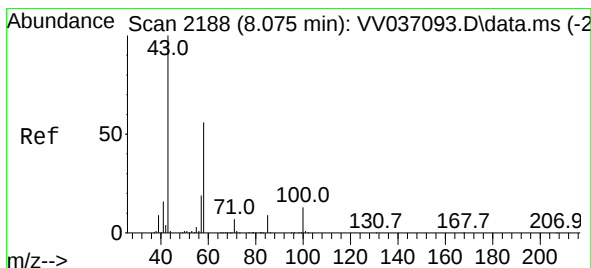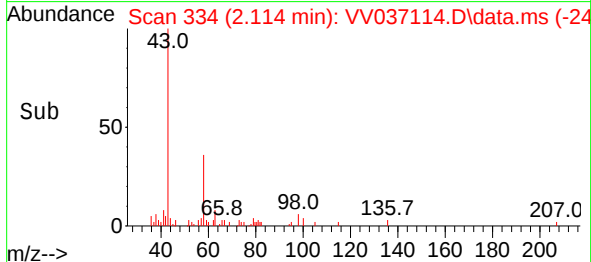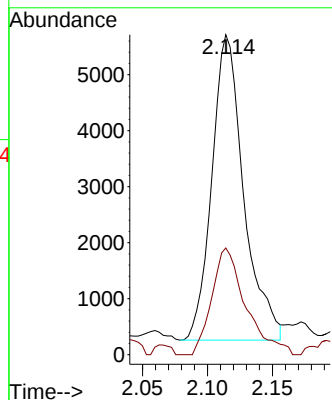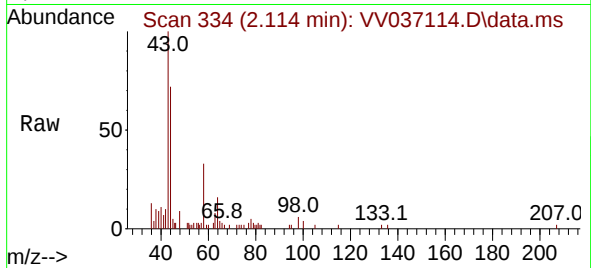

#48
2-Hexanone
Concen: 4.569 ug/L
RT: 8.027 min Scan# 2173
Delta R.T. -0.048 min
Lab File: VV037114.D
Acq: 28 Aug 2024 01:58

Tgt Ion: 43 Resp: 16496
Ion Ratio Lower Upper
43 100
58 36.5 46.0 69.0#
57 26.4 15.6 23.4#
100 2.8 10.6 16.0#

