

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037088.D
 Acq On : 27 Aug 2024 15:58
 Operator : SY/MD
 Sample : P3692-13
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K41

Quant Time: Aug 28 04:21:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 28 04:16:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	678696	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	644056	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	317370	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	202319	32.588	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	65.180%		
7) Chloroethane-d5	1.532	69	183870	38.320	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	76.640%		
11) 1,1-Dichloroethene-d2	2.056	65	102528	39.291	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.580%		
21) 2-Butanone-d5	3.796	46	259739	108.035	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	108.030%		
24) Chloroform-d	4.243	84	427698	44.017	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.040%		
26) 1,2-Dichloroethane-d4	4.937	65	285717	46.693	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.380%		
32) Benzene-d6	4.953	84	837770	43.066	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.140%		
36) 1,2-Dichloropropane-d6	5.986	67	270156	44.339	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.680%		
41) Toluene-d8	7.240	98	755109	43.010	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.020%		
43) trans-1,3-Dichloroprop...	7.551	79	115255	40.887	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.780%		
47) 2-Hexanone-d5	8.024	63	173720	104.470	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	104.470%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	349165	47.251	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.500%		
66) 1,2-Dichlorobenzene-d4	11.554	152	285985	44.992	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.980%		
Target Compounds						Qvalue
20) cis-1,2-Dichloroethene	3.809	96	22128	4.356	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037088.D
Acq On : 27 Aug 2024 15:58
Operator : SY/MD
Sample : P3692-13
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K41


Quant Time: Aug 28 04:21:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 28 04:16:12 2024
Response via : Initial Calibration

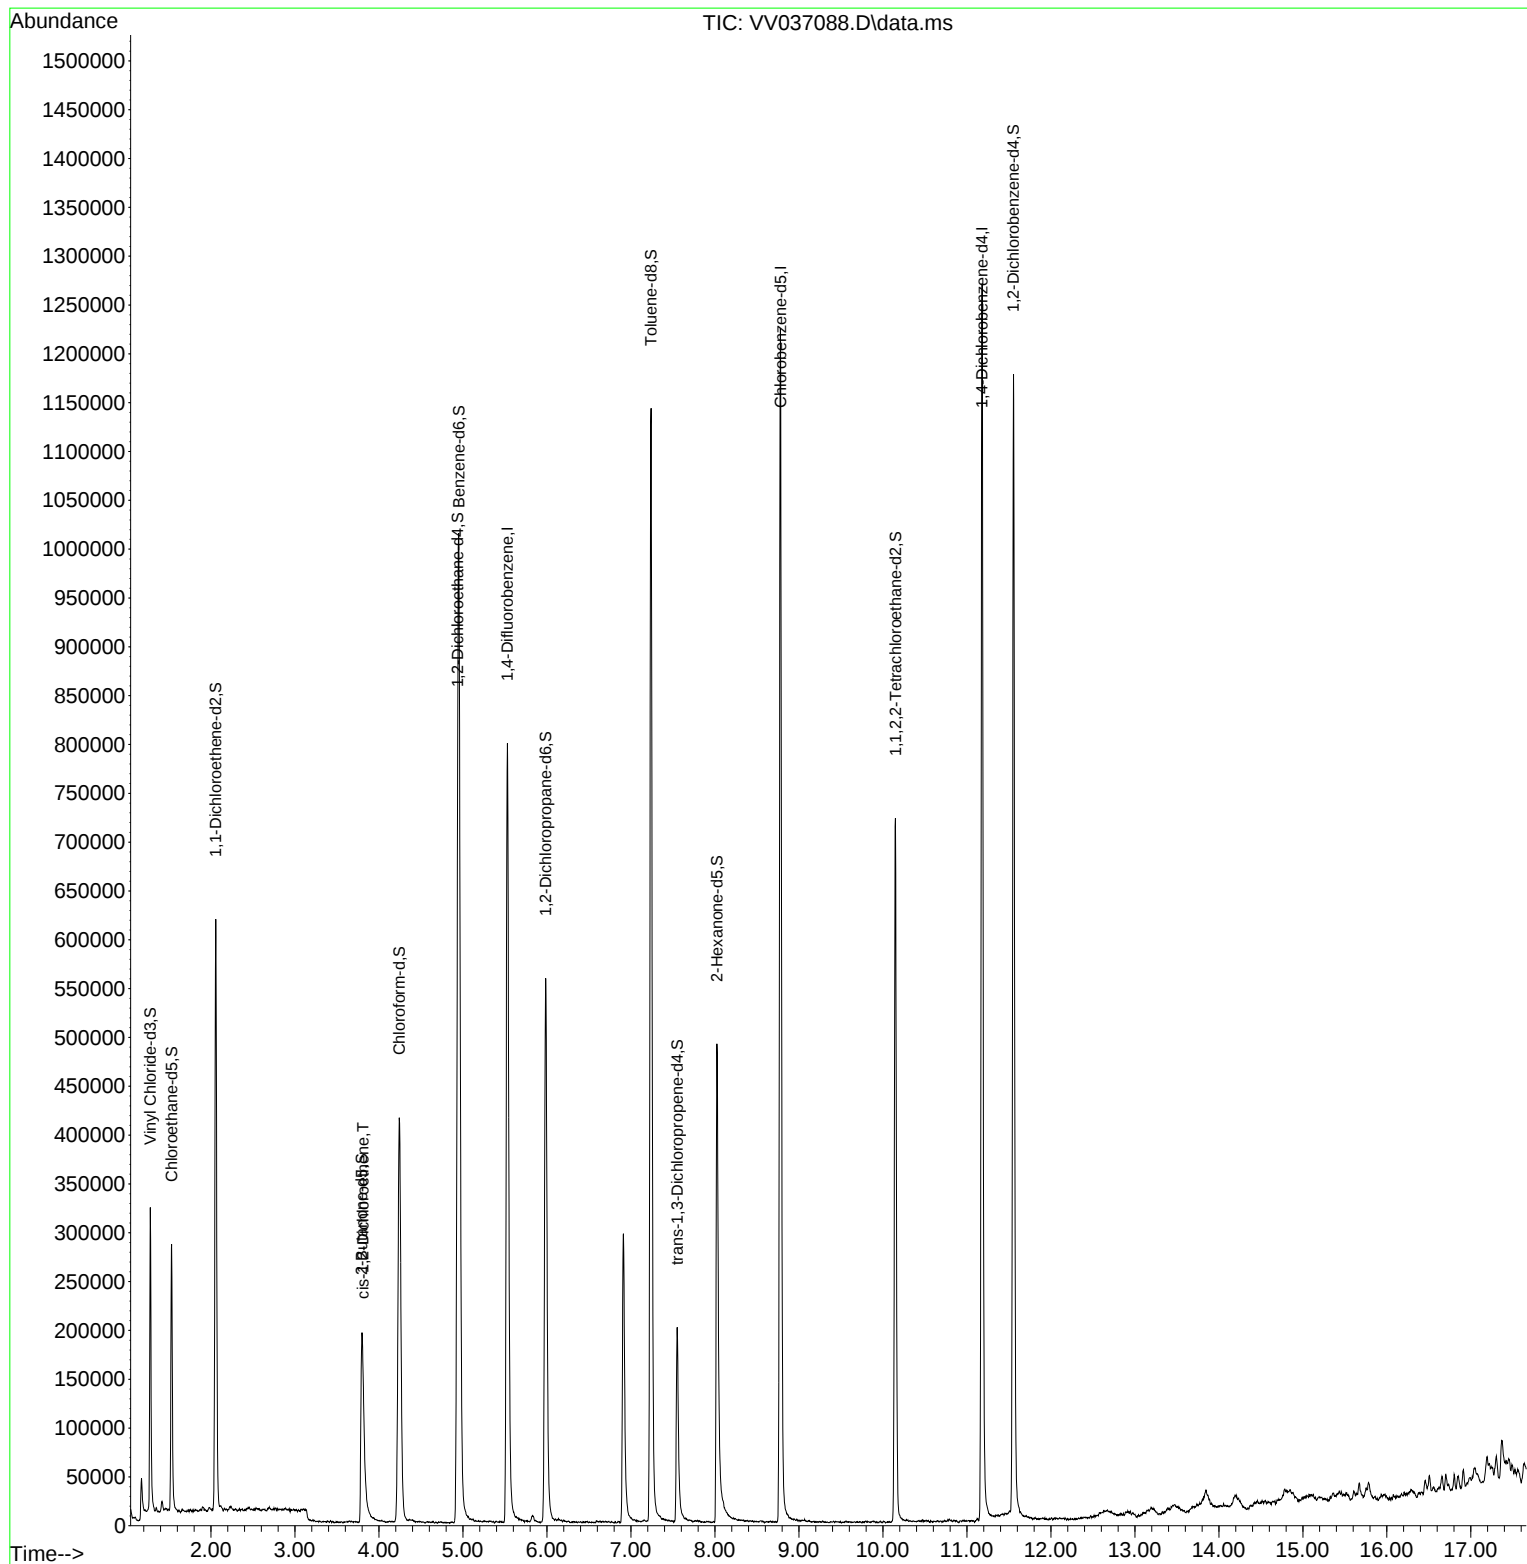

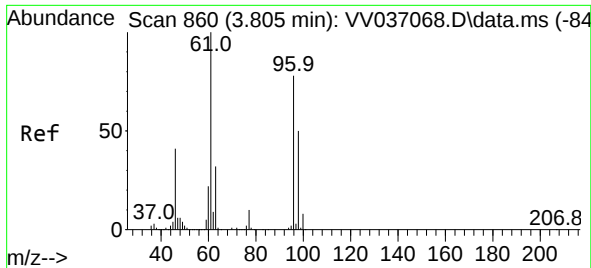

#20
 cis-1,2-Dichloroethene
 Concen: 4.356 ug/L
 RT: 3.809 min Scan# 80
 Delta R.T. 0.003 min
 Lab File: VV037088.D
 Acq: 27 Aug 2024 15:58

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K41

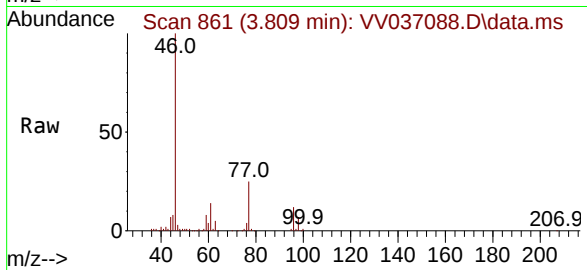

Tgt Ion:	96	Resp:	22128
Ion	Ratio	Lower	Upper
96	100		
61	124.8	89.9	166.9
98	60.5	44.8	83.2

