

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037089.D
 Acq On : 27 Aug 2024 16:20
 Operator : SY/MD
 Sample : P3692-14
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K58

Quant Time: Aug 28 04:22:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 28 04:16:12 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	665075	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	628954	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	314792	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	195523	32.138	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	64.280%		
7) Chloroethane-d5	1.529	69	178239	37.907	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	75.820%		
11) 1,1-Dichloroethene-d2	2.056	65	97317	38.058	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	76.120%		
21) 2-Butanone-d5	3.796	46	254474	108.013	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	108.010%		
24) Chloroform-d	4.243	84	417255	43.821	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.640%		
26) 1,2-Dichloroethane-d4	4.937	65	281236	46.902	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.800%		
32) Benzene-d6	4.953	84	820937	43.214	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.420%		
36) 1,2-Dichloropropane-d6	5.986	67	259039	43.536	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.080%		
41) Toluene-d8	7.240	98	739500	43.133	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.260%		
43) trans-1,3-Dichloroprop...	7.551	79	111726	40.587	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.180%		
47) 2-Hexanone-d5	8.024	63	171150	105.395	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	105.400%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	340874	47.237	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.480%		
66) 1,2-Dichlorobenzene-d4	11.554	152	279630	44.353	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.700%		
Target Compounds						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037089.D
Acq On : 27 Aug 2024 16:20
Operator : SY/MD
Sample : P3692-14
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K58


Quant Time: Aug 28 04:22:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 28 04:16:12 2024
Response via : Initial Calibration

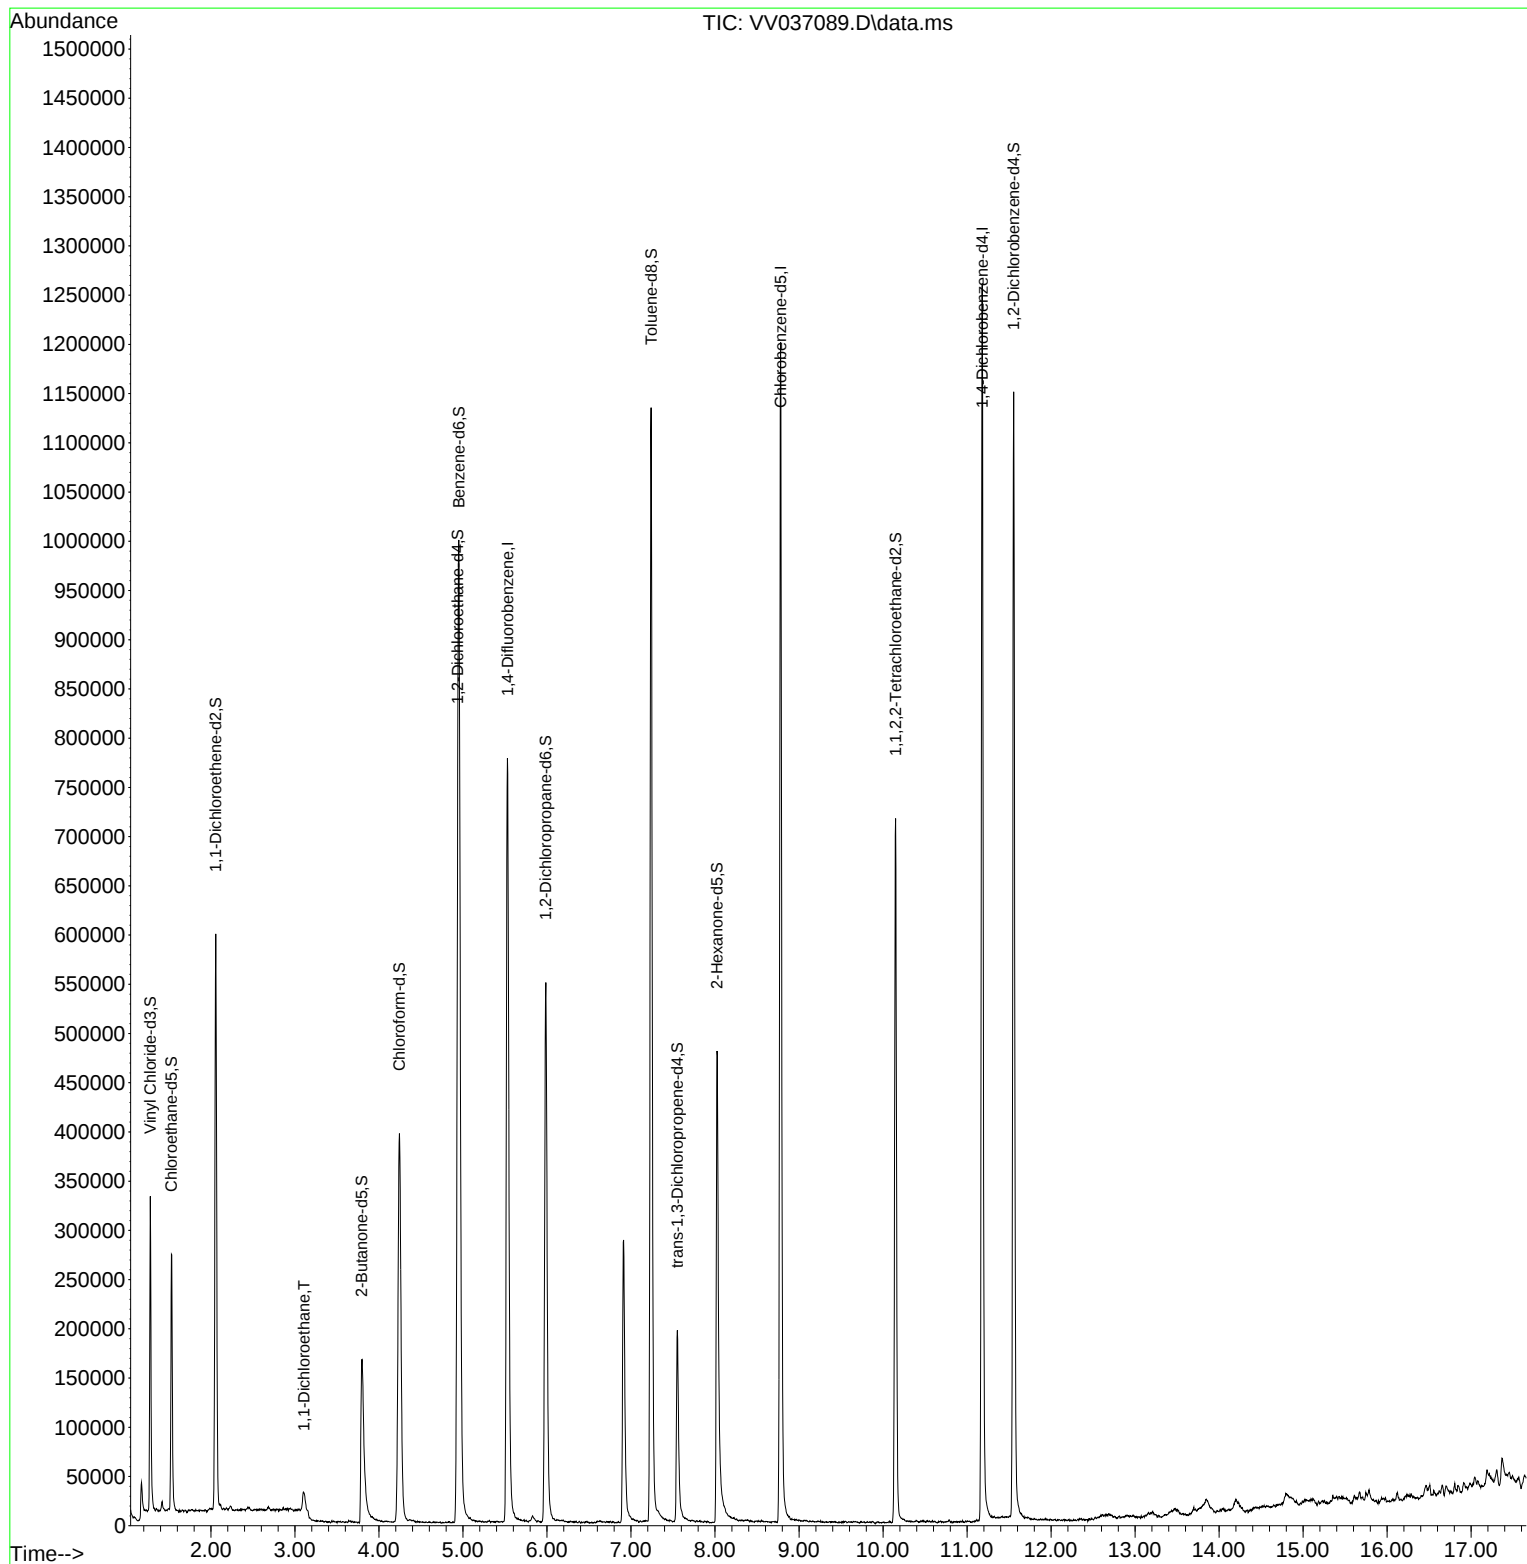

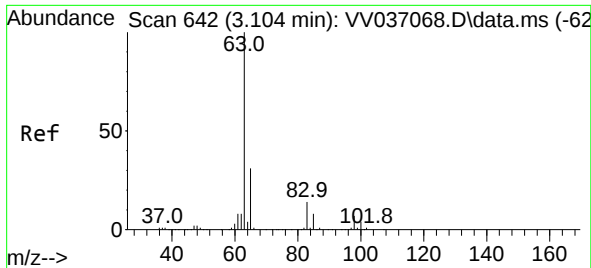

#19
 1,1-Dichloroethane
 Concen: 1.986 ug/L
 RT: 3.108 min Scan# 64
 Delta R.T. 0.003 min
 Lab File: VV037089.D
 Acq: 27 Aug 2024 16:20

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K58

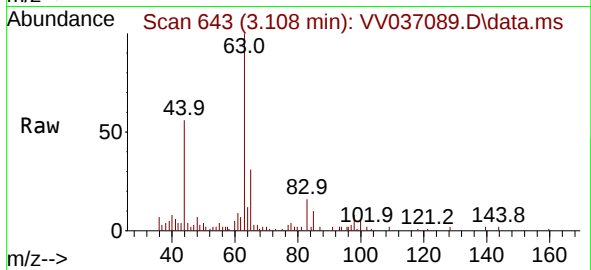

Tgt Ion:	63	Resp:	17769
Ion	Ratio	Lower	Upper
63	100		
65	31.2	22.0	41.0
83	15.5	9.2	17.0

