

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037075.D
 Acq On : 27 Aug 2024 11:14
 Operator : SY/MD
 Sample : P3691-16DL 5X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K67DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	34	40	51	rBV	40888	68083	2.87%	0.376%
2	1.278	67	74	91	rBV2	610491	696593	29.33%	3.851%
3	1.516	142	148	165	rVB	260434	322939	13.60%	1.785%
4	2.053	306	315	335	rVB	561858	813485	34.25%	4.497%
5	3.288	697	699	702	rBV4	1095	734	0.03%	0.004%
6	3.307	702	705	708	rVV5	1308	977	0.04%	0.005%
7	3.513	767	769	772	rBV4	852	494	0.02%	0.003%
8	3.571	785	787	790	rBV4	1118	614	0.03%	0.003%
9	3.616	798	801	803	rBV3	1511	944	0.04%	0.005%
10	3.745	839	841	843	rBV3	721	153	0.01%	0.001%
11	3.799	847	858	885	rBV2	205555	577053	24.30%	3.190%
12	4.240	982	995	1026	rVB	378093	947622	39.90%	5.239%
13	4.523	1082	1083	1085	rBV2	1114	398	0.02%	0.002%
14	4.757	1153	1156	1158	rBV2	1106	670	0.03%	0.004%
15	4.799	1167	1169	1174	rVB6	1083	942	0.04%	0.005%
16	4.825	1174	1177	1179	rBV4	816	535	0.02%	0.003%
17	4.863	1187	1189	1193	rVB3	1250	825	0.03%	0.005%
18	4.886	1193	1196	1199	rBV4	1305	890	0.04%	0.005%
19	4.947	1199	1215	1242	rBV2	954399	2375003	100.00%	13.130%
20	5.394	1352	1354	1360	rVB8	1492	1068	0.04%	0.006%
21	5.529	1383	1396	1428	rBV	671130	1405433	59.18%	7.770%
22	5.982	1524	1537	1563	rBV	522340	1083904	45.64%	5.992%
23	6.288	1630	1632	1638	rVB4	1334	1153	0.05%	0.006%
24	6.314	1638	1640	1643	rVB3	768	440	0.02%	0.002%
25	6.330	1643	1645	1648	rBV4	1283	982	0.04%	0.005%
26	6.365	1653	1656	1657	rBV3	1426	803	0.03%	0.004%
27	6.513	1700	1702	1706	rBV5	1364	846	0.04%	0.005%
28	6.789	1786	1788	1790	rBV3	662	194	0.01%	0.001%
29	6.825	1797	1799	1800	rBV2	1093	501	0.02%	0.003%
30	6.908	1816	1825	1852	rBV	266044	509984	21.47%	2.819%
31	7.236	1916	1927	1952	rBV	1060396	1878209	79.08%	10.384%
32	7.551	2016	2025	2046	rBV	175882	328227	13.82%	1.815%
33	7.793	2097	2100	2103	rBV5	1910	1299	0.05%	0.007%
34	7.924	2139	2141	2145	rBV5	1740	1250	0.05%	0.007%
35	7.966	2152	2154	2156	rBV3	957	573	0.02%	0.003%
36	8.024	2164	2172	2210	rBV	380710	771859	32.50%	4.267%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037075.D
 Acq On : 27 Aug 2024 11:14
 Operator : SY/MD
 Sample : P3691-16DL 5X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K67DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.780	2396	2407	2434	rBV	1065968	1746273	73.53%	9.654%
38	9.281	2561	2563	2565	rBV2	513	203	0.01%	0.001%
39	9.342	2580	2582	2583	rBV2	1231	626	0.03%	0.003%
40	9.362	2586	2588	2590	rVV4	1036	548	0.02%	0.003%
41	9.709	2694	2696	2698	rBV3	1471	891	0.04%	0.005%
42	9.738	2703	2705	2711	rVB6	1406	1077	0.05%	0.006%
43	9.780	2715	2718	2719	rBV2	742	302	0.01%	0.002%
44	9.792	2719	2722	2723	rBV3	908	447	0.02%	0.002%
45	9.812	2726	2728	2729	rBV3	834	386	0.02%	0.002%
46	9.863	2738	2744	2747	rBV5	2160	2089	0.09%	0.012%
47	9.918	2758	2761	2766	rBV6	1380	1303	0.05%	0.007%
48	9.937	2766	2767	2769	rVB2	1061	267	0.01%	0.001%
49	9.956	2769	2773	2776	rBV2	1499	1069	0.05%	0.006%
50	10.005	2784	2788	2791	rVB6	1287	1085	0.05%	0.006%
51	10.021	2791	2793	2794	rBV2	536	223	0.01%	0.001%
52	10.043	2797	2800	2801	rBV2	683	287	0.01%	0.002%
53	10.059	2801	2805	2808	rBV4	1293	994	0.04%	0.005%
54	10.149	2821	2833	2852	rBV	650567	1040626	43.82%	5.753%
55	10.442	2920	2924	2926	rBV4	947	790	0.03%	0.004%
56	10.481	2934	2936	2937	rBV2	901	289	0.01%	0.002%
57	10.609	2974	2976	2978	rBV3	910	427	0.02%	0.002%
58	10.622	2978	2980	2983	rVV3	730	470	0.02%	0.003%
59	10.670	2992	2995	2998	rVB3	855	512	0.02%	0.003%
60	10.693	3000	3002	3004	rVB2	775	256	0.01%	0.001%
61	10.770	3023	3026	3027	rBV2	1364	746	0.03%	0.004%
62	10.834	3044	3046	3048	rBV3	1305	626	0.03%	0.003%
63	10.924	3073	3074	3076	rBV2	877	442	0.02%	0.002%
64	10.963	3083	3086	3091	rVB4	1511	1228	0.05%	0.007%
65	10.989	3091	3094	3095	rVB2	729	285	0.01%	0.002%
66	10.998	3095	3097	3098	rBV2	474	187	0.01%	0.001%
67	11.034	3106	3108	3109	rVB	683	191	0.01%	0.001%
68	11.050	3109	3113	3118	rBV8	1163	1140	0.05%	0.006%
69	11.072	3118	3120	3122	rBV3	586	275	0.01%	0.002%
70	11.124	3131	3136	3138	rBV6	1925	1805	0.08%	0.010%
71	11.182	3143	3154	3177	rVV	1077169	1716010	72.25%	9.487%
72	11.471	3242	3244	3246	rVB2	1133	470	0.02%	0.003%
73	11.554	3258	3270	3294	rBV	1102774	1737442	73.16%	9.606%
74	11.950	3391	3393	3400	rVB6	2099	1628	0.07%	0.009%
75	12.140	3450	3452	3456	rBV4	894	713	0.03%	0.004%
76	12.185	3462	3466	3469	rVB5	1536	1261	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037075.D
 Acq On : 27 Aug 2024 11:14
 Operator : SY/MD
 Sample : P3691-16DL 5X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K67DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	12.204	3469	3472	3473	rBV3	1010	607	0.03%	0.003%
78	12.217	3473	3476	3478	rVB3	1261	718	0.03%	0.004%
79	12.236	3478	3482	3483	rBV3	1043	662	0.03%	0.004%
80	12.423	3537	3540	3543	rBV5	1135	725	0.03%	0.004%
81	12.493	3560	3562	3565	rBV2	784	403	0.02%	0.002%
82	12.657	3608	3613	3616	rBV6	1429	1255	0.05%	0.007%
83	12.709	3625	3629	3632	rBV5	1133	1083	0.05%	0.006%
84	12.821	3662	3664	3668	rVB4	1560	828	0.03%	0.005%
85	12.847	3668	3672	3674	rBV5	1009	871	0.04%	0.005%
86	12.892	3684	3686	3687	rBV	1179	436	0.02%	0.002%
87	13.017	3722	3725	3726	rBV2	1085	427	0.02%	0.002%
88	13.027	3726	3728	3730	rBV3	1050	453	0.02%	0.003%
89	13.069	3737	3741	3745	rVB5	1155	885	0.04%	0.005%
90	13.088	3745	3747	3750	rBV3	1627	698	0.03%	0.004%
91	13.210	3778	3785	3787	rBV6	4076	3997	0.17%	0.022%
92	13.284	3806	3808	3809	rBV3	904	317	0.01%	0.002%
93	13.304	3812	3814	3820	rBV5	1700	1737	0.07%	0.010%
94	13.455	3853	3861	3863	rBV9	2834	3315	0.14%	0.018%
95	13.593	3901	3904	3908	rBV5	1601	1422	0.06%	0.008%
96	13.635	3915	3917	3920	rBV5	897	537	0.02%	0.003%
97	13.863	3986	3988	3989	rBV2	788	254	0.01%	0.001%
98	14.014	4030	4035	4039	rBV8	1843	1963	0.08%	0.011%
99	14.159	4075	4080	4086	rBV8	1523	2436	0.10%	0.013%
100	14.226	4099	4101	4103	rBV3	1064	389	0.02%	0.002%




Sum of corrected areas: 18087986

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037075.D
Acq On : 27 Aug 2024 11:14
Operator : SY/MD
Sample : P3691-16DL 5X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K67DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

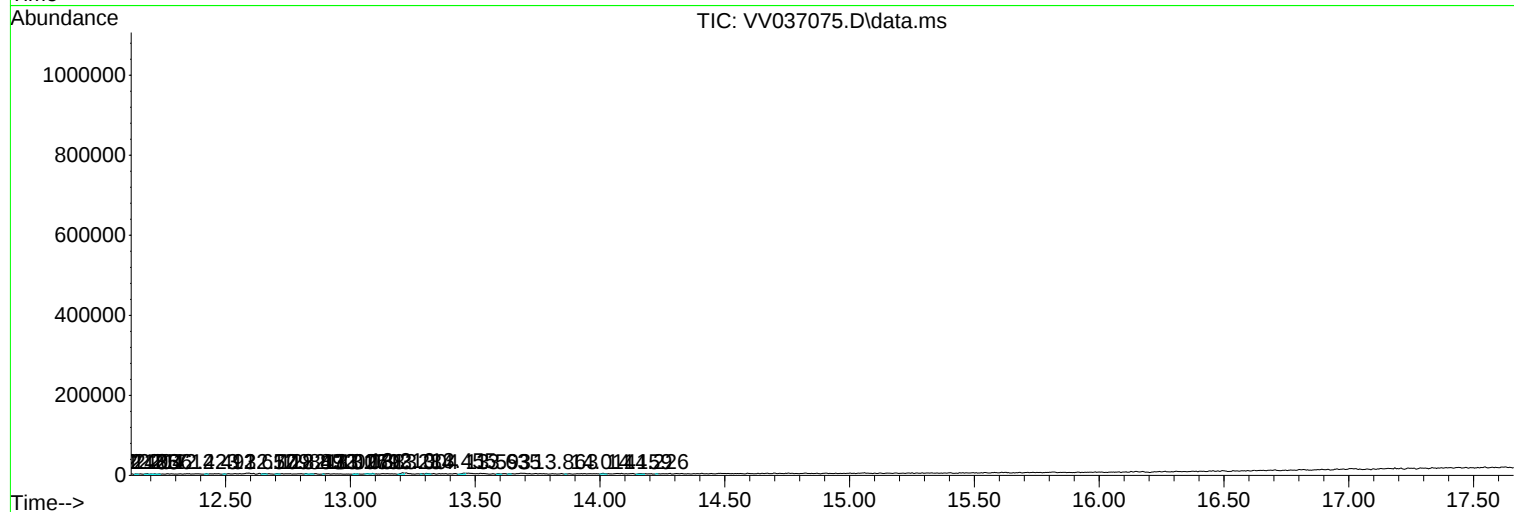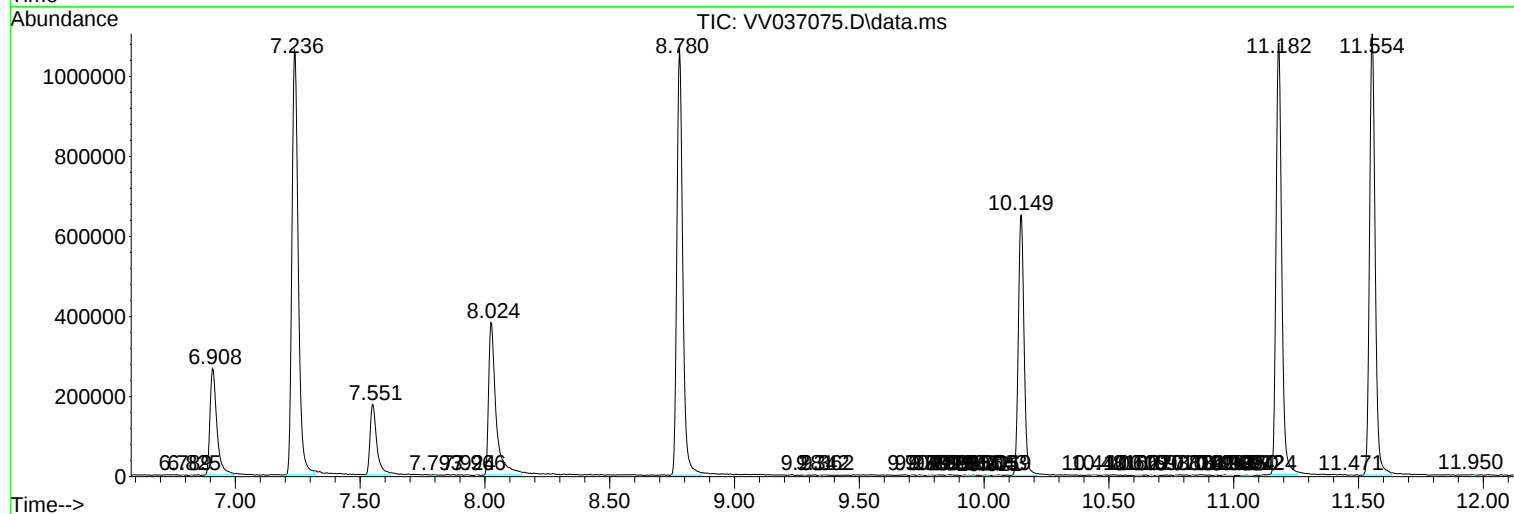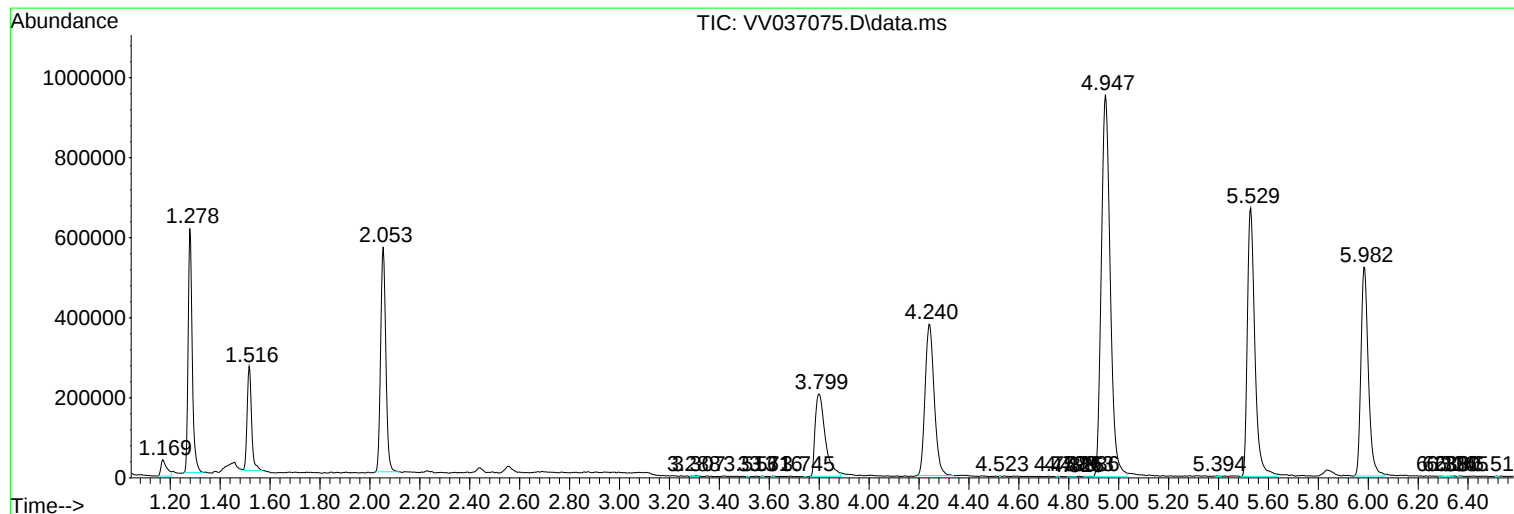

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037075.D
Acq On : 27 Aug 2024 11:14
Operator : SY/MD
Sample : P3691-16DL 5X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K67DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037075.D
Acq On : 27 Aug 2024 11:14
Operator : SY/MD
Sample : P3691-16DL 5X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K67DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
