

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037086.D
 Acq On : 27 Aug 2024 15:15
 Operator : SY/MD
 Sample : P3692-09
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	52	rBV	41743	65870	2.65%	0.347%
2	1.278	67	74	92	rVB	301985	323179	12.98%	1.702%
3	1.529	145	152	168	rVB	267020	322989	12.97%	1.701%
4	2.056	307	316	330	rBV	591030	840836	33.78%	4.428%
5	3.262	689	691	694	rVB3	1540	873	0.04%	0.005%
6	3.314	704	707	709	rBV4	827	469	0.02%	0.002%
7	3.388	728	730	733	rBV4	1026	649	0.03%	0.003%
8	3.404	733	735	738	rVB4	847	486	0.02%	0.003%
9	3.510	765	768	772	rVV6	843	617	0.02%	0.003%
10	3.529	772	774	778	rVB4	902	541	0.02%	0.003%
11	3.561	782	784	786	rBV3	824	544	0.02%	0.003%
12	3.613	795	800	801	rBV5	1947	1750	0.07%	0.009%
13	3.632	801	806	810	rVV6	2817	3727	0.15%	0.020%
14	3.722	832	834	838	rVB4	1109	786	0.03%	0.004%
15	3.796	845	857	893	rBV	162624	456904	18.35%	2.406%
16	3.979	912	914	920	rBV6	1257	1150	0.05%	0.006%
17	4.063	938	940	942	rBV2	1037	483	0.02%	0.003%
18	4.169	970	973	975	rBV3	1059	710	0.03%	0.004%
19	4.185	975	978	980	rVV3	1716	1250	0.05%	0.007%
20	4.243	980	996	1023	rVV	392611	983634	39.51%	5.180%
21	4.368	1033	1035	1038	rVB4	1428	774	0.03%	0.004%
22	4.484	1067	1071	1074	rBV5	1072	785	0.03%	0.004%
23	4.548	1088	1091	1092	rBV2	797	467	0.02%	0.002%
24	4.568	1095	1097	1103	rVB7	1171	903	0.04%	0.005%
25	4.600	1103	1107	1109	rBV3	647	603	0.02%	0.003%
26	4.609	1109	1110	1114	rVV4	814	571	0.02%	0.003%
27	4.735	1145	1149	1152	rBV5	982	1086	0.04%	0.006%
28	4.812	1168	1173	1175	rBV4	1501	1309	0.05%	0.007%
29	4.896	1194	1199	1200	rBV4	941	740	0.03%	0.004%
30	4.950	1200	1216	1253	rBV2	988501	2489436	100.00%	13.111%
31	5.156	1278	1280	1282	rBV2	1083	625	0.03%	0.003%
32	5.207	1291	1296	1298	rBV6	1018	756	0.03%	0.004%
33	5.230	1300	1303	1307	rVB6	1620	835	0.03%	0.004%
34	5.252	1307	1310	1314	rBV4	1963	1424	0.06%	0.007%
35	5.326	1331	1333	1337	rVB5	1367	696	0.03%	0.004%
36	5.445	1367	1370	1374	rBV5	1680	1276	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037086.D
 Acq On : 27 Aug 2024 15:15
 Operator : SY/MD
 Sample : P3692-09
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	5.484	1380	1382	1384	rBV3	1157	613	0.02%	0.003%
38	5.529	1384	1396	1419	rBV	795998	1616548	64.94%	8.514%
39	5.696	1446	1448	1452	rVB5	1941	1170	0.05%	0.006%
40	5.828	1481	1489	1494	rBV10	4374	6951	0.28%	0.037%
41	5.934	1519	1522	1525	rBV4	910	657	0.03%	0.003%
42	5.986	1525	1538	1564	rBV	547677	1120816	45.02%	5.903%
43	6.236	1614	1616	1618	rBV3	845	491	0.02%	0.003%
44	6.285	1627	1631	1633	rBV5	1443	1203	0.05%	0.006%
45	6.429	1673	1676	1677	rBV3	1117	523	0.02%	0.003%
46	6.529	1705	1707	1709	rBV3	1222	526	0.02%	0.003%
47	6.577	1719	1722	1724	rVV4	1365	702	0.03%	0.004%
48	6.603	1727	1730	1732	rBV4	758	602	0.02%	0.003%
49	6.674	1750	1752	1754	rVB2	1147	495	0.02%	0.003%
50	6.725	1764	1768	1771	rBV5	994	823	0.03%	0.004%
51	6.760	1776	1779	1782	rBV5	1552	1173	0.05%	0.006%
52	6.812	1792	1795	1798	rVB4	1481	920	0.04%	0.005%
53	6.828	1798	1800	1801	rBV2	1077	463	0.02%	0.002%
54	6.867	1811	1812	1815	rBV3	977	490	0.02%	0.003%
55	6.912	1815	1826	1847	rBV	282327	540797	21.72%	2.848%
56	7.149	1898	1900	1904	rVB5	888	579	0.02%	0.003%
57	7.240	1915	1928	1956	rBV	1096340	1957303	78.62%	10.308%
58	7.551	2015	2025	2046	rBV	186657	347842	13.97%	1.832%
59	7.741	2080	2084	2086	rBV5	1749	1160	0.05%	0.006%
60	7.805	2100	2104	2108	rBV7	1112	979	0.04%	0.005%
61	7.831	2108	2112	2116	rBV5	1570	1190	0.05%	0.006%
62	7.860	2117	2121	2124	rBV5	1131	1007	0.04%	0.005%
63	7.899	2131	2133	2135	rBV2	1521	631	0.03%	0.003%
64	7.912	2135	2137	2138	rVB2	1247	475	0.02%	0.003%
65	7.921	2138	2140	2145	rVB5	1140	964	0.04%	0.005%
66	8.024	2163	2172	2208	rBV	458603	894400	35.93%	4.710%
67	8.313	2260	2262	2265	rBV3	1176	650	0.03%	0.003%
68	8.410	2290	2292	2293	rBV2	1079	496	0.02%	0.003%
69	8.429	2296	2298	2301	rBV4	1526	859	0.03%	0.005%
70	8.477	2311	2313	2315	rBV4	1168	607	0.02%	0.003%
71	8.535	2329	2331	2333	rBV3	2062	1221	0.05%	0.006%
72	8.580	2342	2345	2348	rBV5	1252	741	0.03%	0.004%
73	8.600	2348	2351	2353	rBV4	1140	666	0.03%	0.004%
74	8.780	2393	2407	2433	rBV	1233922	1995736	80.17%	10.511%
75	9.079	2496	2500	2505	rVB7	1589	1275	0.05%	0.007%
76	9.104	2505	2508	2509	rBV3	1473	854	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037086.D
 Acq On : 27 Aug 2024 15:15
 Operator : SY/MD
 Sample : P3692-09
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	9.191	2533	2535	2539	rBV4	922	552	0.02%	0.003%
78	9.256	2550	2555	2558	rBV5	1367	1708	0.07%	0.009%
79	9.346	2579	2583	2587	rBV6	1532	1459	0.06%	0.008%
80	9.400	2597	2600	2602	rVV3	994	593	0.02%	0.003%
81	9.416	2602	2605	2609	rVB5	1338	913	0.04%	0.005%
82	9.484	2624	2626	2628	rVV3	1642	938	0.04%	0.005%
83	9.497	2628	2630	2636	rVB7	2412	2057	0.08%	0.011%
84	9.522	2636	2638	2642	rBV5	731	502	0.02%	0.003%
85	9.664	2680	2682	2684	rBV3	1108	589	0.02%	0.003%
86	9.709	2694	2696	2702	rVB7	1277	690	0.03%	0.004%
87	9.821	2729	2731	2733	rBV3	715	456	0.02%	0.002%
88	9.924	2761	2763	2769	rVB6	1261	866	0.03%	0.005%
89	9.969	2773	2777	2782	rVB8	1757	1676	0.07%	0.009%
90	10.001	2785	2787	2789	rBV3	997	535	0.02%	0.003%
91	10.014	2789	2791	2797	rVB5	1397	1088	0.04%	0.006%
92	10.043	2798	2800	2804	rBV4	893	510	0.02%	0.003%
93	10.082	2808	2812	2815	rVB5	1006	564	0.02%	0.003%
94	10.149	2819	2833	2851	rBV	703654	1115897	44.83%	5.877%
95	10.352	2892	2896	2897	rBV2	1188	900	0.04%	0.005%
96	10.583	2965	2968	2972	rBV5	2576	1850	0.07%	0.010%
97	10.654	2986	2990	2991	rBV5	1994	1321	0.05%	0.007%
98	10.818	3038	3041	3044	rVB5	1613	1038	0.04%	0.005%
99	11.178	3143	3153	3178	rBV	1272267	2032449	81.64%	10.704%
100	11.554	3260	3270	3294	rVB	1131347	1803051	72.43%	9.496%


Sum of corrected areas: 18987533

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037086.D
Acq On : 27 Aug 2024 15:15
Operator : SY/MD
Sample : P3692-09
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

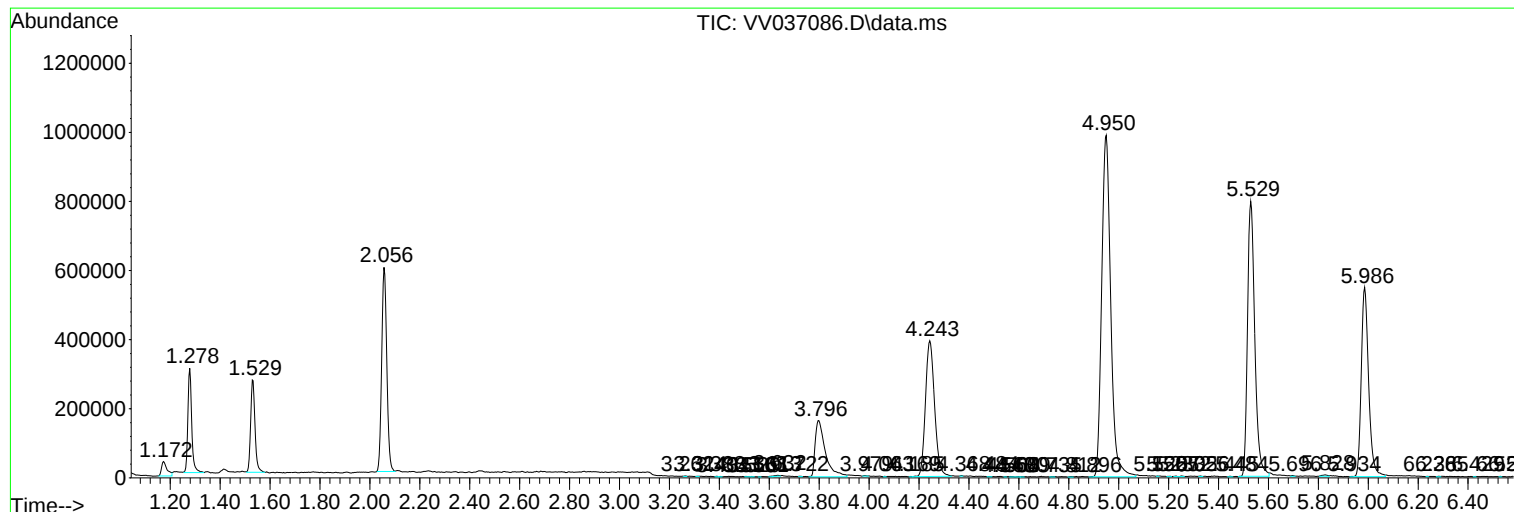

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037086.D
Acq On : 27 Aug 2024 15:15
Operator : SY/MD
Sample : P3692-09
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037086.D
Acq On : 27 Aug 2024 15:15
Operator : SY/MD
Sample : P3692-09
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc