

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037089.D
 Acq On : 27 Aug 2024 16:20
 Operator : SY/MD
 Sample : P3692-14
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	51	rBV	36957	56721	2.28%	0.298%
2	1.278	67	74	88	rBV	318608	330662	13.27%	1.738%
3	1.529	145	152	169	rVB	260172	321902	12.92%	1.692%
4	2.056	307	316	329	rBV	581727	823248	33.04%	4.328%
5	3.259	687	690	692	rBV3	1448	723	0.03%	0.004%
6	3.407	734	736	740	rVB5	1365	906	0.04%	0.005%
7	3.439	743	746	750	rVV5	1947	1404	0.06%	0.007%
8	3.462	750	753	758	rVB7	1278	1021	0.04%	0.005%
9	3.510	765	768	771	rBV5	1515	1321	0.05%	0.007%
10	3.542	775	778	781	rVV4	1371	918	0.04%	0.005%
11	3.568	783	786	793	rVB7	1141	1238	0.05%	0.007%
12	3.638	806	808	811	rBV3	1554	888	0.04%	0.005%
13	3.687	819	823	828	rVB5	1460	1290	0.05%	0.007%
14	3.799	848	858	891	rBV	166178	456865	18.33%	2.402%
15	4.243	979	996	1026	rVV	394479	993462	39.87%	5.223%
16	4.445	1057	1059	1062	rBV4	980	639	0.03%	0.003%
17	4.561	1092	1095	1100	rVB7	751	674	0.03%	0.004%
18	4.757	1151	1156	1157	rBV4	1122	785	0.03%	0.004%
19	4.796	1164	1168	1172	rVB6	847	606	0.02%	0.003%
20	4.828	1172	1178	1179	rVV5	1048	813	0.03%	0.004%
21	4.838	1179	1181	1184	rVB4	1255	798	0.03%	0.004%
22	4.950	1199	1216	1254	rBV2	998135	2491985	100.00%	13.102%
23	5.233	1302	1304	1309	rVB6	1178	735	0.03%	0.004%
24	5.529	1383	1396	1419	rBV	775190	1580213	63.41%	8.308%
25	5.793	1473	1478	1481	rBV5	1656	1948	0.08%	0.010%
26	5.828	1484	1489	1495	rVV10	3853	5450	0.22%	0.029%
27	5.892	1505	1509	1515	rBV8	1581	1687	0.07%	0.009%
28	5.986	1525	1538	1565	rBV	546958	1113488	44.68%	5.854%
29	6.281	1628	1630	1633	rVV4	1097	594	0.02%	0.003%
30	6.346	1648	1650	1657	rVB6	1728	1083	0.04%	0.006%
31	6.384	1657	1662	1667	rVB8	1928	2093	0.08%	0.011%
32	6.410	1667	1670	1672	rBV4	1357	673	0.03%	0.004%
33	6.432	1672	1677	1680	rBV5	1000	951	0.04%	0.005%
34	6.477	1687	1691	1694	rVB4	1214	878	0.04%	0.005%
35	6.603	1723	1730	1734	rBV10	1941	2610	0.10%	0.014%
36	6.709	1760	1763	1765	rBV3	1236	750	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037089.D
 Acq On : 27 Aug 2024 16:20
 Operator : SY/MD
 Sample : P3692-14
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.728	1765	1769	1772	rVB5	803	676	0.03%	0.004%
38	6.754	1776	1777	1782	rVB3	1673	939	0.04%	0.005%
39	6.793	1786	1789	1792	rVB4	1507	1043	0.04%	0.005%
40	6.850	1802	1807	1809	rBV7	1264	1085	0.04%	0.006%
41	6.912	1812	1826	1856	rBV	287249	561362	22.53%	2.951%
42	7.108	1883	1887	1888	rBV3	1620	1144	0.05%	0.006%
43	7.240	1916	1928	1951	rBV	1131183	1963065	78.78%	10.321%
44	7.461	1995	1997	2002	rBV5	1383	1093	0.04%	0.006%
45	7.551	2014	2025	2047	rBV	194265	354671	14.23%	1.865%
46	7.780	2094	2096	2099	rBV3	948	677	0.03%	0.004%
47	7.841	2112	2115	2118	rBV5	857	628	0.03%	0.003%
48	7.873	2122	2125	2126	rBV3	1099	609	0.02%	0.003%
49	7.908	2133	2136	2138	rBV4	1493	850	0.03%	0.004%
50	8.024	2161	2172	2213	rBV	478976	951200	38.17%	5.001%
51	8.420	2292	2295	2298	rBV5	1574	1113	0.04%	0.006%
52	8.439	2298	2301	2304	rVB4	1092	653	0.03%	0.003%
53	8.551	2333	2336	2340	rBV6	1916	1482	0.06%	0.008%
54	8.680	2372	2376	2377	rBV4	1065	876	0.04%	0.005%
55	8.780	2395	2407	2433	rBV	1198375	1963139	78.78%	10.321%
56	9.127	2512	2515	2517	rBV3	1094	624	0.03%	0.003%
57	9.365	2585	2589	2591	rBV3	775	590	0.02%	0.003%
58	9.471	2619	2622	2624	rBV3	1147	637	0.03%	0.003%
59	9.510	2632	2634	2635	rBV2	1422	606	0.02%	0.003%
60	9.532	2638	2641	2643	rVV3	1772	1087	0.04%	0.006%
61	9.551	2643	2647	2653	rVB5	1486	1756	0.07%	0.009%
62	9.593	2655	2660	2663	rBV7	1012	961	0.04%	0.005%
63	9.645	2674	2676	2680	rBV5	1247	903	0.04%	0.005%
64	9.696	2690	2692	2697	rVB5	1024	600	0.02%	0.003%
65	9.738	2700	2705	2706	rBV4	1768	1184	0.05%	0.006%
66	9.812	2724	2728	2733	rVB5	1122	763	0.03%	0.004%
67	9.873	2744	2747	2748	rBV3	1214	710	0.03%	0.004%
68	9.921	2757	2762	2763	rBV5	1637	1303	0.05%	0.007%
69	9.937	2763	2767	2769	rVV4	1623	1545	0.06%	0.008%
70	9.992	2781	2784	2787	rBV3	993	781	0.03%	0.004%
71	10.075	2805	2810	2812	rBV6	1644	1175	0.05%	0.006%
72	10.149	2820	2833	2859	rBV	714897	1141414	45.80%	6.001%
73	10.394	2907	2909	2913	rBV5	1350	948	0.04%	0.005%
74	10.445	2922	2925	2928	rBV5	1412	736	0.03%	0.004%
75	10.464	2928	2931	2935	rBV6	1552	1127	0.05%	0.006%
76	10.484	2935	2937	2941	rVB6	1303	619	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037089.D
 Acq On : 27 Aug 2024 16:20
 Operator : SY/MD
 Sample : P3692-14
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	10.526	2947	2950	2954	rBV6	1620	1352	0.05%	0.007%
78	10.554	2957	2959	2964	rVB5	1449	991	0.04%	0.005%
79	10.587	2967	2969	2971	rVB3	1587	666	0.03%	0.004%
80	10.657	2988	2991	2993	rBV2	1408	779	0.03%	0.004%
81	10.667	2993	2994	2997	rVV2	904	582	0.02%	0.003%
82	10.686	2998	3000	3003	rVB3	1633	912	0.04%	0.005%
83	10.789	3027	3032	3036	rVB6	2573	2593	0.10%	0.014%
84	10.841	3044	3048	3050	rBV5	1589	1016	0.04%	0.005%
85	10.899	3062	3066	3070	rBV7	1024	934	0.04%	0.005%
86	10.924	3070	3074	3079	rVV9	1267	1375	0.06%	0.007%
87	10.982	3089	3092	3096	rBV4	1486	1110	0.04%	0.006%
88	11.005	3096	3099	3101	rBV3	1327	786	0.03%	0.004%
89	11.069	3116	3119	3121	rBV4	1232	742	0.03%	0.004%
90	11.111	3127	3132	3135	rBV6	2030	1660	0.07%	0.009%
91	11.130	3136	3138	3141	rBV4	1511	782	0.03%	0.004%
92	11.181	3141	3154	3180	rBV	1257183	2002924	80.37%	10.531%
93	11.554	3259	3270	3295	rBV	1141954	1823532	73.18%	9.587%
94	12.146	3451	3454	3455	rBV3	1235	770	0.03%	0.004%
95	12.243	3482	3484	3488	rBV4	1089	794	0.03%	0.004%
96	12.339	3511	3514	3516	rBV4	1916	1168	0.05%	0.006%
97	12.442	3544	3546	3548	rBV3	1746	799	0.03%	0.004%
98	12.458	3548	3551	3554	rVV5	2341	1729	0.07%	0.009%
99	12.484	3555	3559	3566	rVV10	1971	2308	0.09%	0.012%
100	13.072	3740	3742	3745	rBV5	2521	1429	0.06%	0.008%


Sum of corrected areas: 19020129

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037089.D
Acq On : 27 Aug 2024 16:20
Operator : SY/MD
Sample : P3692-14
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

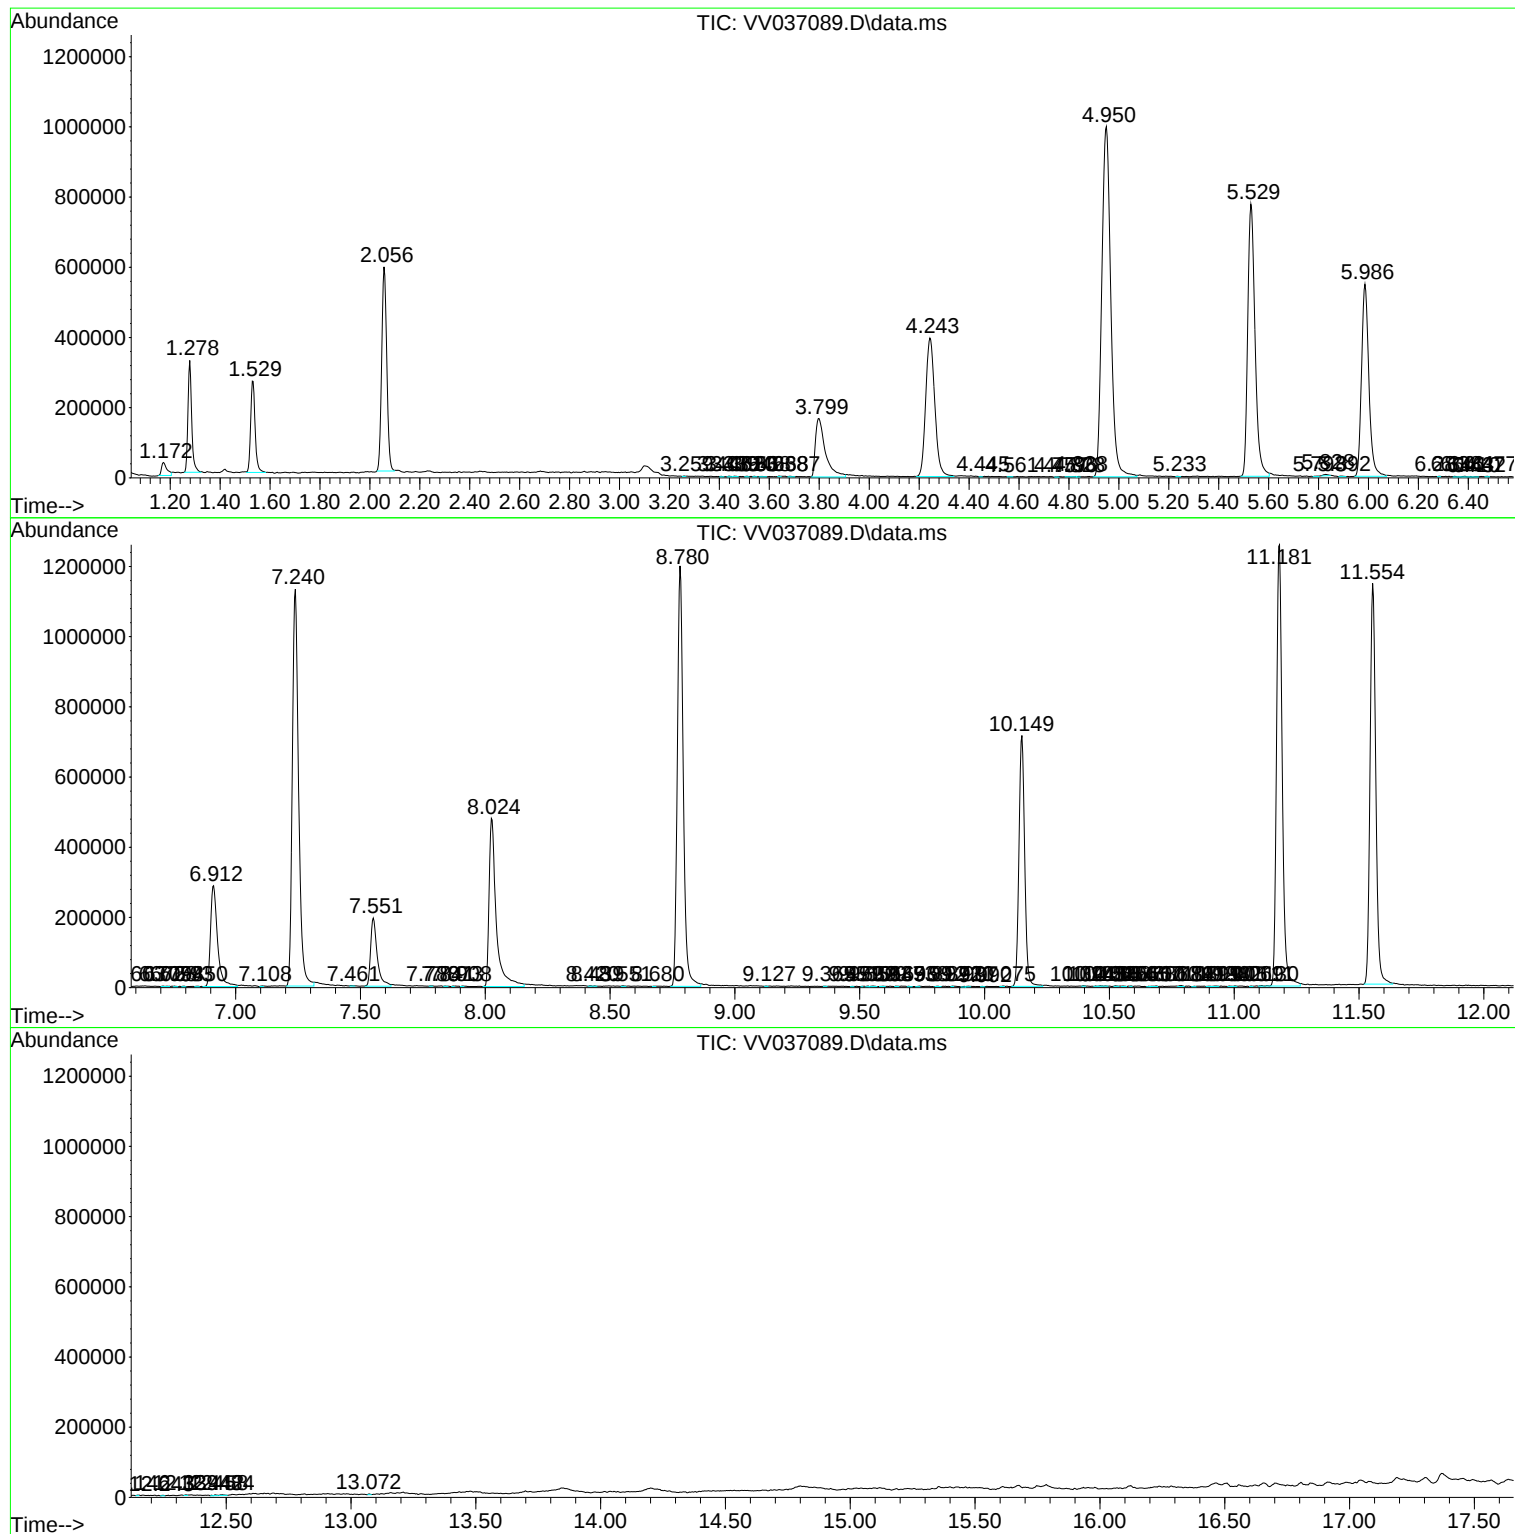

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037089.D
Acq On : 27 Aug 2024 16:20
Operator : SY/MD
Sample : P3692-14
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037089.D
Acq On : 27 Aug 2024 16:20
Operator : SY/MD
Sample : P3692-14
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc