

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037090.D
 Acq On : 27 Aug 2024 16:43
 Operator : SY/MD
 Sample : P3692-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	34	41	51	rBV	36400	57187	0.75%	0.187%
2	1.281	67	75	105	rBV	7063957	7663239	100.00%	24.999%
3	1.529	145	152	169	rBV	255287	309606	4.04%	1.010%
4	2.056	307	316	332	rVB	579358	820940	10.71%	2.678%
5	3.355	717	720	726	rVB6	1874	1643	0.02%	0.005%
6	3.638	804	808	811	rVB4	1270	1091	0.01%	0.004%
7	3.658	811	814	816	rBV3	1377	1008	0.01%	0.003%
8	3.725	833	835	838	rVB3	1562	899	0.01%	0.003%
9	3.802	843	859	896	rBV2	1991964	4807026	62.73%	15.682%
10	4.243	981	996	1025	rVB	391094	979143	12.78%	3.194%
11	4.529	1083	1085	1089	rVB4	1413	952	0.01%	0.003%
12	4.712	1140	1142	1145	rBV3	1274	712	0.01%	0.002%
13	4.738	1149	1150	1155	rVB4	1481	839	0.01%	0.003%
14	4.776	1155	1162	1165	rBV5	1231	1379	0.02%	0.004%
15	4.947	1198	1215	1255	rBV2	981800	2457796	32.07%	8.018%
16	5.191	1289	1291	1294	rBV4	999	733	0.01%	0.002%
17	5.313	1326	1329	1332	rBV4	1876	1077	0.01%	0.004%
18	5.529	1383	1396	1433	rBV	779769	1597895	20.85%	5.213%
19	5.754	1463	1466	1468	rBV4	991	723	0.01%	0.002%
20	5.821	1481	1487	1490	rBV7	5034	6024	0.08%	0.020%
21	5.928	1517	1520	1523	rBV4	1711	1410	0.02%	0.005%
22	5.985	1523	1538	1563	rBV	543388	1117114	14.58%	3.644%
23	6.297	1630	1635	1638	rVB5	1041	981	0.01%	0.003%
24	6.368	1652	1657	1660	rBV7	1663	1724	0.02%	0.006%
25	6.448	1679	1682	1686	rVB5	1533	841	0.01%	0.003%
26	6.551	1712	1714	1715	rBV2	1642	701	0.01%	0.002%
27	6.583	1722	1724	1726	rBV4	1144	683	0.01%	0.002%
28	6.683	1753	1755	1759	rVB6	975	672	0.01%	0.002%
29	6.767	1778	1781	1784	rBV3	1670	1078	0.01%	0.004%
30	6.844	1802	1805	1810	rVB6	1142	1042	0.01%	0.003%
31	6.911	1813	1826	1859	rBV	289047	564228	7.36%	1.841%
32	7.130	1890	1894	1900	rVB5	1559	1379	0.02%	0.004%
33	7.159	1901	1903	1907	rVB3	1499	791	0.01%	0.003%
34	7.239	1915	1928	1952	rBV	1110932	1958027	25.55%	6.388%
35	7.551	2015	2025	2046	rBV	189462	348705	4.55%	1.138%
36	7.870	2120	2124	2129	rVB7	1437	1602	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037090.D
 Acq On : 27 Aug 2024 16:43
 Operator : SY/MD
 Sample : P3692-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	7.899	2131	2133	2137	rVV4	1348	915	0.01%	0.003%
38	7.918	2137	2139	2143	rVB4	1158	696	0.01%	0.002%
39	7.973	2154	2156	2163	rBV9	955	1120	0.01%	0.004%
40	8.024	2163	2172	2209	rBV	494161	968291	12.64%	3.159%
41	8.323	2261	2265	2268	rBV6	1678	1728	0.02%	0.006%
42	8.464	2306	2309	2311	rBV3	1582	1060	0.01%	0.003%
43	8.542	2331	2333	2335	rBV3	1074	676	0.01%	0.002%
44	8.571	2340	2342	2346	rBV5	810	716	0.01%	0.002%
45	8.635	2359	2362	2365	rVB5	1417	835	0.01%	0.003%
46	8.661	2365	2370	2371	rBV4	1207	957	0.01%	0.003%
47	8.780	2396	2407	2437	rBV	1183192	1953122	25.49%	6.372%
48	9.085	2500	2502	2505	rVB4	1784	991	0.01%	0.003%
49	9.181	2529	2532	2534	rBV3	1467	951	0.01%	0.003%
50	9.198	2534	2537	2541	rVV5	1597	1293	0.02%	0.004%
51	9.252	2551	2554	2558	rBV5	1456	998	0.01%	0.003%
52	9.307	2565	2571	2572	rBV4	1226	1084	0.01%	0.004%
53	9.339	2576	2581	2585	rVV7	1362	1568	0.02%	0.005%
54	9.362	2586	2588	2592	rVV4	1836	973	0.01%	0.003%
55	9.384	2592	2595	2598	rVV5	781	774	0.01%	0.003%
56	9.432	2607	2610	2612	rVB3	1308	680	0.01%	0.002%
57	9.487	2621	2627	2631	rBV7	1491	1572	0.02%	0.005%
58	9.516	2634	2636	2641	rVB6	836	678	0.01%	0.002%
59	9.542	2641	2644	2646	rBV4	1325	912	0.01%	0.003%
60	9.616	2663	2667	2669	rBV5	793	650	0.01%	0.002%
61	9.664	2679	2682	2684	rBV4	1101	692	0.01%	0.002%
62	9.699	2689	2693	2697	rBV7	787	731	0.01%	0.002%
63	9.799	2720	2724	2725	rBV4	1277	745	0.01%	0.002%
64	9.828	2729	2733	2736	rBV5	1214	845	0.01%	0.003%
65	9.853	2736	2741	2742	rBV5	1183	1031	0.01%	0.003%
66	9.889	2750	2752	2758	rVB6	1357	1034	0.01%	0.003%
67	9.924	2758	2763	2766	rVB5	1009	810	0.01%	0.003%
68	9.953	2769	2772	2774	rBV3	1128	633	0.01%	0.002%
69	10.005	2784	2788	2791	rBV6	1659	1293	0.02%	0.004%
70	10.024	2791	2794	2797	rBV4	1095	743	0.01%	0.002%
71	10.050	2800	2802	2807	rVB5	1040	883	0.01%	0.003%
72	10.149	2821	2833	2858	rBV	721957	1140117	14.88%	3.719%
73	10.400	2907	2911	2913	rBV5	1526	1068	0.01%	0.003%
74	10.567	2960	2963	2968	rVV6	1547	1540	0.02%	0.005%
75	10.590	2968	2970	2975	rVV5	1302	1020	0.01%	0.003%
76	10.612	2975	2977	2981	rVB5	1275	1087	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037090.D
 Acq On : 27 Aug 2024 16:43
 Operator : SY/MD
 Sample : P3692-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	10.693	2998	3002	3006	rBV6	921	900	0.01%	0.003%
78	10.725	3011	3012	3016	rVB3	1280	786	0.01%	0.003%
79	10.789	3030	3032	3037	rVB5	1469	1070	0.01%	0.003%
80	10.841	3044	3048	3050	rBV4	995	831	0.01%	0.003%
81	10.895	3062	3065	3070	rBV5	1271	905	0.01%	0.003%
82	10.960	3082	3085	3089	rBV5	898	826	0.01%	0.003%
83	11.053	3110	3114	3115	rBV3	1176	811	0.01%	0.003%
84	11.091	3124	3126	3131	rBV6	1092	721	0.01%	0.002%
85	11.120	3132	3135	3137	rBV4	1250	905	0.01%	0.003%
86	11.181	3143	3154	3192	rBV	1262735	1996081	26.05%	6.512%
87	11.554	3258	3270	3293	rBV	1144202	1824629	23.81%	5.952%
88	11.812	3348	3350	3353	rVB4	1659	929	0.01%	0.003%
89	11.831	3353	3356	3358	rBV4	1672	1122	0.01%	0.004%
90	11.873	3365	3369	3373	rVB6	1751	1589	0.02%	0.005%
91	11.972	3397	3400	3403	rBV5	1656	950	0.01%	0.003%
92	12.056	3421	3426	3432	rBV9	1885	2196	0.03%	0.007%
93	12.146	3451	3454	3459	rBV7	1076	1118	0.01%	0.004%
94	12.178	3462	3464	3466	rBV3	1516	981	0.01%	0.003%
95	12.246	3483	3485	3489	rBV4	1431	1225	0.02%	0.004%
96	12.294	3497	3500	3501	rBV3	1589	781	0.01%	0.003%
97	12.493	3560	3562	3565	rVB4	1526	632	0.01%	0.002%
98	12.821	3658	3664	3665	rBV5	2242	2381	0.03%	0.008%
99	13.046	3730	3734	3737	rBV5	1994	1779	0.02%	0.006%
100	13.316	3815	3818	3819	rBV3	1660	1046	0.01%	0.003%




Sum of corrected areas: 30653596

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037090.D
Acq On : 27 Aug 2024 16:43
Operator : SY/MD
Sample : P3692-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

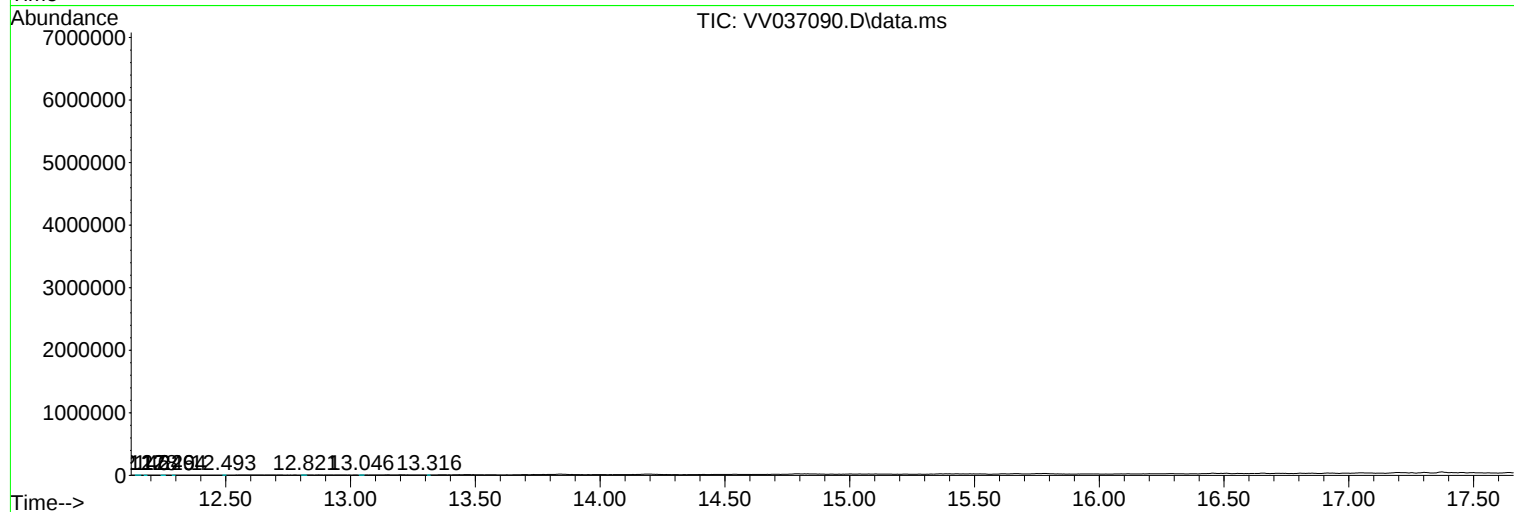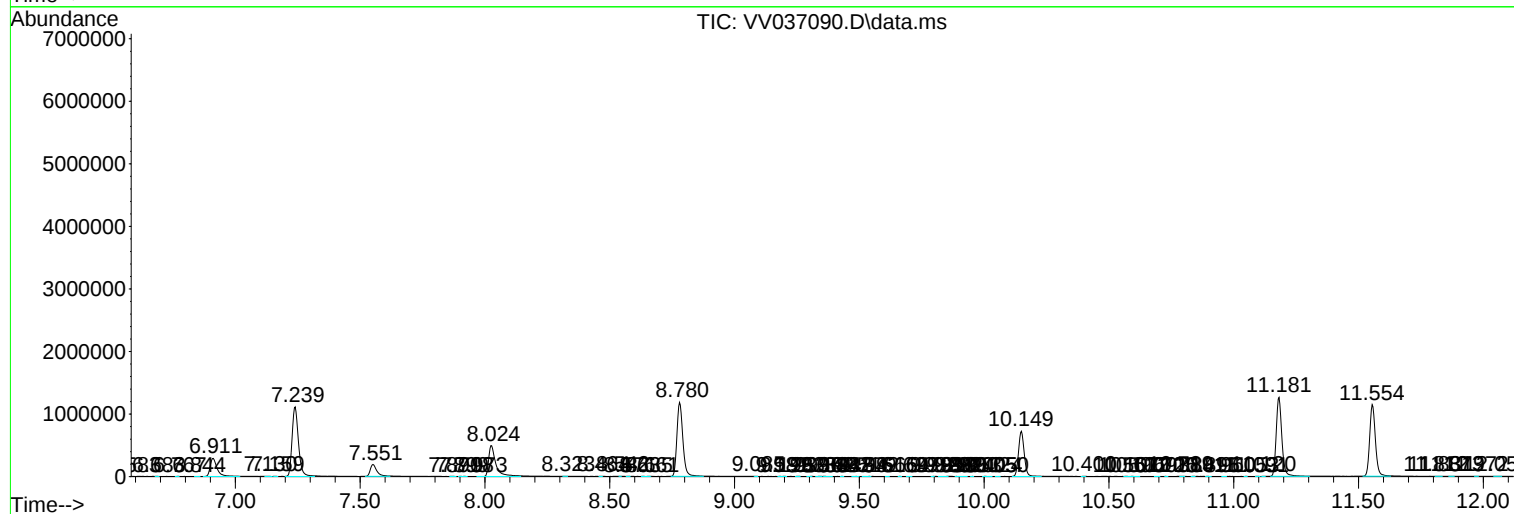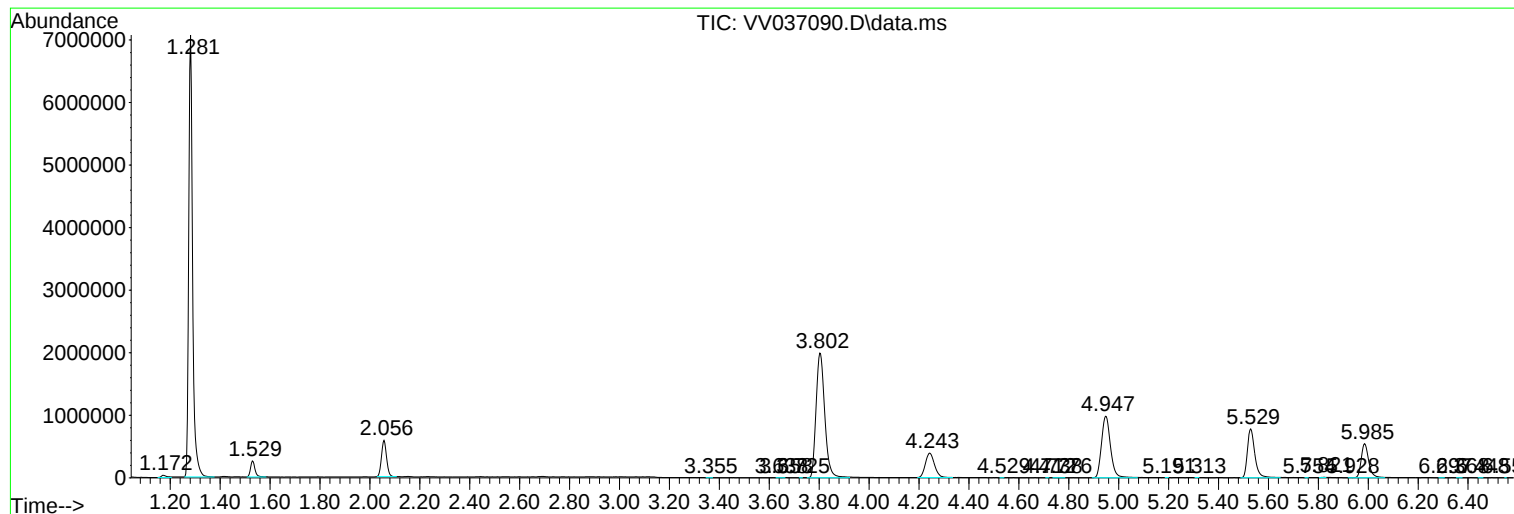

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037090.D
Acq On : 27 Aug 2024 16:43
Operator : SY/MD
Sample : P3692-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037090.D
Acq On : 27 Aug 2024 16:43
Operator : SY/MD
Sample : P3692-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc