

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037096.D
 Acq On : 27 Aug 2024 19:18
 Operator : SY/MD
 Sample : P3692-15
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	36	41	50	rBV	24356	32117	1.32%	0.168%
2	1.278	68	74	93	rVB	299045	312561	12.82%	1.630%
3	1.529	146	152	172	rVB	258397	318120	13.05%	1.659%
4	2.056	307	316	331	rBV	558854	796039	32.65%	4.153%
5	3.256	685	689	691	rBV5	1636	1392	0.06%	0.007%
6	3.481	755	759	761	rBV5	1212	880	0.04%	0.005%
7	3.513	767	769	770	rBV3	687	307	0.01%	0.002%
8	3.584	788	791	793	rBV3	1130	794	0.03%	0.004%
9	3.648	809	811	812	rBV	639	249	0.01%	0.001%
10	3.677	818	820	822	rBV2	855	267	0.01%	0.001%
11	3.761	842	846	848	rBV3	1252	869	0.04%	0.005%
12	3.799	848	858	888	rBV	171645	479003	19.65%	2.499%
13	4.243	981	996	1022	rBV	383267	986292	40.45%	5.145%
14	4.458	1061	1063	1067	rBV5	1294	796	0.03%	0.004%
15	4.545	1088	1090	1091	rBV	1366	595	0.02%	0.003%
16	4.670	1126	1129	1131	rBV4	1200	851	0.03%	0.004%
17	4.725	1141	1146	1147	rBV5	1085	873	0.04%	0.005%
18	4.793	1164	1167	1169	rBV4	872	471	0.02%	0.002%
19	4.828	1175	1178	1180	rBV3	801	673	0.03%	0.004%
20	4.838	1180	1181	1183	rBV2	885	416	0.02%	0.002%
21	4.950	1199	1216	1247	rBV2	985723	2438160	100.00%	12.719%
22	5.455	1371	1373	1377	rVB4	1281	841	0.03%	0.004%
23	5.529	1384	1396	1434	rBV	783640	1604753	65.82%	8.371%
24	5.831	1479	1490	1513	rBV	202923	419896	17.22%	2.190%
25	5.986	1525	1538	1564	rBV	536352	1104315	45.29%	5.761%
26	6.333	1643	1646	1648	rBV4	1138	773	0.03%	0.004%
27	6.445	1679	1681	1683	rVB3	927	468	0.02%	0.002%
28	6.503	1695	1699	1704	rVB6	1171	1225	0.05%	0.006%
29	6.558	1714	1716	1718	rBV4	744	347	0.01%	0.002%
30	6.593	1725	1727	1729	rBV3	1138	628	0.03%	0.003%
31	6.619	1732	1735	1738	rVV5	954	613	0.03%	0.003%
32	6.728	1765	1769	1773	rBV5	1300	1238	0.05%	0.006%
33	6.783	1784	1786	1790	rVB5	757	555	0.02%	0.003%
34	6.815	1794	1796	1799	rBV4	800	530	0.02%	0.003%
35	6.828	1799	1800	1802	rVB2	849	231	0.01%	0.001%
36	6.841	1802	1804	1805	rBV2	613	313	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037096.D
 Acq On : 27 Aug 2024 19:18
 Operator : SY/MD
 Sample : P3692-15
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.912	1816	1826	1851	rBV	275028	528515	21.68%	2.757%
38	7.143	1895	1898	1900	rBV2	1345	910	0.04%	0.005%
39	7.239	1916	1928	1958	rBV	1084230	1934010	79.32%	10.089%
40	7.551	2016	2025	2053	rBV	182625	342182	14.03%	1.785%
41	7.841	2112	2115	2116	rBV3	633	420	0.02%	0.002%
42	7.960	2148	2152	2154	rBV5	1349	895	0.04%	0.005%
43	8.027	2162	2173	2217	rBV	472240	947176	38.85%	4.941%
44	8.606	2352	2353	2356	rBV3	920	511	0.02%	0.003%
45	8.731	2390	2392	2394	rVB2	918	429	0.02%	0.002%
46	8.780	2396	2407	2431	rBV	1206597	1956920	80.26%	10.208%
47	9.326	2574	2577	2580	rBV5	1258	803	0.03%	0.004%
48	9.403	2600	2601	2604	rBV4	710	322	0.01%	0.002%
49	9.458	2614	2618	2622	rBV5	1335	1270	0.05%	0.007%
50	9.474	2622	2623	2624	rBV	930	319	0.01%	0.002%
51	9.619	2667	2668	2670	rVB2	933	238	0.01%	0.001%
52	9.680	2686	2687	2688	rBV	674	219	0.01%	0.001%
53	9.738	2701	2705	2707	rBV4	1245	956	0.04%	0.005%
54	9.780	2716	2718	2720	rVB3	961	411	0.02%	0.002%
55	9.818	2727	2730	2732	rBV4	612	365	0.01%	0.002%
56	9.834	2732	2735	2737	rBV4	733	460	0.02%	0.002%
57	9.847	2737	2739	2740	rBV2	877	440	0.02%	0.002%
58	9.934	2764	2766	2768	rBV2	1016	467	0.02%	0.002%
59	9.956	2768	2773	2776	rBV6	1541	1766	0.07%	0.009%
60	9.989	2781	2783	2785	rVV3	1276	546	0.02%	0.003%
61	10.149	2820	2833	2852	rBV	715801	1129119	46.31%	5.890%
62	10.358	2896	2898	2899	rVB2	1007	253	0.01%	0.001%
63	10.426	2915	2919	2920	rBV4	1245	713	0.03%	0.004%
64	10.452	2926	2927	2929	rBV	1000	487	0.02%	0.003%
65	10.609	2970	2976	2979	rBV7	1162	1335	0.05%	0.007%
66	10.673	2993	2996	2998	rBV3	437	276	0.01%	0.001%
67	10.686	2998	3000	3004	rVB5	968	599	0.02%	0.003%
68	10.712	3006	3008	3010	rVB3	633	322	0.01%	0.002%
69	10.735	3010	3015	3018	rBV5	1094	1096	0.04%	0.006%
70	10.786	3024	3031	3038	rVB9	2123	2940	0.12%	0.015%
71	10.818	3038	3041	3044	rBV5	1474	1238	0.05%	0.006%
72	10.979	3089	3091	3092	rBV2	850	240	0.01%	0.001%
73	11.046	3110	3112	3114	rBV2	1111	606	0.02%	0.003%
74	11.085	3122	3124	3125	rVB	431	129	0.01%	0.001%
75	11.098	3125	3128	3129	rBV2	881	539	0.02%	0.003%
76	11.181	3143	3154	3185	rBV	1243597	1983373	81.35%	10.346%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037096.D
 Acq On : 27 Aug 2024 19:18
 Operator : SY/MD
 Sample : P3692-15
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.554	3259	3270	3298	rBV	1107327	1785440	73.23%	9.314%
78	11.837	3355	3358	3361	rBV5	1562	1343	0.06%	0.007%
79	11.969	3395	3399	3402	rVB5	1843	1258	0.05%	0.007%
80	11.998	3406	3408	3411	rBV5	1587	902	0.04%	0.005%
81	12.046	3420	3423	3425	rBV5	1431	909	0.04%	0.005%
82	12.091	3433	3437	3441	rBV5	1296	1187	0.05%	0.006%
83	12.146	3452	3454	3456	rVB4	649	247	0.01%	0.001%
84	12.162	3456	3459	3460	rBV3	1070	584	0.02%	0.003%
85	12.249	3485	3486	3487	rBV	645	189	0.01%	0.001%
86	12.349	3513	3517	3519	rBV3	1406	973	0.04%	0.005%
87	12.487	3558	3560	3561	rBV3	808	263	0.01%	0.001%
88	12.583	3581	3590	3592	rBV8	4942	6091	0.25%	0.032%
89	12.670	3615	3617	3621	rBV3	1187	1017	0.04%	0.005%
90	12.718	3630	3632	3635	rBV3	1122	546	0.02%	0.003%
91	12.767	3645	3647	3650	rVB4	927	404	0.02%	0.002%
92	12.783	3650	3652	3655	rBV4	1457	919	0.04%	0.005%
93	12.882	3679	3683	3684	rBV2	1675	1170	0.05%	0.006%
94	13.062	3737	3739	3741	rBV3	1019	307	0.01%	0.002%
95	13.201	3776	3782	3787	rBV7	5405	7861	0.32%	0.041%
96	13.339	3822	3825	3827	rBV4	995	564	0.02%	0.003%
97	13.390	3837	3841	3844	rBV4	1110	859	0.04%	0.004%
98	13.979	4022	4024	4029	rBV4	1770	1469	0.06%	0.008%
99	14.175	4083	4085	4088	rBV3	2453	1654	0.07%	0.009%
100	14.696	4245	4247	4249	rBV3	2283	1376	0.06%	0.007%



Sum of corrected areas: 19169798

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037096.D
Acq On : 27 Aug 2024 19:18
Operator : SY/MD
Sample : P3692-15
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

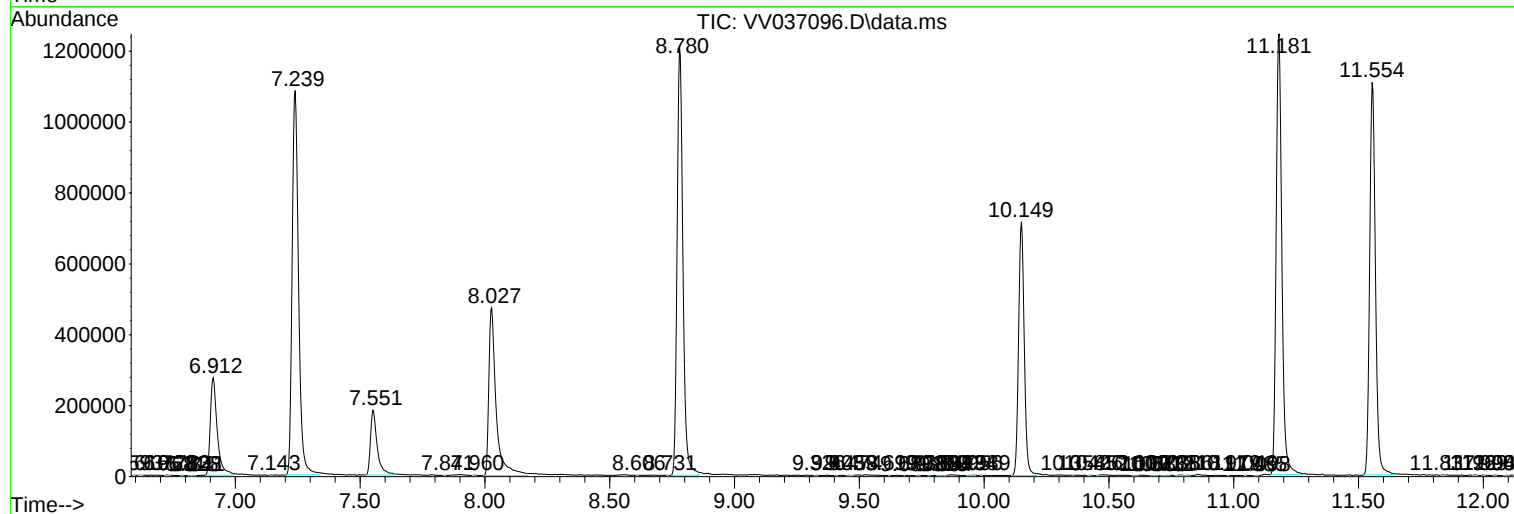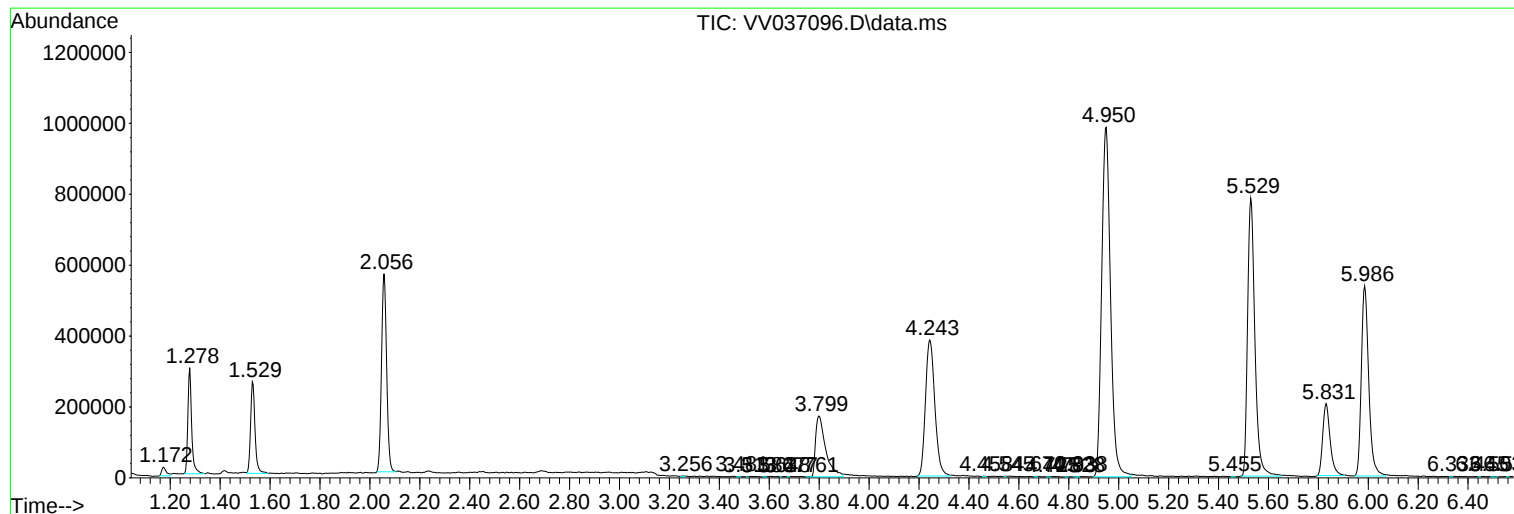

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037096.D
Acq On : 27 Aug 2024 19:18
Operator : SY/MD
Sample : P3692-15
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037096.D
Acq On : 27 Aug 2024 19:18
Operator : SY/MD
Sample : P3692-15
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc