

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037113.D
 Acq On : 28 Aug 2024 01:36
 Operator : SY/MD
 Sample : P3693-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	52	rBV	38052	58208	2.53%	0.342%
2	1.278	68	74	93	rVB2	280929	303672	13.22%	1.782%
3	1.532	146	153	166	rVB	234377	268987	11.71%	1.579%
4	2.056	308	316	329	rBV	469778	673337	29.31%	3.952%
5	3.432	742	744	749	rVB4	1504	953	0.04%	0.006%
6	3.580	789	790	793	rVB2	953	385	0.02%	0.002%
7	3.667	813	817	818	rBV4	1069	770	0.03%	0.005%
8	3.796	846	857	889	rBV	149646	431214	18.77%	2.531%
9	4.243	981	996	1028	rBV	358843	907406	39.50%	5.326%
10	4.648	1120	1122	1124	rBV3	704	261	0.01%	0.002%
11	4.712	1140	1142	1144	rBV3	922	465	0.02%	0.003%
12	4.776	1159	1162	1168	rBV5	842	775	0.03%	0.005%
13	4.799	1168	1169	1171	rBV2	970	475	0.02%	0.003%
14	4.950	1200	1216	1255	rBV2	895987	2297102	100.00%	13.483%
15	5.529	1384	1396	1421	rBV	704105	1450450	63.14%	8.513%
16	5.838	1481	1492	1507	rBV	13193	32742	1.43%	0.192%
17	5.985	1526	1538	1560	rBV	501883	1028405	44.77%	6.036%
18	6.407	1666	1669	1673	rBV5	1660	1224	0.05%	0.007%
19	6.574	1719	1721	1723	rBV3	1411	605	0.03%	0.004%
20	6.651	1741	1745	1746	rBV3	925	654	0.03%	0.004%
21	6.712	1759	1764	1769	rBV8	2127	2600	0.11%	0.015%
22	6.860	1807	1810	1813	rBV5	1509	1119	0.05%	0.007%
23	6.911	1816	1826	1857	rVV	233871	456719	19.88%	2.681%
24	7.239	1917	1928	1956	rBV	995731	1761312	76.68%	10.338%
25	7.506	2009	2011	2014	rBV4	1606	977	0.04%	0.006%
26	7.551	2016	2025	2050	rVV	155171	292064	12.71%	1.714%
27	7.808	2103	2105	2107	rVB3	2183	903	0.04%	0.005%
28	7.940	2144	2146	2148	rBV3	980	334	0.01%	0.002%
29	8.024	2164	2172	2208	rBV	405141	821102	35.75%	4.820%
30	8.497	2317	2319	2320	rBV2	1134	479	0.02%	0.003%
31	8.519	2324	2326	2331	rVV6	1584	1151	0.05%	0.007%
32	8.780	2396	2407	2434	rBV	1088398	1786929	77.79%	10.488%
33	9.365	2586	2589	2591	rBV4	1231	778	0.03%	0.005%
34	9.426	2604	2608	2614	rBV7	1808	1650	0.07%	0.010%
35	9.452	2614	2616	2619	rBV3	1035	605	0.03%	0.004%
36	9.493	2627	2629	2634	rVB6	1852	1137	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
 Data File : VV037113.D
 Acq On : 28 Aug 2024 01:36
 Operator : SY/MD
 Sample : P3693-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.519	2634	2637	2641	rBV6	1491	1273	0.06%	0.007%
38	9.545	2641	2645	2646	rBV3	1149	715	0.03%	0.004%
39	9.619	2664	2668	2669	rBV3	1162	953	0.04%	0.006%
40	9.638	2673	2674	2677	rBV3	1055	492	0.02%	0.003%
41	9.712	2695	2697	2700	rVB3	764	343	0.01%	0.002%
42	9.834	2730	2735	2738	rBV6	1285	1372	0.06%	0.008%
43	9.940	2764	2768	2769	rBV4	1337	913	0.04%	0.005%
44	10.091	2812	2815	2818	rVB5	840	468	0.02%	0.003%
45	10.149	2821	2833	2850	rBV	657274	1037642	45.17%	6.090%
46	10.426	2917	2919	2923	rVB5	1139	812	0.04%	0.005%
47	10.477	2931	2935	2936	rBV3	1059	654	0.03%	0.004%
48	10.567	2961	2963	2964	rBV2	1237	502	0.02%	0.003%
49	10.635	2980	2984	2987	rBV5	1120	748	0.03%	0.004%
50	10.657	2989	2991	2993	rBV3	503	248	0.01%	0.001%
51	10.693	3001	3002	3006	rVB3	923	434	0.02%	0.003%
52	10.731	3006	3014	3015	rBV5	1163	1071	0.05%	0.006%
53	10.853	3048	3052	3053	rBV3	1386	873	0.04%	0.005%
54	10.943	3075	3080	3083	rBV6	1091	1101	0.05%	0.006%
55	11.114	3129	3133	3136	rBV5	1292	1217	0.05%	0.007%
56	11.181	3143	3154	3182	rBV	1101380	1748789	76.13%	10.265%
57	11.471	3242	3244	3246	rBV3	1023	404	0.02%	0.002%
58	11.554	3259	3270	3296	rBV	997869	1629559	70.94%	9.565%
59	11.824	3352	3354	3357	rBV4	1510	916	0.04%	0.005%
60	12.078	3429	3433	3436	rBV5	906	767	0.03%	0.005%
61	12.094	3436	3438	3440	rBV3	1084	602	0.03%	0.004%
62	12.130	3446	3449	3453	rBV5	1547	1357	0.06%	0.008%
63	12.291	3497	3499	3502	rBV4	1168	638	0.03%	0.004%
64	12.406	3533	3535	3538	rBV3	1061	462	0.02%	0.003%
65	12.593	3589	3593	3600	rBV8	2122	3040	0.13%	0.018%
66	12.673	3617	3618	3621	rBV3	1233	694	0.03%	0.004%
67	12.734	3634	3637	3639	rBV4	1083	919	0.04%	0.005%
68	12.873	3676	3680	3681	rBV3	1505	1212	0.05%	0.007%
69	12.975	3710	3712	3713	rBV2	954	325	0.01%	0.002%
70	13.001	3717	3720	3721	rBV2	921	407	0.02%	0.002%
71	13.352	3827	3829	3832	rVB3	1313	517	0.02%	0.003%
72	13.400	3841	3844	3846	rBV3	1111	758	0.03%	0.004%
73	13.602	3902	3907	3911	rBV7	2173	2059	0.09%	0.012%
74	14.043	4042	4044	4047	rBV4	1548	919	0.04%	0.005%
75	14.078	4054	4055	4061	rVB4	1900	1293	0.06%	0.008%
76	14.101	4061	4062	4065	rBV4	1307	818	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037113.D
Acq On : 28 Aug 2024 01:36
Operator : SY/MD
Sample : P3693-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K76

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis

77	14.300	4122	4124	4126	rBV2	1676	824	0.04%	0.005%
----	--------	------	------	------	------	------	-----	-------	--------




Sum of corrected areas: 17037059

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037113.D
Acq On : 28 Aug 2024 01:36
Operator : SY/MD
Sample : P3693-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

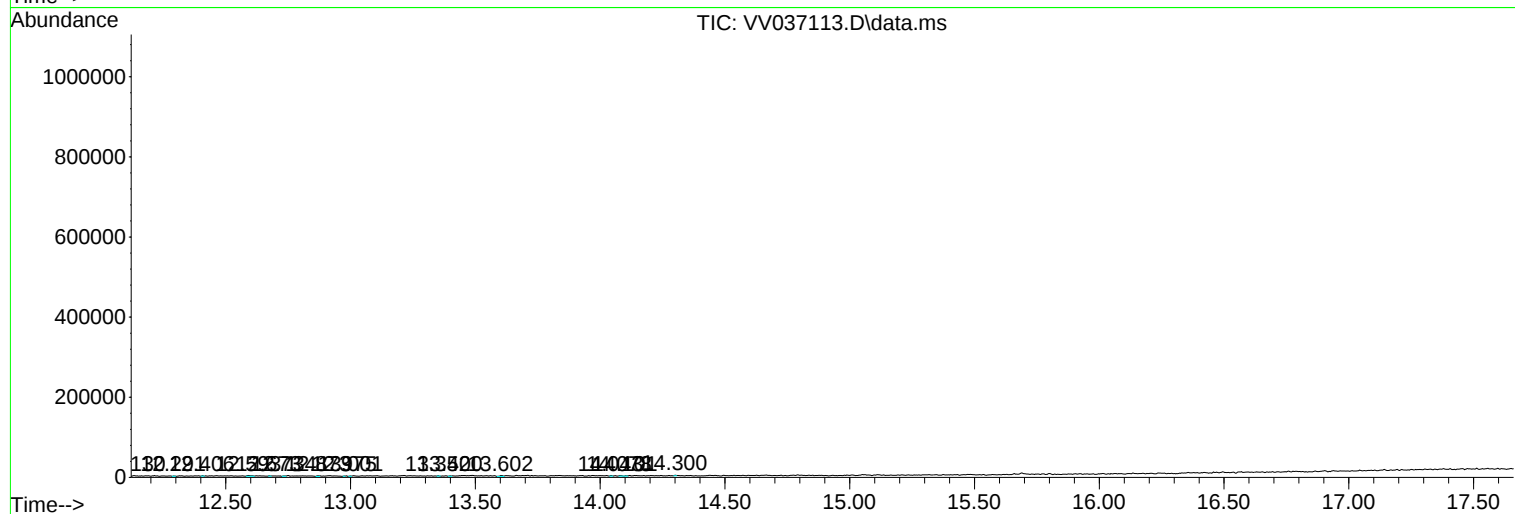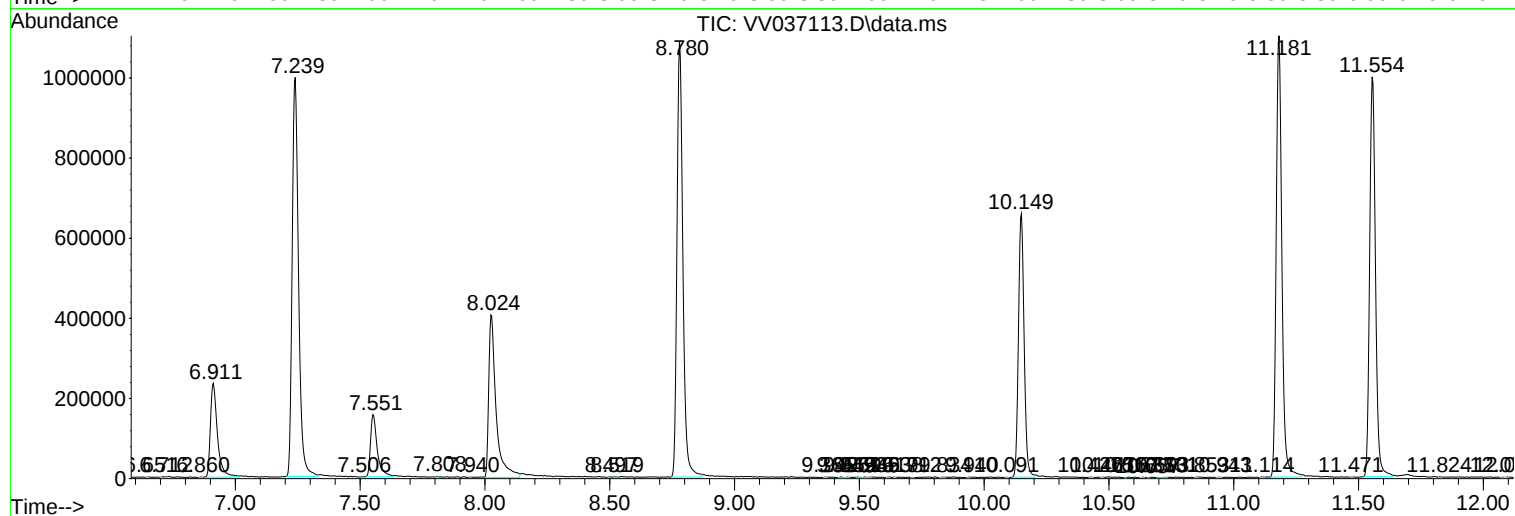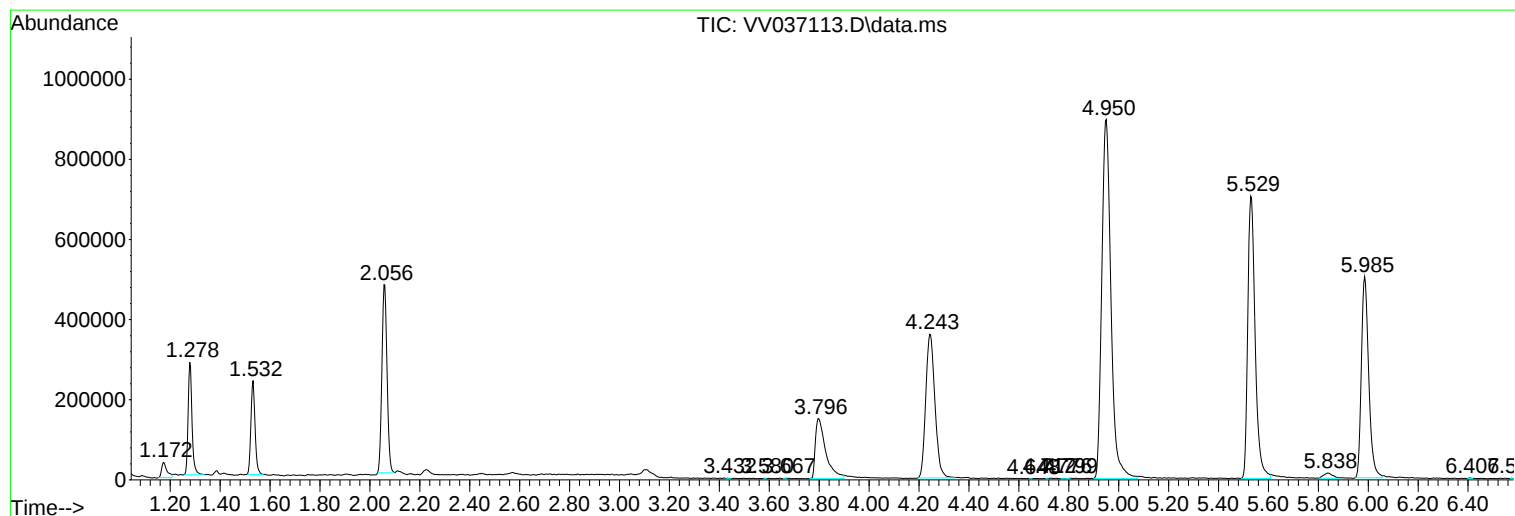

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037113.D
Acq On : 28 Aug 2024 01:36
Operator : SY/MD
Sample : P3693-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037113.D
Acq On : 28 Aug 2024 01:36
Operator : SY/MD
Sample : P3693-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------