
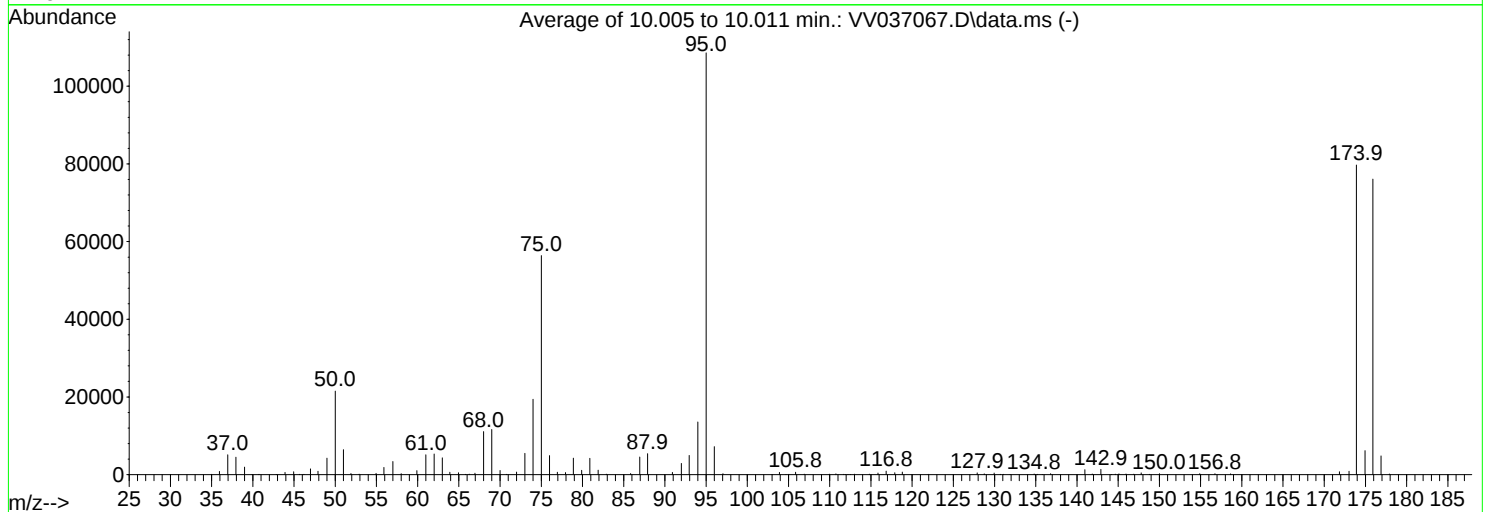


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082724\
Data File : VV037067.D
Acq On : 27 Aug 2024 07:42
Operator : SY/MD
Sample : BFB369
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB369

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis
Last Update : Thu Aug 29 04:43:38 2024

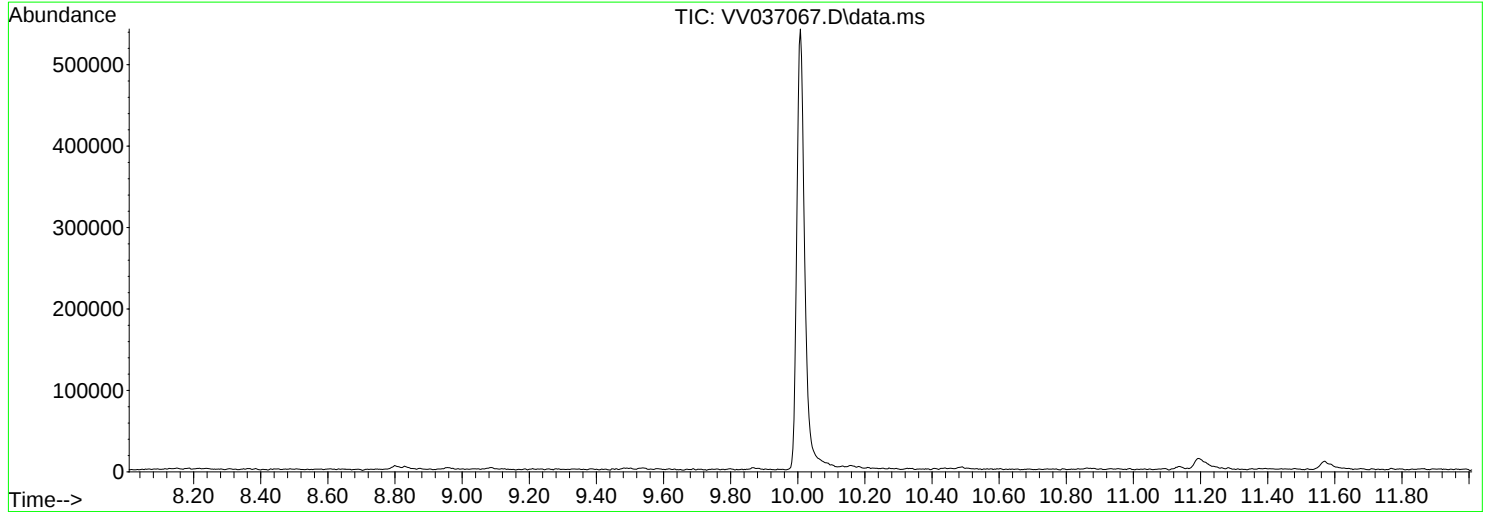

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	21485	PASS
75	95	30	80	51.9	56381	PASS
95	95	100	100	100.0	108592	PASS
96	95	5	9	6.7	7222	PASS
173	174	0.00	2	1.1	870	PASS
174	95	50	120	73.4	79720	PASS
175	174	5	9	7.7	6164	PASS
176	174	95	105	95.5	76101	PASS
177	176	5	10	6.3	4810	PASS

m/z	Abundance
35.40	106.0
35.90	137.0
36.90	110.0
37.80	162.0
39.00	157.0
39.80	410.0
41.80	153.0
42.80	194.0
43.20	178.0
43.90	860.0
44.80	168.0
48.20	169.0
207.00	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

m/z	Abundance
35.00	151.0
36.00	995.0
37.00	5240.0
38.00	4797.0
39.00	2034.0
40.00	498.0
40.80	174.0
42.80	235.0
43.90	1519.0
45.00	865.0
46.20	140.0
47.00	1544.0
47.90	792.0
49.00	4378.0
50.00	21336.0
51.00	6733.0
51.90	293.0
55.00	424.0
55.90	2022.0
57.00	3483.0
58.00	202.0
59.90	1175.0
61.00	5319.0
62.00	5245.0
63.00	4343.0
63.90	757.0
64.90	504.0
66.30	177.0
66.90	377.0
68.00	10998.0
69.00	11623.0
70.00	1054.0
72.00	688.0
73.00	5293.0
74.00	19512.0
75.00	57184.0
76.00	5036.0
76.90	663.0
78.00	593.0
78.90	4354.0
79.90	1053.0
80.90	4185.0
81.90	1124.0
82.80	114.0
85.80	283.0
86.90	4475.0
87.90	5323.0
90.90	594.0
92.00	2830.0
93.00	5002.0
94.00	14003.0
95.00	108928.0
96.00	7219.0
97.10	311.0
103.90	495.0
105.10	183.0
105.90	600.0
106.80	148.0
110.00	103.0
110.70	163.0
111.70	128.0
112.20	118.0
114.80	136.0
115.90	389.0
116.80	750.0
117.90	539.0
118.80	618.0
121.90	136.0
127.90	434.0
128.70	182.0
130.00	355.0
130.70	169.0
131.90	101.0
134.80	227.0
136.80	293.0
140.90	1204.0
141.90	199.0
142.90	1346.0
144.20	114.0
145.00	202.0
145.90	166.0
147.00	114.0
147.80	397.0
150.00	225.0
154.90	223.0
156.80	274.0
158.60	222.0
171.90	681.0
173.00	818.0
173.90	77424.0
175.00	6191.0
175.90	75080.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

176.904656.0

177.90156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

m/z	Abundance
35.00	129.0
36.00	944.0
37.00	5353.0
38.00	4762.0
39.00	2173.0
40.00	454.0
40.70	119.0
42.90	230.0
43.90	1439.0
45.00	900.0
45.60	146.0
46.20	152.0
47.00	1541.0
47.90	946.0
49.00	4305.0
50.00	22168.0
51.00	6647.0
51.90	317.0
52.90	148.0
55.00	327.0
55.90	1913.0
57.00	3462.0
58.00	232.0
59.90	1032.0
61.00	5314.0
62.00	5455.0
63.00	4441.0
63.90	665.0
65.00	466.0
65.80	140.0
66.30	144.0
66.90	390.0
68.00	11583.0
69.00	11956.0
70.00	1127.0
70.80	113.0
72.00	678.0
73.00	5642.0
74.00	20080.0
75.00	58472.0
76.00	5164.0
76.90	581.0
77.90	576.0
78.90	4349.0
79.90	1137.0
80.90	4326.0
81.90	1183.0
82.90	152.0
85.80	312.0
86.90	4579.0
87.90	5656.0
90.90	624.0
92.00	3019.0
93.00	5110.0
94.00	13857.0
95.00	112128.0
96.00	7365.0
97.00	281.0
103.90	599.0
105.00	138.0
105.80	666.0
106.90	142.0
110.00	148.0
110.80	206.0
111.70	143.0
113.00	154.0
114.80	129.0
115.80	393.0
116.80	961.0
117.90	553.0
118.80	642.0
122.00	139.0
127.90	481.0
128.70	223.0
129.90	421.0
130.70	121.0
131.10	153.0
134.80	175.0
135.20	175.0
135.80	108.0
136.80	284.0
140.90	1343.0
141.80	189.0
142.90	1410.0
144.70	173.0
145.10	209.0
145.90	184.0
146.90	123.0
147.80	470.0
148.80	148.0
150.00	258.0
154.90	235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

156.80	229.0
158.70	241.0
171.90	756.0
173.00	918.0
173.90	82616.0
174.90	6443.0
175.90	78736.0
176.90	4904.0
177.90	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

m/z	Abundance
36.00	973.0
37.00	5056.0
38.00	4459.0
39.00	2062.0
40.00	411.0
43.00	208.0
43.90	1329.0
45.00	927.0
45.70	132.0
47.00	1395.0
47.90	920.0
49.00	4031.0
50.00	20952.0
51.00	5924.0
51.90	323.0
52.90	182.0
54.90	262.0
55.90	1669.0
57.00	3206.0
58.00	275.0
59.90	888.0
61.00	4707.0
62.00	5292.0
63.00	4139.0
63.90	451.0
65.00	523.0
65.80	161.0
66.20	120.0
67.00	388.0
68.00	10641.0
69.00	11251.0
70.00	1085.0
70.80	132.0
72.00	644.0
73.00	5500.0
74.00	18560.0
75.00	53488.0
76.00	4555.0
77.00	645.0
77.90	494.0
78.90	3999.0
79.90	1131.0
80.90	4108.0
81.90	1104.0
83.00	163.0
85.90	259.0
87.00	4574.0
87.90	5189.0
90.90	544.0
92.00	2848.0
92.90	4759.0
94.00	12790.0
95.00	104720.0
96.00	7081.0
97.00	183.0
103.00	122.0
103.90	627.0
104.70	126.0
105.80	630.0
107.00	110.0
109.90	191.0
110.80	215.0
111.90	156.0
112.50	116.0
113.00	189.0
114.80	132.0
115.80	408.0
116.90	1036.0
117.90	437.0
118.80	691.0
127.90	502.0
128.80	252.0
129.90	447.0
131.10	135.0
134.70	131.0
135.20	122.0
136.80	217.0
141.00	1330.0
141.80	152.0
142.90	1298.0
144.60	168.0
145.20	156.0
146.00	180.0
146.80	123.0
147.80	445.0
148.80	165.0
150.00	272.0
154.90	233.0
156.70	209.0
158.70	175.0
171.80	783.0
173.00	875.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

173.90	79120.0
174.90	5857.0
175.90	74488.0
176.90	4871.0
177.90	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369