

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037125.D
 Acq On : 28 Aug 2024 12:25
 Operator : SY/MD
 Sample : P3693-23
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K86

Quant Time: Aug 29 04:45:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 29 04:43:38 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.526	114	604684	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.776	117	580474	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.178	152	277862	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	285573	51.628	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	103.260%	
7) Chloroethane-d5		1.532	69	220770	51.642	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.280%	
11) 1,1-Dichloroethene-d2		2.056	65	120368	51.774	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	103.540%	
21) 2-Butanone-d5		3.789	46	221650	103.476	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.480%	
24) Chloroform-d		4.240	84	447766	51.722	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.440%	
26) 1,2-Dichloroethane-d4		4.934	65	287964	52.820	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.640%	
32) Benzene-d6		4.947	84	907013	51.733	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.460%	
36) 1,2-Dichloropropane-d6		5.979	67	284836	51.869	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.740%	
41) Toluene-d8		7.236	98	806044	50.940	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.880%	
43) trans-1,3-Dichloroprop...		7.548	79	120035	47.247	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.500%	
47) 2-Hexanone-d5		8.021	63	150282	100.274	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.270%	
56) 1,1,2,2-Tetrachloroeth...		10.146	84	333454	50.068	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.140%	
66) 1,2-Dichlorobenzene-d4		11.554	152	289275	51.981	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.960%	
Target Compounds							
20) cis-1,2-Dichloroethene		3.802	96	7238	1.599	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037125.D
Acq On : 28 Aug 2024 12:25
Operator : SY/MD
Sample : P3693-23
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K86

Quant Time: Aug 29 04:45:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 29 04:43:38 2024
Response via : Initial Calibration

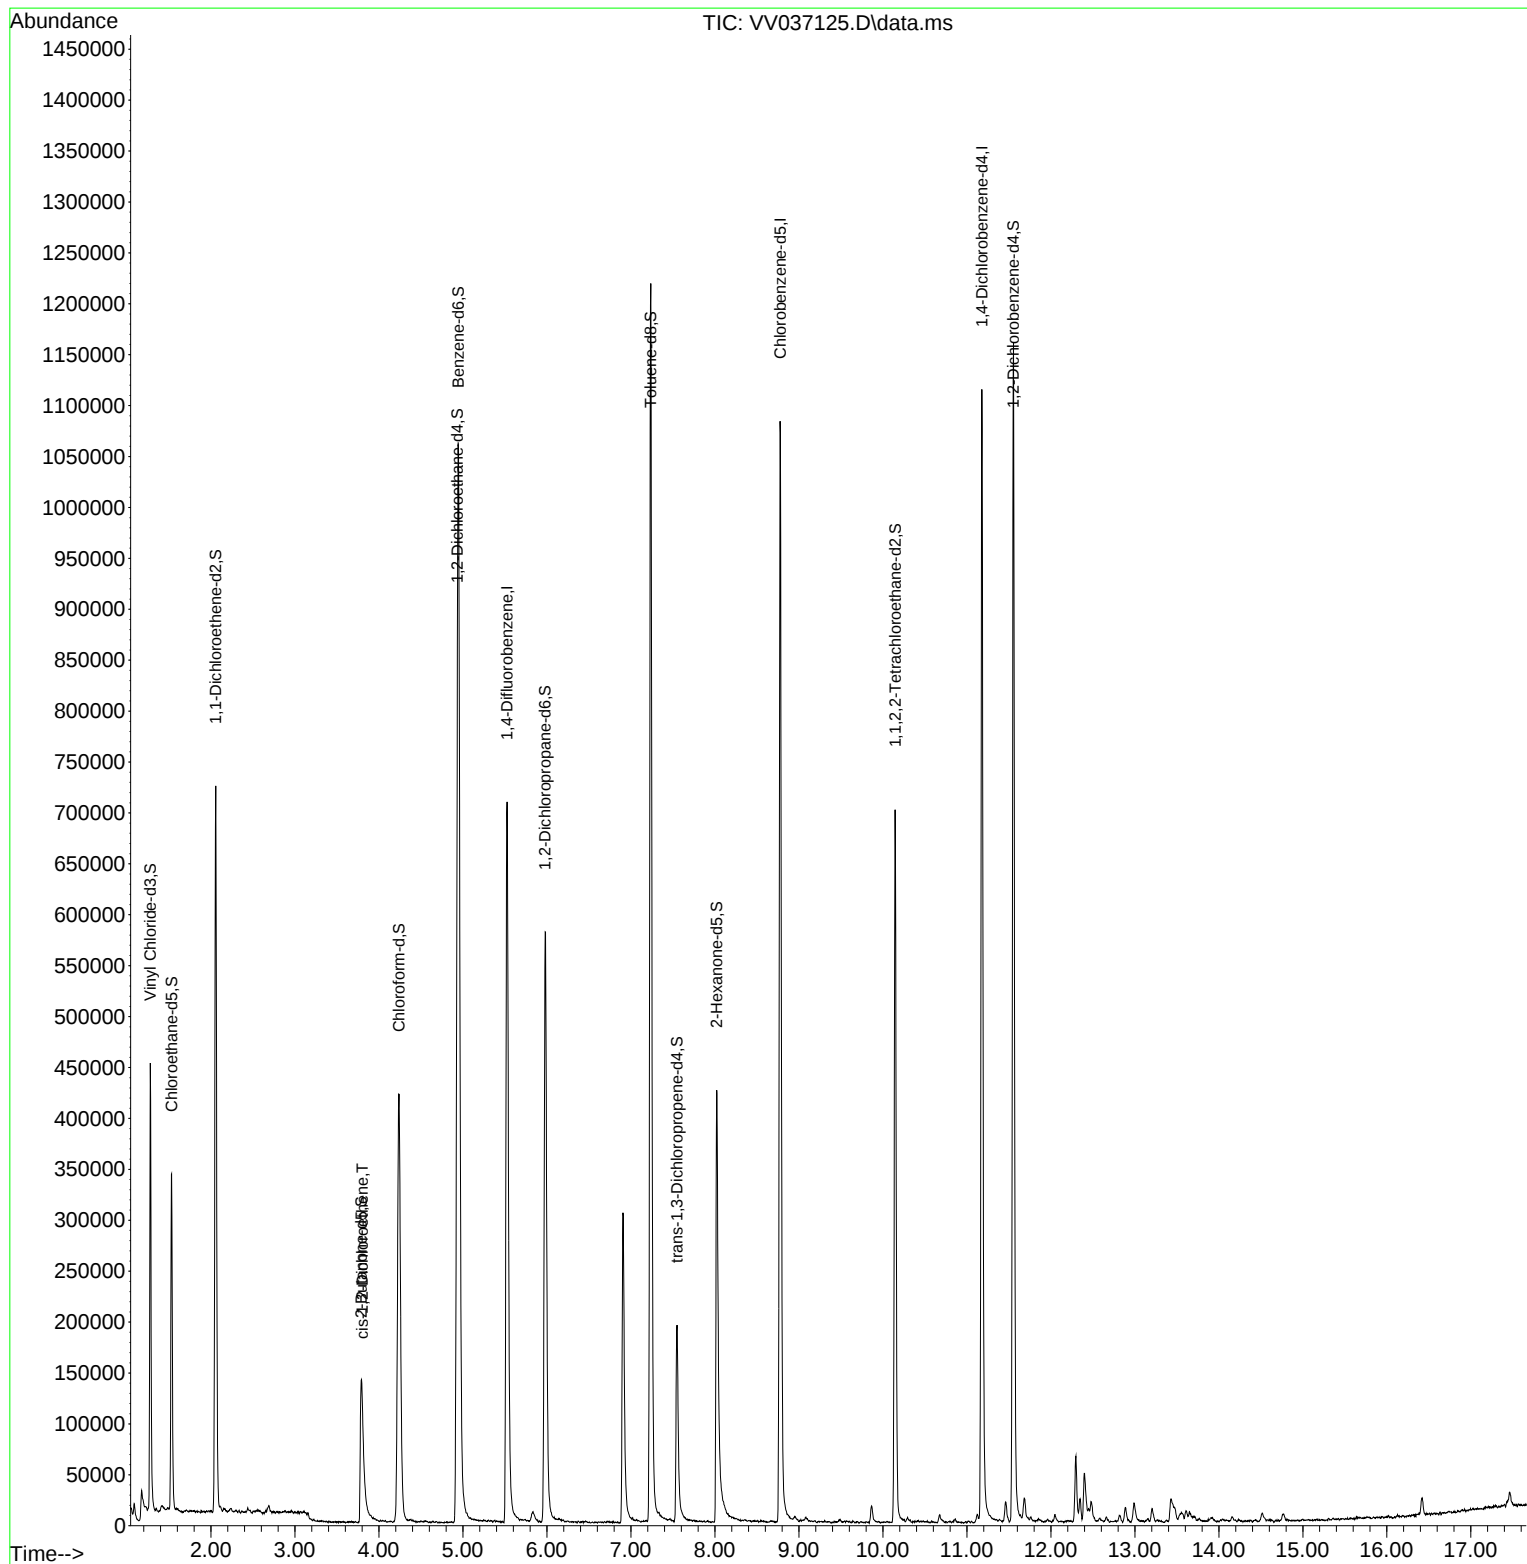

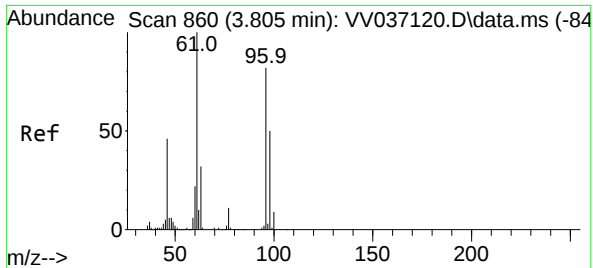

#20
 cis-1,2-Dichloroethene
 Concen: 1.599 ug/L
 RT: 3.802 min Scan# 81
 Delta R.T. -0.003 min
 Lab File: VV037125.D
 Acq: 28 Aug 2024 12:25

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K86

Tgt Ion:	96	Resp:	7238
Ion	Ratio	Lower	Upper
96	100		
61	116.5	89.9	166.9
98	66.8	44.8	83.2

