

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037127.D
 Acq On : 28 Aug 2024 14:01
 Operator : SY/MD
 Sample : P3692-05DL 10X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K42DL

Quant Time: Aug 29 04:45:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 29 04:43:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	674371	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	649101	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	311210	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	287879	46.666	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.340%
7) Chloroethane-d5	1.529	69	225561	47.310	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.620%
11) 1,1-Dichloroethene-d2	2.056	65	122595	47.283	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.560%
21) 2-Butanone-d5	3.789	46	232256	97.223	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.220%
24) Chloroform-d	4.240	84	453374	46.958	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.920%
26) 1,2-Dichloroethane-d4	4.934	65	288603	47.467	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.940%
32) Benzene-d6	4.947	84	928764	47.373	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.740%
36) 1,2-Dichloropropane-d6	5.979	67	288184	46.930	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.860%
41) Toluene-d8	7.236	98	821460	46.426	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.860%
43) trans-1,3-Dichloroprop...	7.548	79	122836	43.238	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.480%
47) 2-Hexanone-d5	8.021	63	157121	93.753	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.750%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	338822	45.495	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.000%
66) 1,2-Dichlorobenzene-d4	11.554	152	292615	46.947	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.900%
Target Compounds						
					Qvalue	
33) Benzene	4.998	78	1069060	57.070	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037127.D
Acq On : 28 Aug 2024 14:01
Operator : SY/MD
Sample : P3692-05DL 10X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K42DL

Quant Time: Aug 29 04:45:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 29 04:43:38 2024
Response via : Initial Calibration

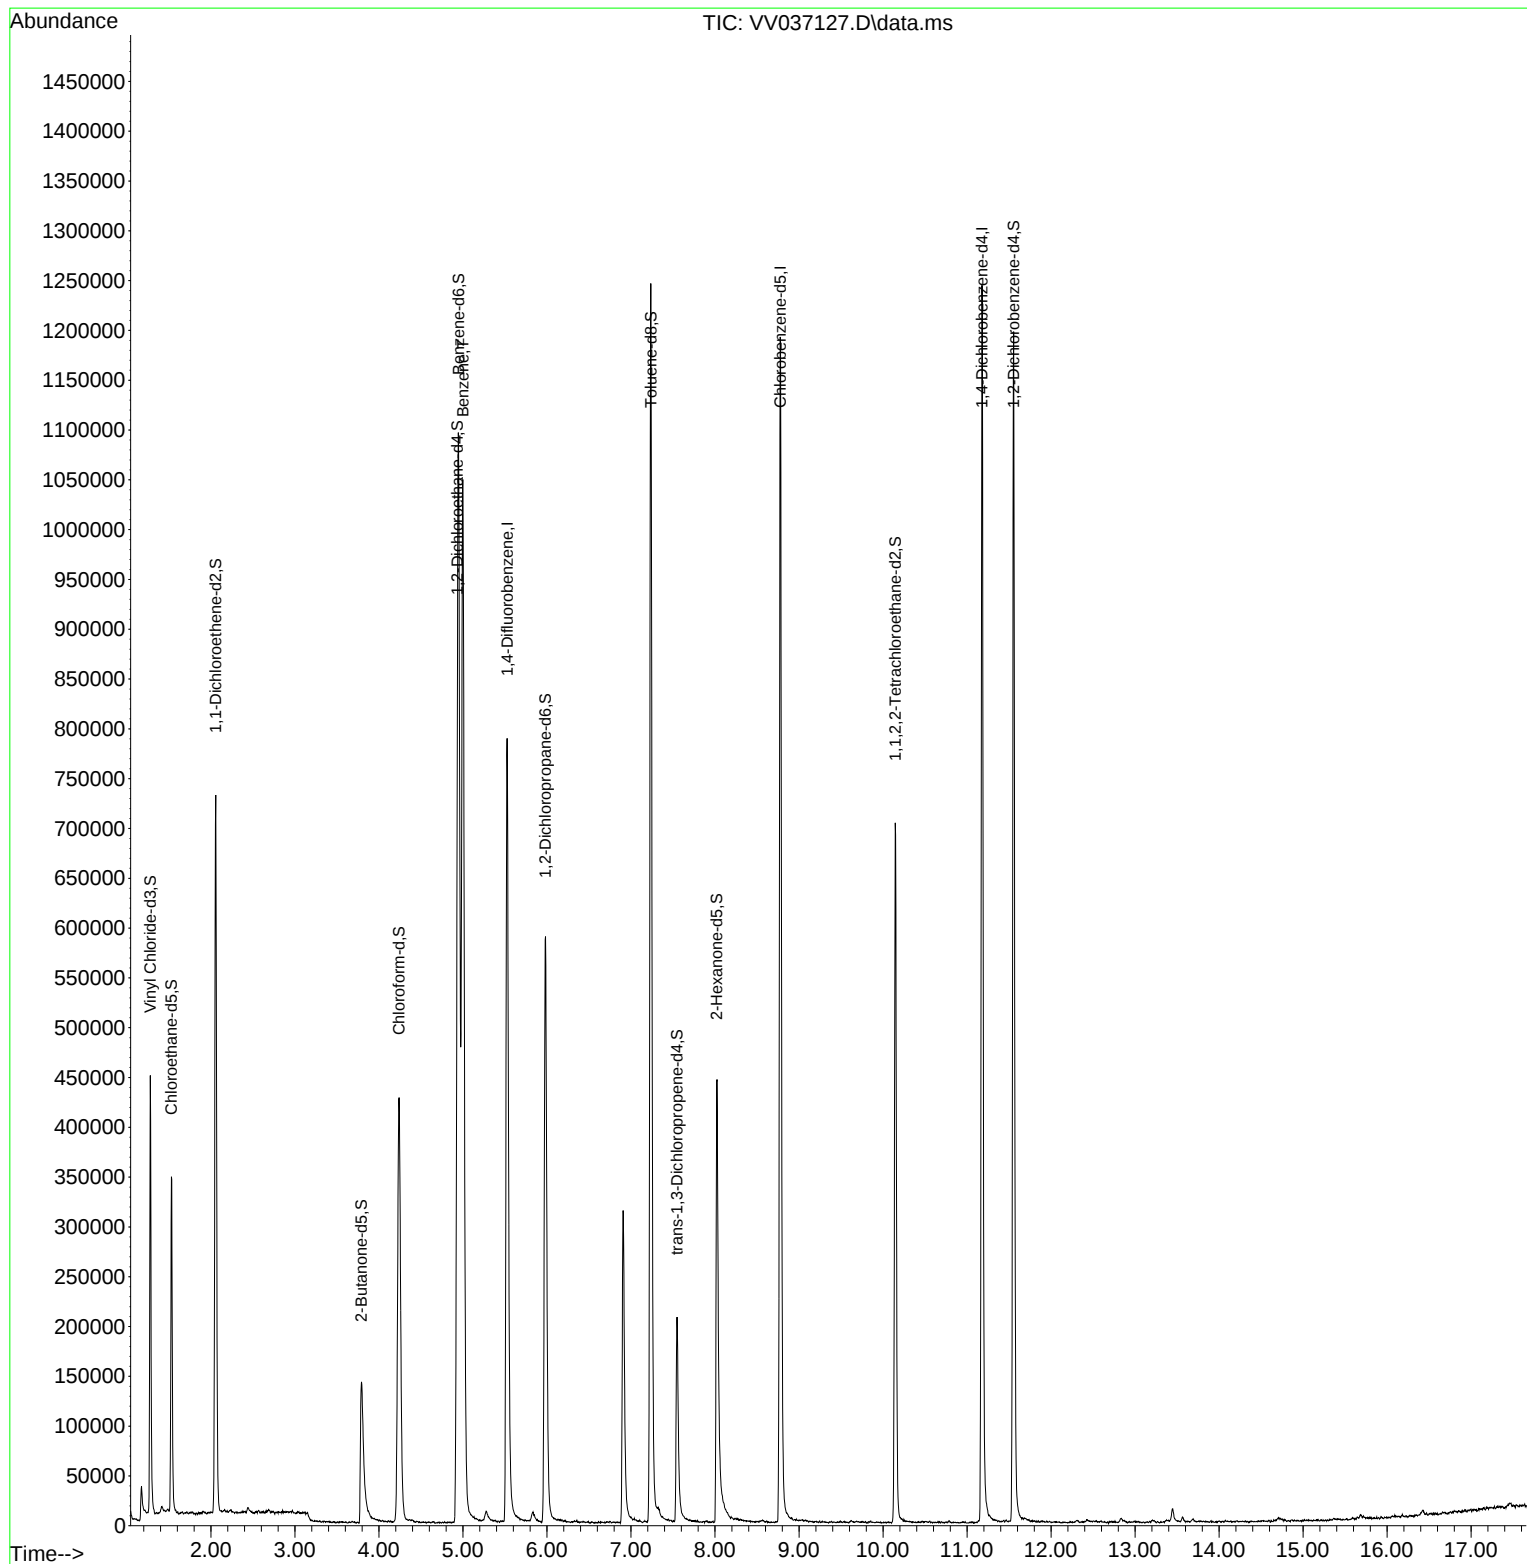

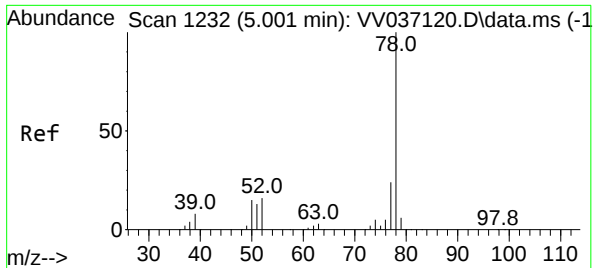

#33
Benzene
Concen: 57.070 ug/L
RT: 4.998 min Scan# 11
Delta R.T. -0.003 min
Lab File: VV037127.D
Acq: 28 Aug 2024 14:01

Instrument :
MSVOA_V
ClientSampleId :
E1K42DL

Tgt Ion: 78 Resp: 1069060

