

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037138.D
 Acq On : 28 Aug 2024 18:04
 Operator : SY/MD
 Sample : P3734-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B0

Quant Time: Aug 29 04:48:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 29 04:43:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	566508	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	554106	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	261956	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	251585	48.548	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.100%
7) Chloroethane-d5	1.532	69	200240	49.996	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.000%
11) 1,1-Dichloroethene-d2	2.056	65	109859	50.438	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.880%
21) 2-Butanone-d5	3.799	46	231750	115.482	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	115.480%
24) Chloroform-d	4.243	84	404526	49.876	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.760%
26) 1,2-Dichloroethane-d4	4.937	65	257883	50.490	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.980%
32) Benzene-d6	4.953	84	818396	48.900	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.800%
36) 1,2-Dichloropropane-d6	5.986	67	257241	49.073	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.140%
41) Toluene-d8	7.239	98	722384	47.826	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.660%
43) trans-1,3-Dichloroprop...	7.551	79	106567	43.942	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.880%
47) 2-Hexanone-d5	8.024	63	150254	105.026	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.030%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	322822	50.778	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.560%
66) 1,2-Dichlorobenzene-d4	11.558	152	264827	50.477	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.960%
Target Compounds						
					Qvalue	
13) Acetone	2.114	43	14841	6.896	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037138.D
Acq On : 28 Aug 2024 18:04
Operator : SY/MD
Sample : P3734-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44B0

Quant Time: Aug 29 04:48:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 29 04:43:38 2024
Response via : Initial Calibration

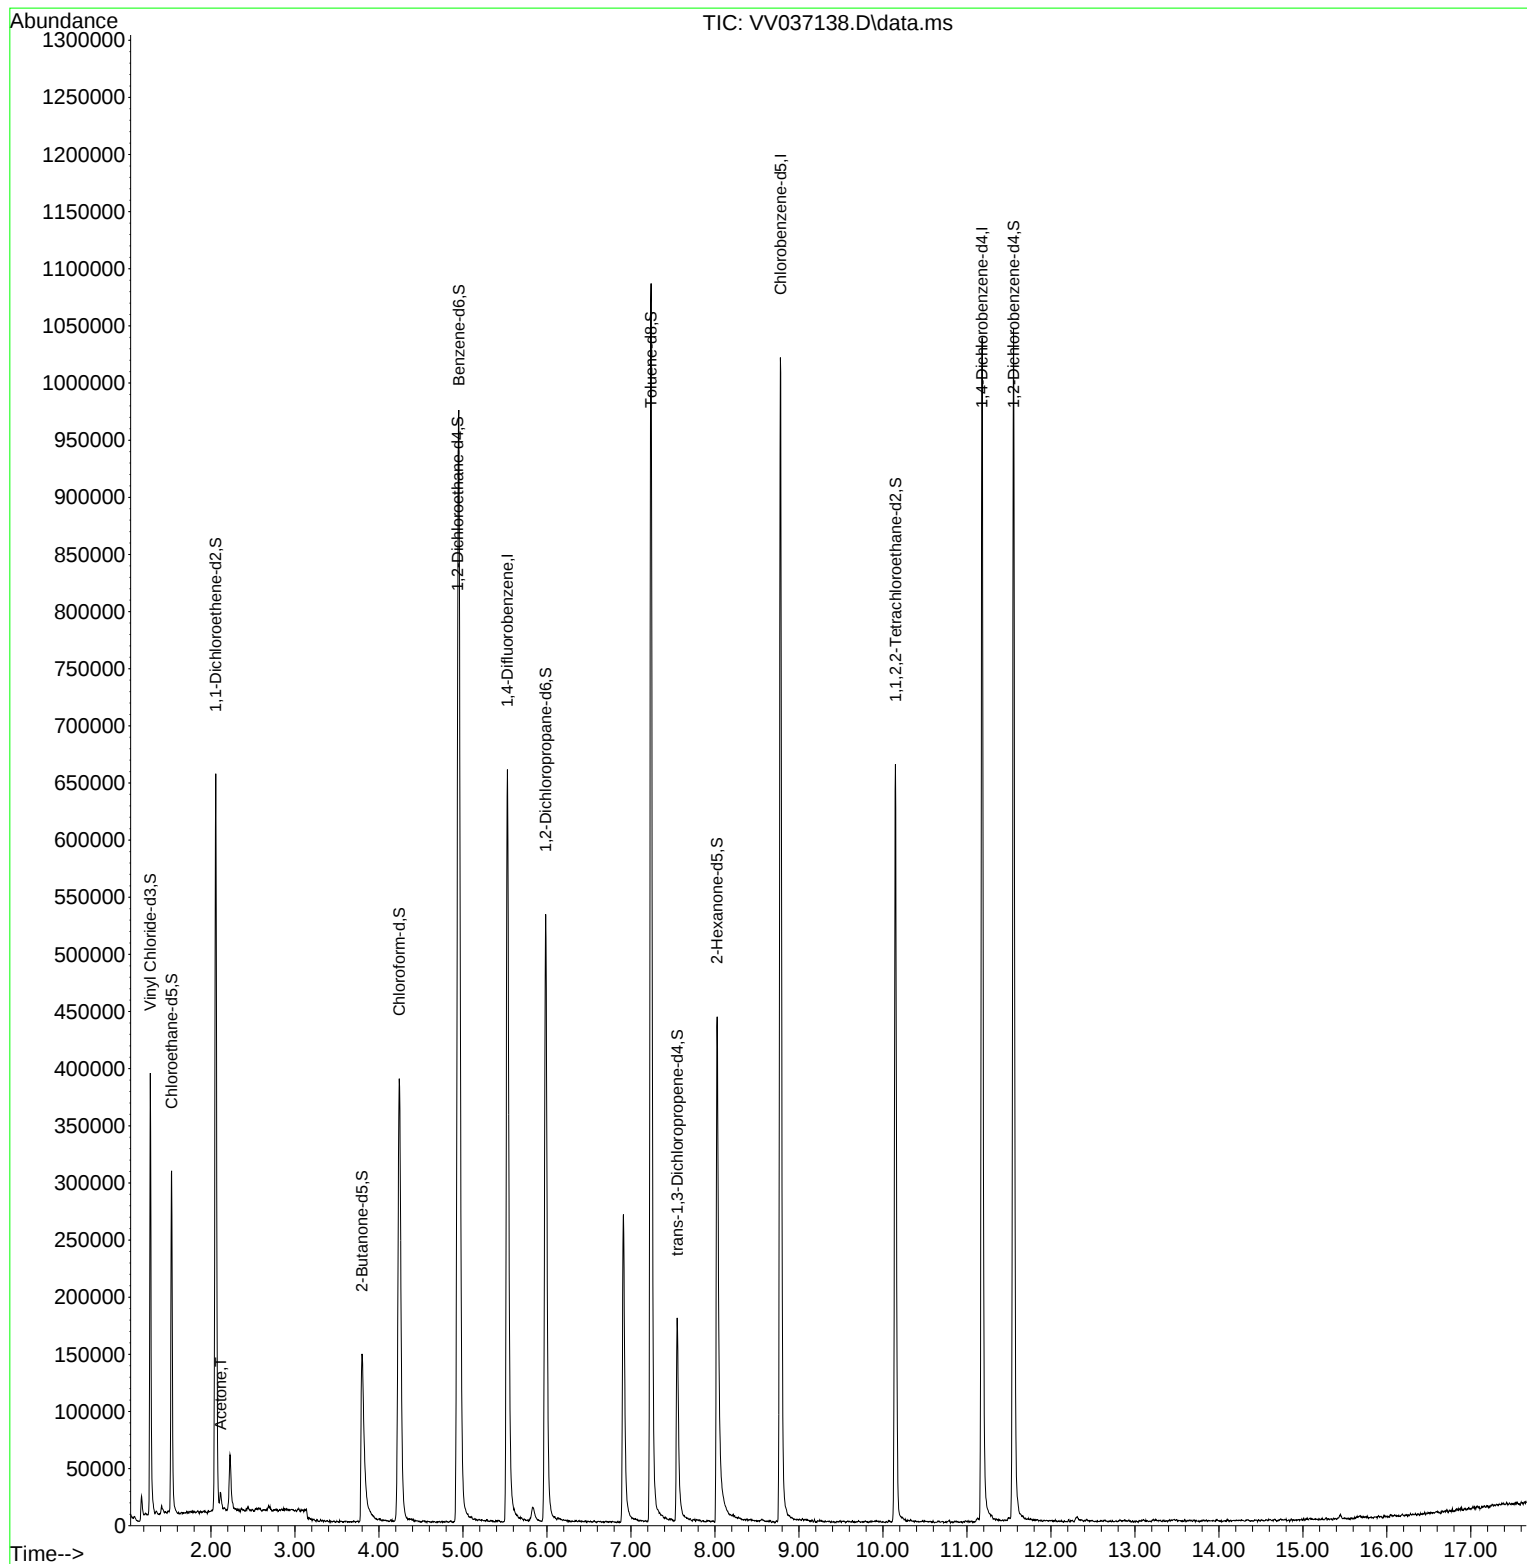

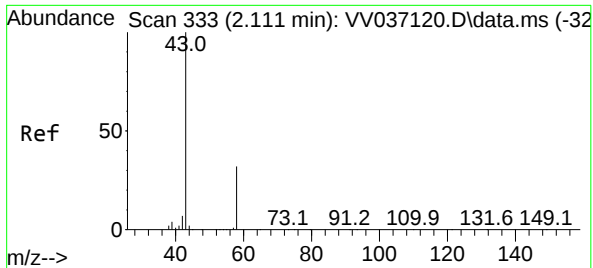

#13
 Acetone
 Concen: 6.896 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV037138.D
 Acq: 28 Aug 2024 18:04

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B0

Tgt Ion: 43 Resp: 14841
 Ion Ratio Lower Upper
 43 100
 58 35.4 0.0 64.8

