

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037139.D
 Acq On : 28 Aug 2024 18:26
 Operator : SY/MD
 Sample : P3734-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B1

Quant Time: Aug 29 04:48:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 29 04:43:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	569747	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	549671	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	254768	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	255389	49.002	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	98.000%
7) Chloroethane-d5	1.529	69	200984	49.897	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.800%
11) 1,1-Dichloroethene-d2	2.057	65	109737	50.096	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.200%
21) 2-Butanone-d5	3.799	46	230109	114.013	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	114.010%
24) Chloroform-d	4.243	84	409549	50.209	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.420%
26) 1,2-Dichloroethane-d4	4.937	65	261959	50.996	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.000%
32) Benzene-d6	4.954	84	826026	49.754	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.500%
36) 1,2-Dichloropropane-d6	5.986	67	266296	51.211	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.420%
41) Toluene-d8	7.240	98	732616	48.894	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.780%
43) trans-1,3-Dichloroprop...	7.551	79	108408	45.062	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.120%
47) 2-Hexanone-d5	8.024	63	150914	106.339	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	106.340%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	328240	52.047	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.100%
66) 1,2-Dichlorobenzene-d4	11.555	152	266300	52.190	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.380%
Target Compounds						
					Qvalue	
13) Acetone	2.114	43	16781	7.753	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037139.D
Acq On : 28 Aug 2024 18:26
Operator : SY/MD
Sample : P3734-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44B1

Quant Time: Aug 29 04:48:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 29 04:43:38 2024
Response via : Initial Calibration

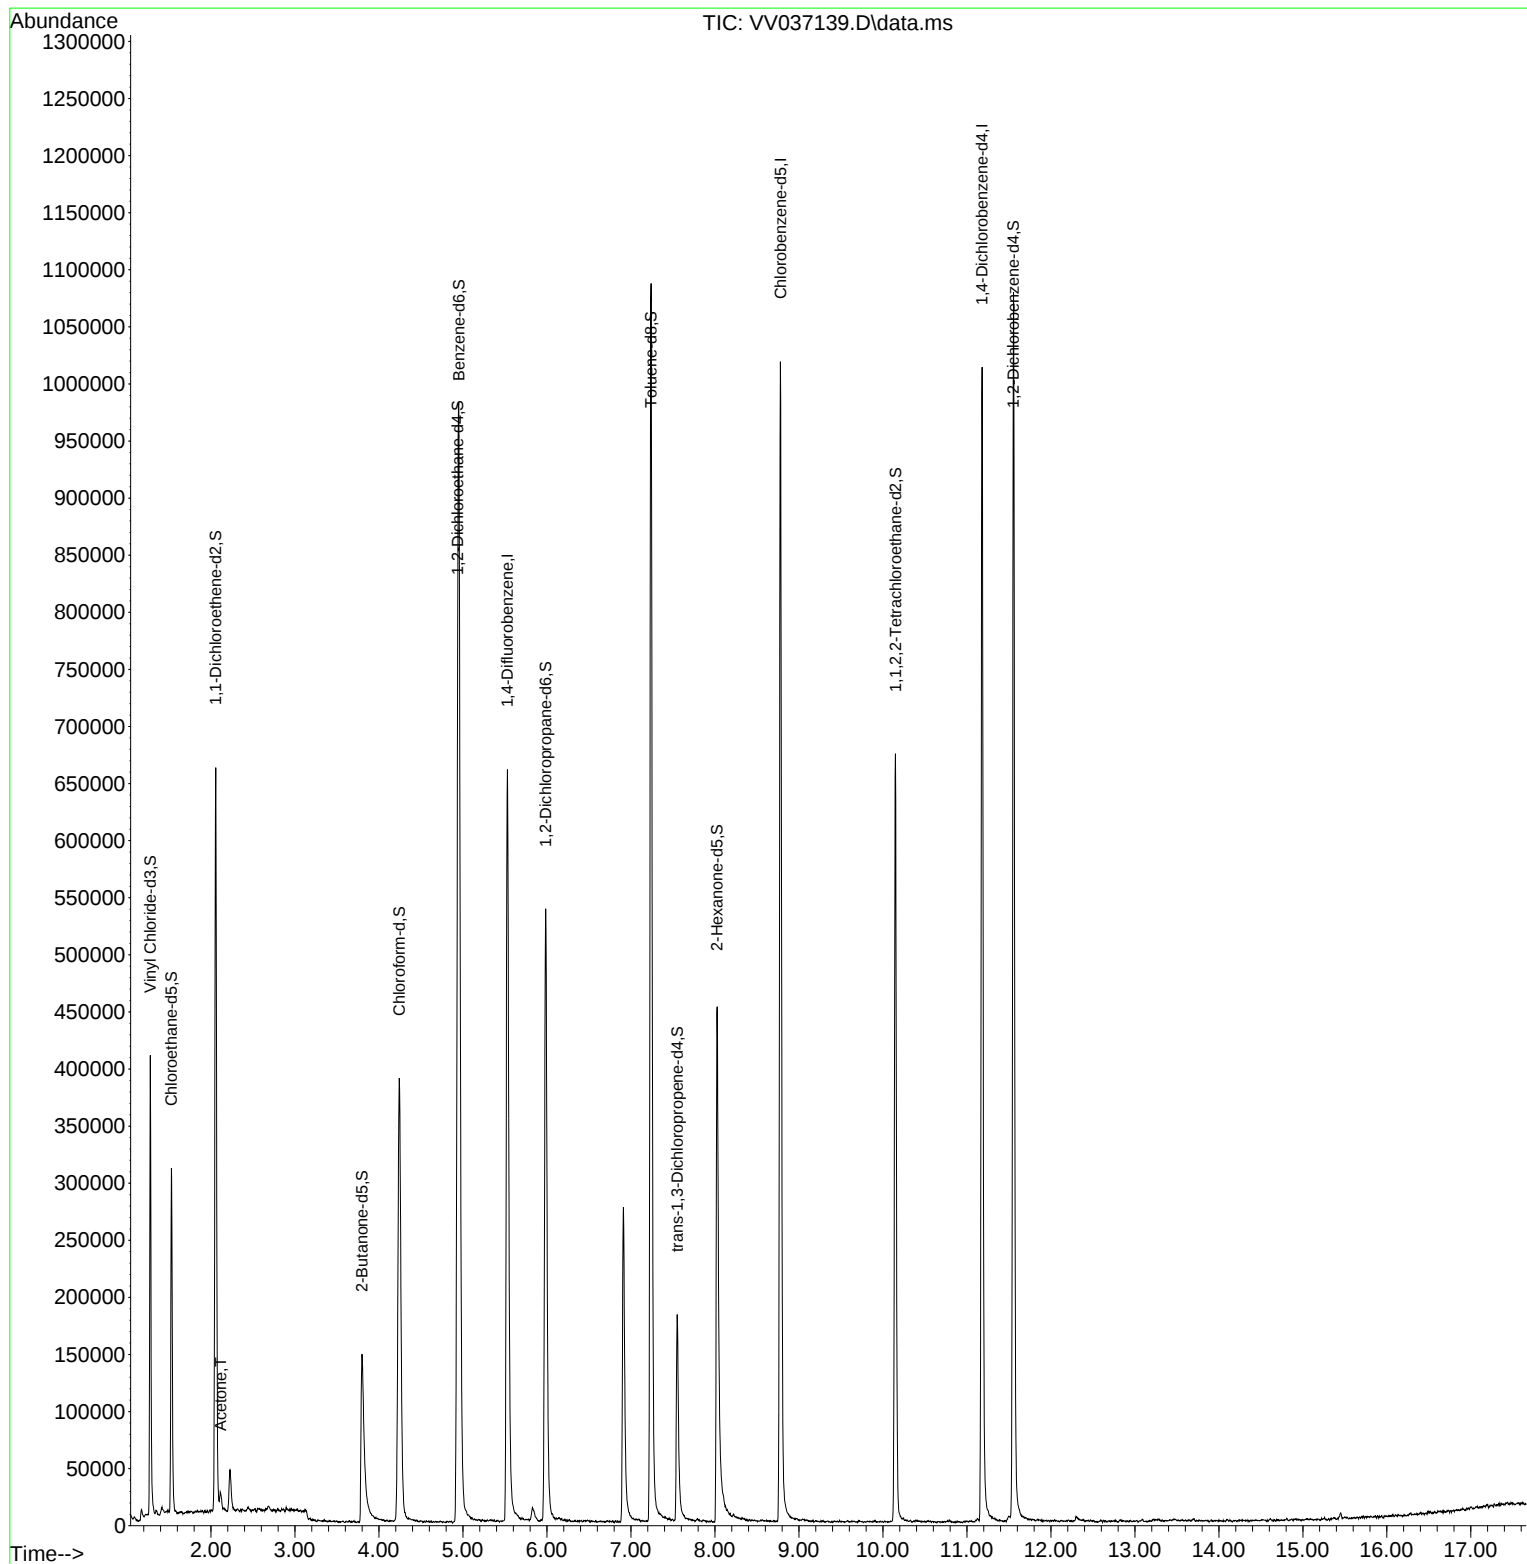

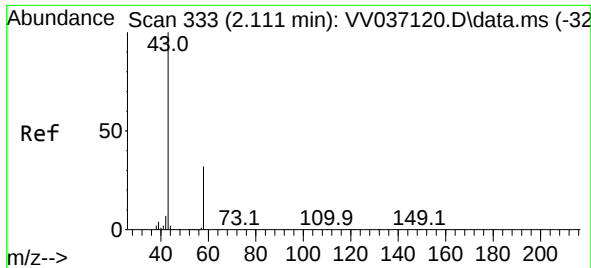

#13

Acetone

Concen: 7.753 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV037139.D

Acq: 28 Aug 2024 18:26

Instrument :

MSVOA_V

ClientSampleId :

A44B1

Tgt Ion: 43 Resp: 16781

Ion Ratio Lower Upper

43 100

58 32.1 0.0 64.8

