

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037135.D
Acq On : 28 Aug 2024 16:57
Operator : SY/MD
Sample : P3692-20DL 10X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	35	40	51	rBV	22379	37285	1.42%	0.180%
2	1.278	67	74	91	rVB	410612	453585	17.24%	2.189%
3	1.516	142	148	178	rVB	307289	404042	15.36%	1.950%
4	2.053	306	315	330	rVB	660562	945096	35.92%	4.560%
5	3.368	722	724	726	rBV2	986	515	0.02%	0.002%
6	3.584	788	791	794	rBV4	1032	620	0.02%	0.003%
7	3.616	799	801	803	rVB3	926	322	0.01%	0.002%
8	3.661	813	815	817	rBV3	671	378	0.01%	0.002%
9	3.748	840	842	843	rBV2	718	209	0.01%	0.001%
10	3.802	843	859	886	rBV2	1087624	2630852	100.00%	12.694%
11	4.240	978	995	1025	rBV	394025	1004535	38.18%	4.847%
12	4.519	1077	1082	1085	rBV5	1689	1699	0.06%	0.008%
13	4.709	1139	1141	1143	rBV3	843	396	0.02%	0.002%
14	4.719	1143	1144	1149	rBV4	800	563	0.02%	0.003%
15	4.744	1149	1152	1154	rVB4	1108	615	0.02%	0.003%
16	4.767	1158	1159	1160	rBV	1221	470	0.02%	0.002%
17	4.947	1200	1215	1246	rBV2	1021929	2511064	95.45%	12.116%
18	5.529	1384	1396	1426	rBV	674509	1401136	53.26%	6.761%
19	5.982	1526	1537	1564	rBV	544337	1113425	42.32%	5.372%
20	6.433	1675	1677	1680	rBV4	1091	665	0.03%	0.003%
21	6.519	1702	1704	1705	rBV2	792	318	0.01%	0.002%
22	6.851	1804	1807	1813	rBV8	1220	1339	0.05%	0.006%
23	6.908	1816	1825	1853	rVV	280464	538310	20.46%	2.597%
24	7.236	1916	1927	1952	rBV	1122833	1998559	75.97%	9.643%
25	7.551	2016	2025	2051	rBV	187500	347066	13.19%	1.675%
26	7.992	2160	2162	2163	rBV2	1050	411	0.02%	0.002%
27	8.024	2164	2172	2204	rBV	482162	936192	35.59%	4.517%
28	8.780	2396	2407	2433	rBV	1070641	1748764	66.47%	8.438%
29	9.178	2529	2531	2532	rBV2	1044	496	0.02%	0.002%
30	9.342	2581	2582	2583	rBV	712	220	0.01%	0.001%
31	9.410	2600	2603	2604	rBV3	873	427	0.02%	0.002%
32	9.529	2637	2640	2645	rBV6	1170	1066	0.04%	0.005%
33	9.715	2695	2698	2701	rBV4	654	408	0.02%	0.002%
34	9.741	2701	2706	2712	rVV7	1503	1650	0.06%	0.008%
35	9.764	2712	2713	2717	rVV4	1176	476	0.02%	0.002%
36	9.780	2717	2718	2722	rVB3	902	549	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037135.D
 Acq On : 28 Aug 2024 16:57
 Operator : SY/MD
 Sample : P3692-20DL 10X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.973	2776	2778	2782	rVB3	1222	783	0.03%	0.004%
38	10.034	2793	2797	2800	rBV6	953	725	0.03%	0.003%
39	10.047	2800	2801	2803	rBV2	845	395	0.02%	0.002%
40	10.092	2814	2815	2817	rBV2	601	252	0.01%	0.001%
41	10.149	2821	2833	2852	rBV	710391	1116736	42.45%	5.388%
42	10.294	2875	2878	2882	rBV6	1725	1154	0.04%	0.006%
43	10.423	2916	2918	2919	rBV	915	306	0.01%	0.001%
44	10.616	2976	2978	2981	rBV4	817	451	0.02%	0.002%
45	10.699	2999	3004	3005	rBV4	920	641	0.02%	0.003%
46	10.712	3005	3008	3014	rVB7	1164	1120	0.04%	0.005%
47	10.747	3014	3019	3021	rBV4	1353	1163	0.04%	0.006%
48	10.780	3027	3029	3030	rBV2	1037	525	0.02%	0.003%
49	10.825	3038	3043	3045	rBV5	1448	956	0.04%	0.005%
50	10.918	3068	3072	3075	rBV6	1191	1108	0.04%	0.005%
51	10.956	3079	3084	3087	rBV5	1160	1100	0.04%	0.005%
52	10.976	3087	3090	3092	rBV3	1217	653	0.02%	0.003%
53	11.056	3111	3115	3116	rBV4	876	691	0.03%	0.003%
54	11.182	3143	3154	3180	rBV	1073560	1706723	64.87%	8.235%
55	11.554	3259	3270	3301	rBV	1117127	1795423	68.24%	8.663%
56	11.854	3361	3363	3366	rBV4	1102	539	0.02%	0.003%
57	11.963	3391	3397	3400	rBV7	1282	1516	0.06%	0.007%
58	12.268	3489	3492	3495	rBV3	1452	995	0.04%	0.005%
59	12.300	3499	3502	3504	rBV3	839	554	0.02%	0.003%
60	12.323	3504	3509	3510	rBV4	995	770	0.03%	0.004%
61	12.345	3514	3516	3517	rBV2	706	246	0.01%	0.001%
62	12.355	3517	3519	3520	rBV2	709	233	0.01%	0.001%
63	12.458	3548	3551	3553	rBV4	1556	986	0.04%	0.005%
64	12.718	3630	3632	3634	rBV3	848	404	0.02%	0.002%
65	12.754	3642	3643	3646	rBV3	875	431	0.02%	0.002%
66	13.394	3840	3842	3845	rBV5	994	643	0.02%	0.003%
67	13.644	3918	3920	3921	rBV2	1127	511	0.02%	0.002%
68	13.802	3968	3969	3972	rBV3	1222	576	0.02%	0.003%
69	13.818	3972	3974	3977	rBV3	1063	695	0.03%	0.003%
70	14.239	4101	4105	4106	rBV4	1695	1011	0.04%	0.005%




Sum of corrected areas: 20724738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037135.D
Acq On : 28 Aug 2024 16:57
Operator : SY/MD
Sample : P3692-20DL 10X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

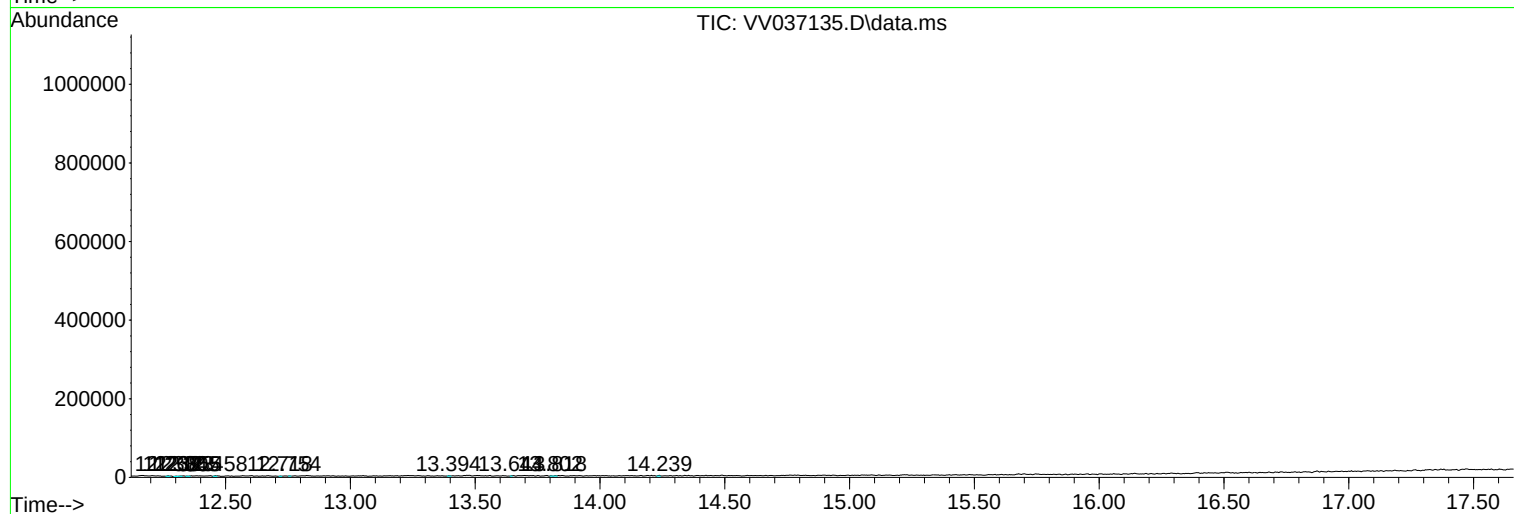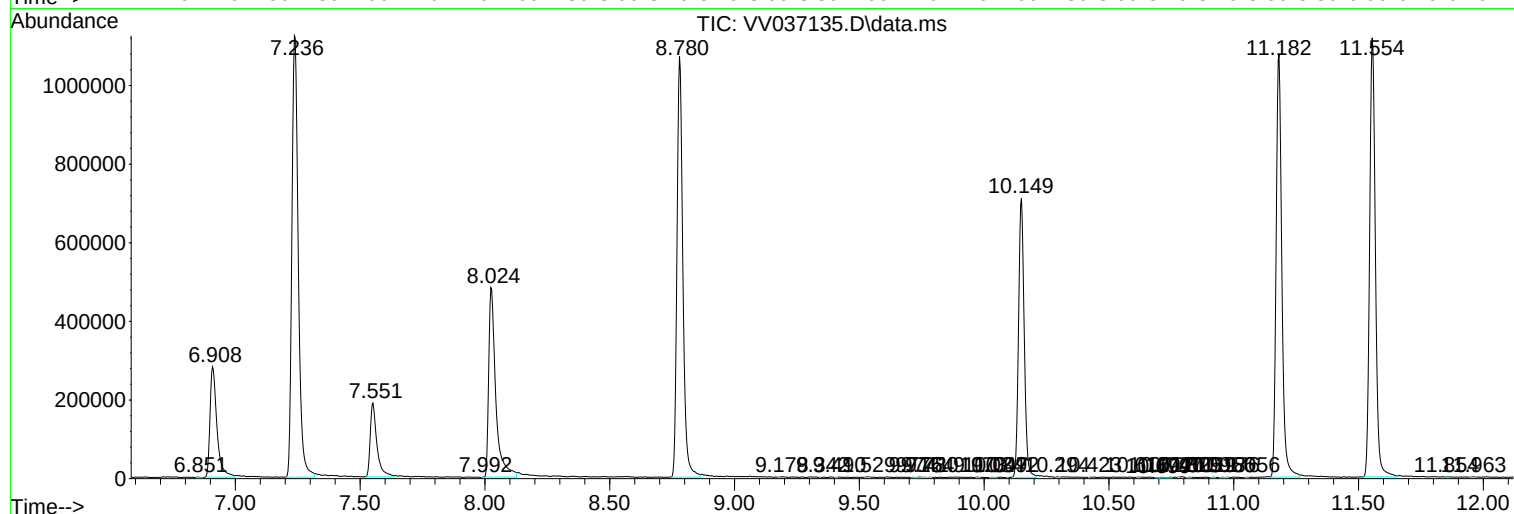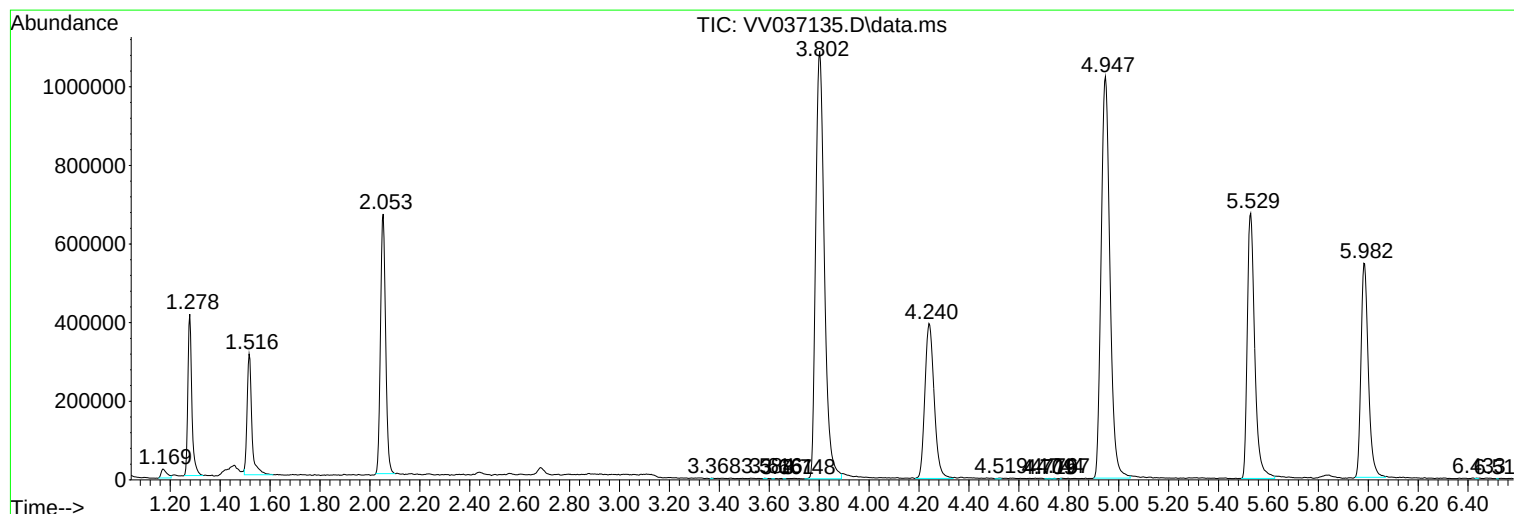

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037135.D
Acq On : 28 Aug 2024 16:57
Operator : SY/MD
Sample : P3692-20DL 10X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037135.D
Acq On : 28 Aug 2024 16:57
Operator : SY/MD
Sample : P3692-20DL 10X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc