

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037136.D
 Acq On : 28 Aug 2024 17:19
 Operator : SY/MD
 Sample : P3692-21DL 20X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K81DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	50	rBV	15319	23242	0.91%	0.118%
2	1.278	68	74	95	rVB	416702	444629	17.48%	2.256%
3	1.529	146	152	167	rVB	304588	370427	14.56%	1.880%
4	2.056	307	316	337	rVB	661481	956851	37.62%	4.855%
5	3.310	703	706	709	rVB3	1629	1060	0.04%	0.005%
6	3.326	709	711	715	rBV3	1551	1386	0.05%	0.007%
7	3.468	753	755	757	rBV3	1111	474	0.02%	0.002%
8	3.519	768	771	775	rBV5	1511	1282	0.05%	0.007%
9	3.757	841	845	846	rBV3	1058	635	0.02%	0.003%
10	3.806	846	860	898	rBV3	608108	1564368	61.50%	7.938%
11	4.246	982	997	1025	rVB2	397129	993345	39.05%	5.041%
12	4.561	1094	1095	1099	rVB3	1579	734	0.03%	0.004%
13	4.622	1112	1114	1120	rBV5	1644	1393	0.05%	0.007%
14	4.802	1164	1170	1174	rBV6	2110	1783	0.07%	0.009%
15	4.822	1174	1176	1177	rBV	636	335	0.01%	0.002%
16	4.851	1182	1185	1188	rVB4	1464	916	0.04%	0.005%
17	4.867	1188	1190	1194	rVB5	1423	752	0.03%	0.004%
18	4.896	1194	1199	1200	rBV4	937	726	0.03%	0.004%
19	4.950	1200	1216	1246	rBV2	1026419	2543734	100.00%	12.908%
20	5.301	1323	1325	1328	rBV4	1696	1181	0.05%	0.006%
21	5.432	1365	1366	1369	rVB2	1051	349	0.01%	0.002%
22	5.490	1382	1384	1385	rBV2	1336	480	0.02%	0.002%
23	5.529	1385	1396	1427	rVV	684247	1427642	56.12%	7.244%
24	5.986	1526	1538	1572	rBV	553126	1139443	44.79%	5.782%
25	6.384	1660	1662	1664	rBV3	949	414	0.02%	0.002%
26	6.471	1687	1689	1692	rBV5	1355	826	0.03%	0.004%
27	6.551	1712	1714	1716	rBV3	759	509	0.02%	0.003%
28	6.638	1737	1741	1743	rBV4	905	730	0.03%	0.004%
29	6.715	1761	1765	1767	rBV4	852	621	0.02%	0.003%
30	6.770	1779	1782	1785	rVB6	833	520	0.02%	0.003%
31	6.805	1788	1793	1795	rBV5	1533	1510	0.06%	0.008%
32	6.912	1814	1826	1857	rVV	286469	554114	21.78%	2.812%
33	7.239	1916	1928	1961	rBV	1145532	2028095	79.73%	10.291%
34	7.551	2016	2025	2047	rBV	192414	346635	13.63%	1.759%
35	8.027	2163	2173	2216	rBV	467484	949902	37.34%	4.820%
36	8.474	2311	2312	2314	rBV2	958	496	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037136.D
 Acq On : 28 Aug 2024 17:19
 Operator : SY/MD
 Sample : P3692-21DL 20X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K81DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.728	2389	2391	2395	rBV5	949	544	0.02%	0.003%
38	8.780	2396	2407	2430	rBV	1072538	1759293	69.16%	8.927%
39	9.384	2592	2595	2598	rBV4	1582	979	0.04%	0.005%
40	9.493	2624	2629	2631	rBV6	1165	979	0.04%	0.005%
41	9.551	2642	2647	2649	rBV6	1398	1109	0.04%	0.006%
42	9.574	2651	2654	2657	rVB3	1490	915	0.04%	0.005%
43	9.596	2657	2661	2664	rBV4	1360	1330	0.05%	0.007%
44	9.657	2677	2680	2682	rBV3	1084	543	0.02%	0.003%
45	9.702	2692	2694	2696	rVB3	1067	532	0.02%	0.003%
46	9.728	2699	2702	2705	rBV6	1443	1128	0.04%	0.006%
47	9.789	2718	2721	2722	rBV2	1243	803	0.03%	0.004%
48	9.812	2726	2728	2730	rBV2	779	353	0.01%	0.002%
49	9.821	2730	2731	2734	rBV3	863	534	0.02%	0.003%
50	9.870	2741	2746	2750	rBV5	1949	2011	0.08%	0.010%
51	9.908	2756	2758	2759	rBV2	859	394	0.02%	0.002%
52	9.979	2775	2780	2784	rVV6	1774	1516	0.06%	0.008%
53	10.018	2789	2792	2797	rVB6	872	733	0.03%	0.004%
54	10.108	2816	2820	2821	rBV3	693	503	0.02%	0.003%
55	10.149	2821	2833	2856	rBV	684120	1096279	43.10%	5.563%
56	10.448	2924	2926	2928	rBV3	668	336	0.01%	0.002%
57	10.603	2971	2974	2977	rBV4	992	707	0.03%	0.004%
58	10.728	3010	3013	3014	rVB3	830	376	0.01%	0.002%
59	10.780	3025	3029	3031	rBV3	2149	1708	0.07%	0.009%
60	10.812	3037	3039	3042	rBV4	988	664	0.03%	0.003%
61	10.834	3045	3046	3048	rVB2	1055	397	0.02%	0.002%
62	10.866	3054	3056	3059	rBV3	704	351	0.01%	0.002%
63	10.924	3068	3074	3077	rVB4	1399	1154	0.05%	0.006%
64	10.940	3077	3079	3084	rVB6	1444	940	0.04%	0.005%
65	10.966	3084	3087	3088	rBV3	553	390	0.02%	0.002%
66	11.014	3100	3102	3105	rVB3	1323	812	0.03%	0.004%
67	11.181	3143	3154	3185	rBV	1069865	1696172	66.68%	8.607%
68	11.554	3258	3270	3295	rBV	1107827	1747396	68.69%	8.867%
69	11.937	3387	3389	3392	rBV4	1206	599	0.02%	0.003%
70	11.966	3396	3398	3400	rBV3	1434	743	0.03%	0.004%
71	12.027	3415	3417	3421	rVB6	1367	979	0.04%	0.005%
72	12.043	3421	3422	3424	rBV2	841	387	0.02%	0.002%
73	12.069	3427	3430	3433	rBV5	903	746	0.03%	0.004%
74	12.217	3474	3476	3478	rVB3	1057	440	0.02%	0.002%
75	12.233	3478	3481	3482	rVV3	776	421	0.02%	0.002%
76	12.246	3483	3485	3489	rVB3	1006	628	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037136.D
 Acq On : 28 Aug 2024 17:19
 Operator : SY/MD
 Sample : P3692-21DL 20X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K81DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	12.323	3507	3509	3511	rBV3	1291	752	0.03%	0.004%
78	12.349	3514	3517	3518	rBV2	1243	755	0.03%	0.004%
79	12.464	3551	3553	3555	rBV2	1161	620	0.02%	0.003%
80	12.538	3573	3576	3578	rBV3	947	709	0.03%	0.004%
81	12.554	3578	3581	3583	rVV3	797	522	0.02%	0.003%
82	12.648	3608	3610	3614	rBV6	1189	904	0.04%	0.005%
83	12.718	3628	3632	3633	rBV4	751	525	0.02%	0.003%
84	12.760	3643	3645	3648	rVB3	973	504	0.02%	0.003%
85	12.805	3657	3659	3661	rVB3	1228	488	0.02%	0.002%
86	12.892	3683	3686	3688	rBV3	1334	863	0.03%	0.004%
87	12.921	3693	3695	3696	rBV2	733	398	0.02%	0.002%
88	13.088	3744	3747	3750	rBV5	1697	1126	0.04%	0.006%
89	13.210	3783	3785	3790	rBV5	1413	1083	0.04%	0.005%
90	13.320	3817	3819	3820	rBV	1213	495	0.02%	0.003%
91	13.400	3842	3844	3846	rBV3	740	410	0.02%	0.002%
92	13.458	3858	3862	3865	rVB6	1733	1309	0.05%	0.007%
93	13.599	3902	3906	3911	rVB7	2103	1776	0.07%	0.009%
94	13.651	3920	3922	3928	rBV7	961	678	0.03%	0.003%
95	13.818	3972	3974	3979	rBV6	1293	971	0.04%	0.005%
96	13.876	3989	3992	3993	rBV3	1100	712	0.03%	0.004%
97	13.947	4012	4014	4016	rBV3	971	520	0.02%	0.003%
98	13.995	4027	4029	4033	rVB5	1334	978	0.04%	0.005%
99	14.017	4033	4036	4039	rBV4	1168	781	0.03%	0.004%
100	14.641	4228	4230	4232	rBV2	1471	882	0.03%	0.004%




Sum of corrected areas: 19707124

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037136.D
Acq On : 28 Aug 2024 17:19
Operator : SY/MD
Sample : P3692-21DL 20X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K81DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

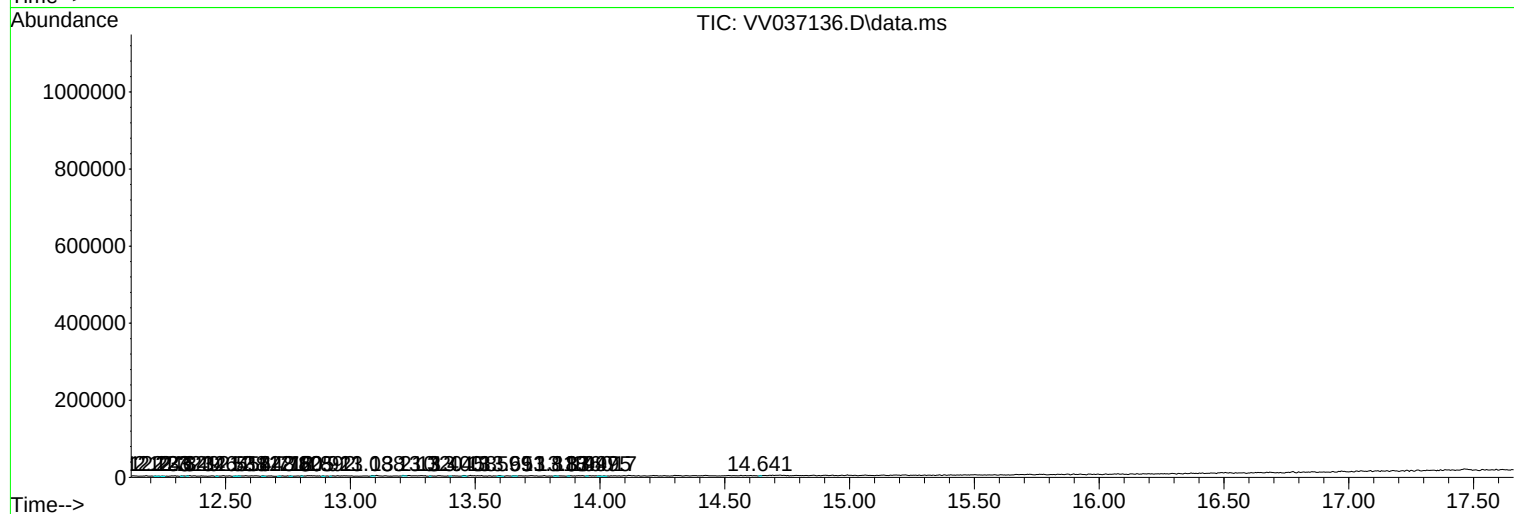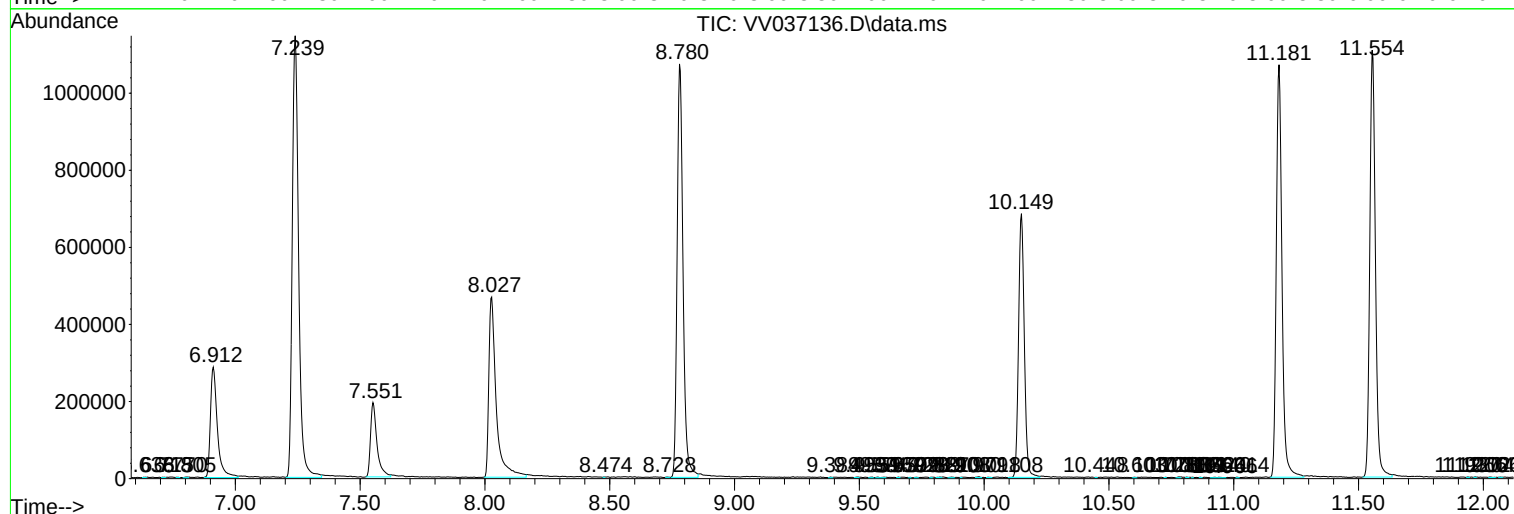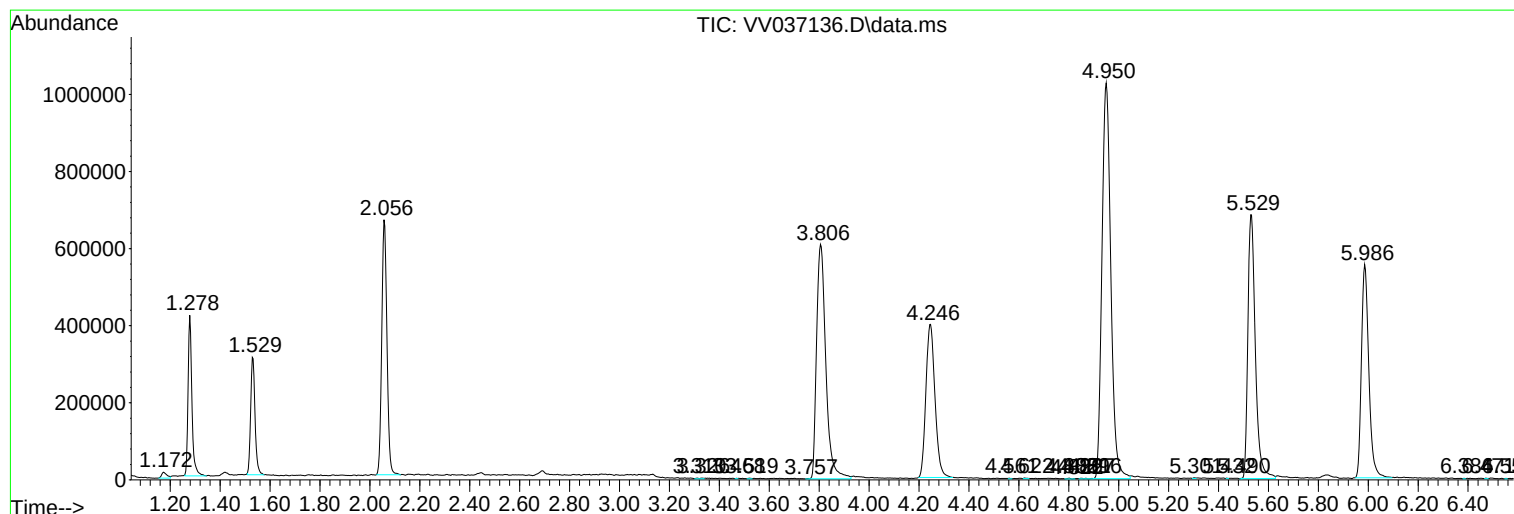

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037136.D
Acq On : 28 Aug 2024 17:19
Operator : SY/MD
Sample : P3692-21DL 20X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K81DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037136.D
Acq On : 28 Aug 2024 17:19
Operator : SY/MD
Sample : P3692-21DL 20X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K81DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------