

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037137.D
 Acq On : 28 Aug 2024 17:42
 Operator : SY/MD
 Sample : P3692-16DL 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K65DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	36	41	50	rBV	8794	13605	0.53%	0.062%
2	1.278	67	74	94	rBV2	434114	468800	18.38%	2.140%
3	1.532	145	153	169	rVB	307227	371421	14.56%	1.696%
4	2.056	307	316	332	rVB	652884	929813	36.46%	4.245%
5	3.326	709	711	715	rBV4	1209	1071	0.04%	0.005%
6	3.516	765	770	774	rBV5	1784	2284	0.09%	0.010%
7	3.571	784	787	789	rBV4	1538	1074	0.04%	0.005%
8	3.648	808	811	813	rBV3	1446	882	0.03%	0.004%
9	3.748	841	842	845	rVB2	656	308	0.01%	0.001%
10	3.805	845	860	894	rBV2	1029713	2550461	100.00%	11.644%
11	4.243	982	996	1022	rBV	389113	971597	38.09%	4.436%
12	4.629	1114	1116	1118	rBV3	1300	453	0.02%	0.002%
13	4.757	1154	1156	1160	rBV5	1177	1084	0.04%	0.005%
14	4.789	1164	1166	1168	rVB4	982	385	0.02%	0.002%
15	4.818	1173	1175	1179	rVB5	981	569	0.02%	0.003%
16	4.950	1200	1216	1254	rBV2	999803	2511724	98.48%	11.467%
17	5.442	1365	1369	1371	rBV4	1347	1080	0.04%	0.005%
18	5.529	1385	1396	1432	rBV	654231	1343582	52.68%	6.134%
19	5.828	1477	1489	1515	rBV2	833669	1675379	65.69%	7.649%
20	5.985	1527	1538	1570	rVB	550257	1123101	44.04%	5.128%
21	6.397	1661	1666	1668	rBV6	1818	1611	0.06%	0.007%
22	6.519	1700	1704	1706	rBV5	1530	1055	0.04%	0.005%
23	6.590	1720	1726	1728	rBV6	1272	1326	0.05%	0.006%
24	6.706	1759	1762	1764	rBV4	1606	918	0.04%	0.004%
25	6.747	1773	1775	1777	rBV3	1131	615	0.02%	0.003%
26	6.805	1789	1793	1795	rBV5	1265	1068	0.04%	0.005%
27	6.911	1815	1826	1852	rBV	285254	547679	21.47%	2.500%
28	7.156	1900	1902	1906	rBV5	1548	1064	0.04%	0.005%
29	7.239	1916	1928	1957	rBV	1115980	1968285	77.17%	8.986%
30	7.551	2016	2025	2054	rBV	185557	344760	13.52%	1.574%
31	7.776	2092	2095	2099	rBV4	1514	1169	0.05%	0.005%
32	7.899	2131	2133	2136	rBV3	1652	771	0.03%	0.004%
33	7.972	2153	2156	2161	rBV7	1761	1163	0.05%	0.005%
34	8.027	2163	2173	2211	rBV	470690	955831	37.48%	4.364%
35	8.661	2368	2370	2371	rBV2	1197	349	0.01%	0.002%
36	8.734	2390	2393	2395	rVB3	1495	842	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037137.D
 Acq On : 28 Aug 2024 17:42
 Operator : SY/MD
 Sample : P3692-16DL 200X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K65DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.780	2396	2407	2435	rBV	1001499	1653974	64.85%	7.551%
38	9.529	2636	2640	2642	rBV5	1556	1210	0.05%	0.006%
39	9.567	2650	2652	2655	rBV4	793	483	0.02%	0.002%
40	9.689	2688	2690	2692	rBV2	806	403	0.02%	0.002%
41	9.744	2704	2707	2709	rBV3	1104	628	0.02%	0.003%
42	9.773	2714	2716	2720	rVB5	990	704	0.03%	0.003%
43	9.802	2720	2725	2726	rBV5	1731	1209	0.05%	0.006%
44	9.850	2737	2740	2743	rBV4	596	567	0.02%	0.003%
45	9.960	2772	2774	2776	rBV2	1597	862	0.03%	0.004%
46	9.979	2778	2780	2783	rVV4	1082	720	0.03%	0.003%
47	10.062	2802	2806	2807	rBV3	776	418	0.02%	0.002%
48	10.078	2808	2811	2815	rVB5	1736	1318	0.05%	0.006%
49	10.104	2815	2819	2821	rBV4	905	728	0.03%	0.003%
50	10.149	2821	2833	2855	rBV	692372	1106034	43.37%	5.050%
51	10.371	2899	2902	2907	rBV5	1620	2029	0.08%	0.009%
52	10.464	2928	2931	2932	rBV3	1318	818	0.03%	0.004%
53	10.548	2954	2957	2961	rBV6	1168	936	0.04%	0.004%
54	10.660	2990	2992	2996	rBV3	1082	653	0.03%	0.003%
55	10.709	3002	3007	3009	rBV4	1585	1258	0.05%	0.006%
56	10.796	3033	3034	3039	rBV5	874	467	0.02%	0.002%
57	10.889	3060	3063	3069	rVB7	996	781	0.03%	0.004%
58	10.914	3069	3071	3076	rBV5	1084	1000	0.04%	0.005%
59	11.033	3105	3108	3110	rBV4	2495	1343	0.05%	0.006%
60	11.133	3134	3139	3141	rBV6	2205	1689	0.07%	0.008%
61	11.181	3144	3154	3186	rVV	987465	1576737	61.82%	7.199%
62	11.554	3259	3270	3297	rBV	1069834	1732639	67.93%	7.910%
63	11.747	3327	3330	3331	rBV2	1938	849	0.03%	0.004%
64	12.104	3438	3441	3444	rVB5	1218	881	0.03%	0.004%
65	12.146	3453	3454	3457	rBV3	737	270	0.01%	0.001%
66	12.162	3457	3459	3462	rVB4	1371	734	0.03%	0.003%
67	12.287	3494	3498	3500	rBV3	905	701	0.03%	0.003%
68	12.313	3503	3506	3509	rBV4	1284	888	0.03%	0.004%
69	12.503	3562	3565	3568	rBV5	1361	840	0.03%	0.004%
70	12.564	3581	3584	3585	rBV3	1238	689	0.03%	0.003%
71	12.654	3609	3612	3614	rVB4	839	485	0.02%	0.002%
72	12.670	3614	3617	3618	rBV4	750	340	0.01%	0.002%
73	12.741	3637	3639	3644	rBV5	1090	1033	0.04%	0.005%
74	12.808	3657	3660	3666	rBV6	1668	1487	0.06%	0.007%
75	12.837	3666	3669	3673	rBV4	1627	1150	0.05%	0.005%
76	13.062	3735	3739	3742	rBV6	1488	1281	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037137.D
Acq On : 28 Aug 2024 17:42
Operator : SY/MD
Sample : P3692-16DL 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K65DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	13.078	3742	3744	3747	rBV3	837	549	0.02%	0.003%
78	13.104	3750	3752	3754	rBV3	796	411	0.02%	0.002%
79	13.358	3829	3831	3833	rBV3	797	413	0.02%	0.002%
80	13.561	3893	3894	3895	rBV	1138	436	0.02%	0.002%
81	13.776	3959	3961	3964	rBV3	1162	534	0.02%	0.002%
82	13.837	3978	3980	3984	rBV5	1351	972	0.04%	0.004%
83	13.927	4006	4008	4010	rBV3	930	407	0.02%	0.002%
84	14.117	4065	4067	4068	rBV2	1200	486	0.02%	0.002%
85	14.310	4125	4127	4130	rBV3	1056	616	0.02%	0.003%




Sum of corrected areas: 21903239

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037137.D
Acq On : 28 Aug 2024 17:42
Operator : SY/MD
Sample : P3692-16DL 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K65DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

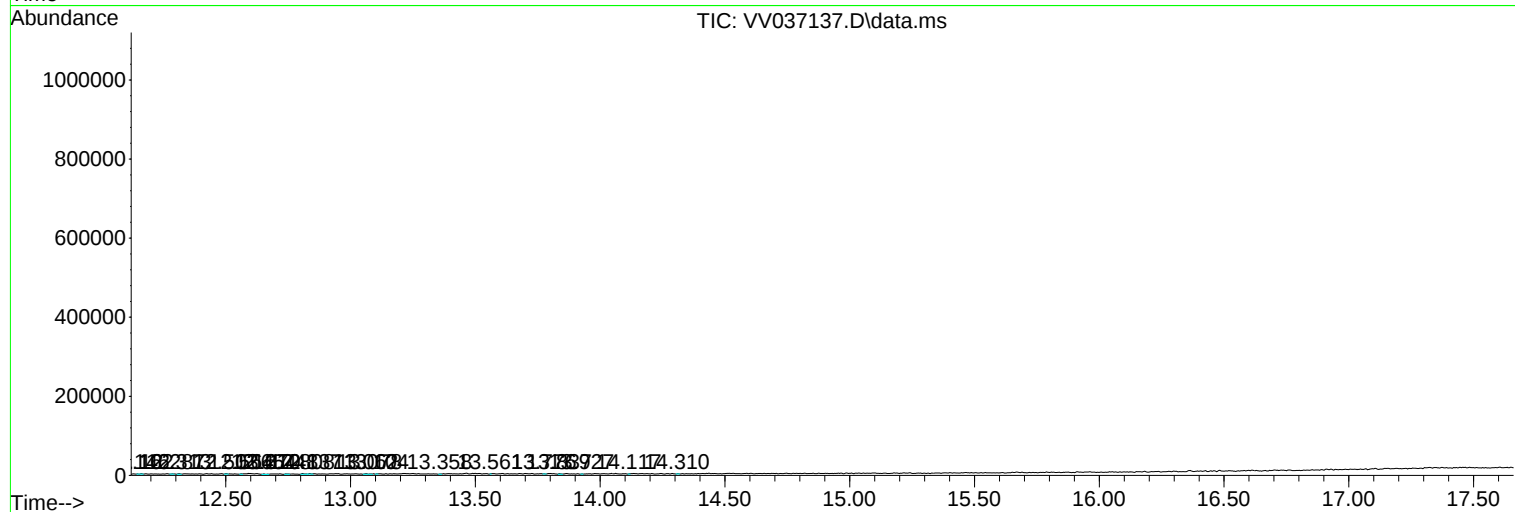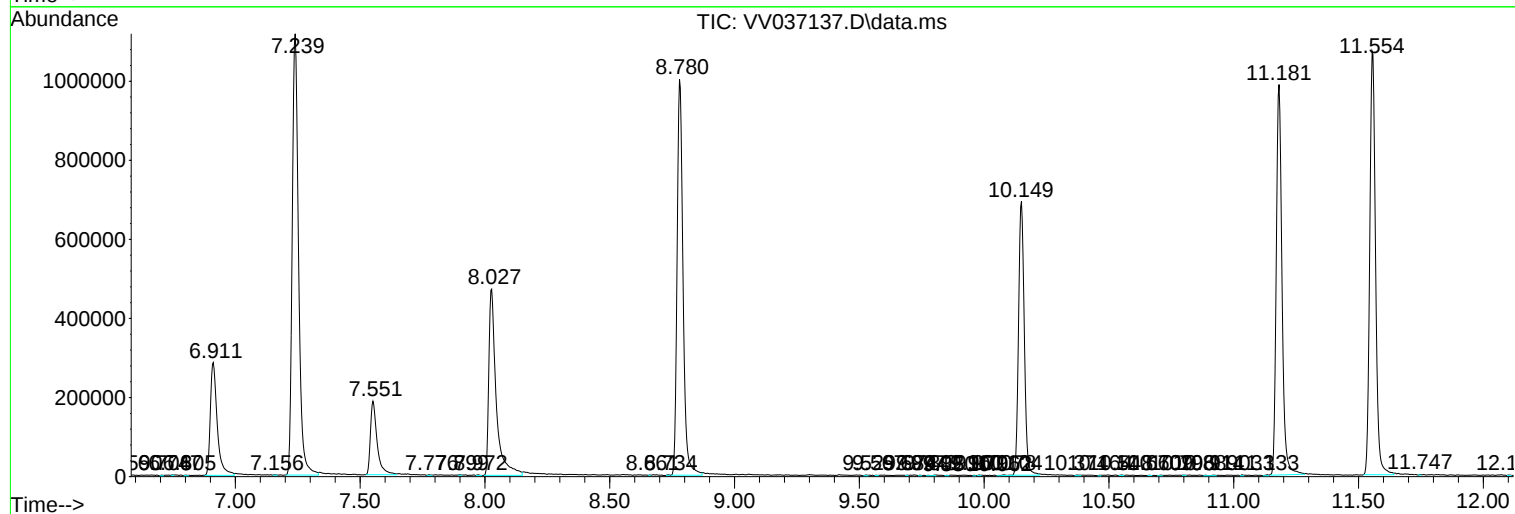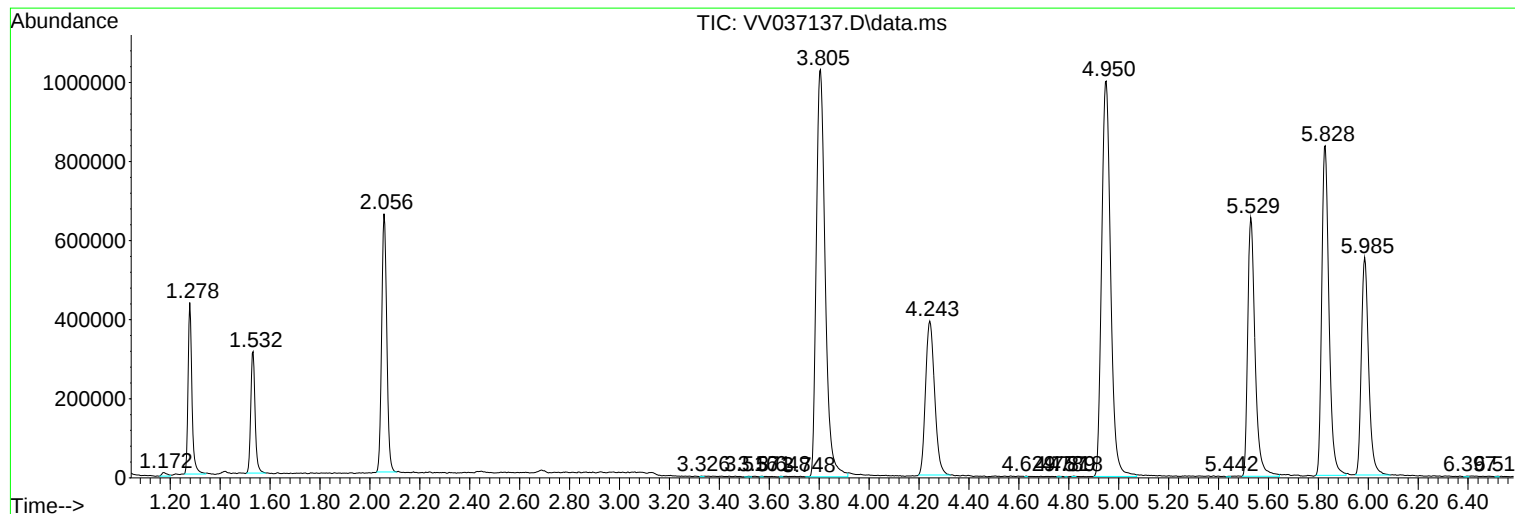

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037137.D
Acq On : 28 Aug 2024 17:42
Operator : SY/MD
Sample : P3692-16DL 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K65DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037137.D
Acq On : 28 Aug 2024 17:42
Operator : SY/MD
Sample : P3692-16DL 200X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K65DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc