

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037138.D
 Acq On : 28 Aug 2024 18:04
 Operator : SY/MD
 Sample : P3734-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037138.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	50	rBV	22072	31520	1.30%	0.177%
2	1.278	68	74	91	rVB	385490	403575	16.69%	2.270%
3	1.532	146	153	175	rVB	299873	365861	15.13%	2.058%
4	2.056	307	316	329	rBV	641565	904407	37.40%	5.087%
5	3.349	715	718	722	rBV5	1442	1243	0.05%	0.007%
6	3.413	736	738	742	rVB3	1739	1095	0.05%	0.006%
7	3.436	742	745	748	rBV5	913	768	0.03%	0.004%
8	3.532	774	775	779	rVV4	1500	712	0.03%	0.004%
9	3.658	811	814	819	rBV4	748	808	0.03%	0.005%
10	3.703	826	828	833	rVB4	1191	761	0.03%	0.004%
11	3.738	835	839	840	rBV4	832	642	0.03%	0.004%
12	3.799	849	858	895	rBV	146507	409041	16.92%	2.301%
13	4.243	980	996	1023	rBV	386734	967148	40.00%	5.440%
14	4.580	1098	1101	1103	rBV3	1032	817	0.03%	0.005%
15	4.632	1114	1117	1118	rBV3	1179	656	0.03%	0.004%
16	4.690	1132	1135	1136	rBV2	855	549	0.02%	0.003%
17	4.709	1138	1141	1143	rBV4	916	643	0.03%	0.004%
18	4.722	1143	1145	1150	rVB4	930	747	0.03%	0.004%
19	4.751	1150	1154	1156	rVB3	1314	872	0.04%	0.005%
20	4.767	1156	1159	1160	rBV3	932	533	0.02%	0.003%
21	4.799	1167	1169	1172	rBV3	703	455	0.02%	0.003%
22	4.889	1195	1197	1198	rBV2	669	292	0.01%	0.002%
23	4.950	1200	1216	1248	rVV2	972748	2417989	100.00%	13.601%
24	5.365	1343	1345	1350	rVB6	933	754	0.03%	0.004%
25	5.391	1351	1353	1357	rVB5	1272	725	0.03%	0.004%
26	5.461	1372	1375	1379	rBV4	862	630	0.03%	0.004%
27	5.529	1384	1396	1428	rBV	657961	1357384	56.14%	7.635%
28	5.986	1526	1538	1566	rBV	529863	1085031	44.87%	6.103%
29	6.265	1623	1625	1627	rBV4	998	535	0.02%	0.003%
30	6.297	1632	1635	1637	rBV4	955	647	0.03%	0.004%
31	6.336	1645	1647	1649	rBV4	834	331	0.01%	0.002%
32	6.477	1690	1691	1693	rBV	801	363	0.02%	0.002%
33	6.564	1712	1718	1722	rBV9	1474	1733	0.07%	0.010%
34	6.600	1726	1729	1730	rBV2	1059	601	0.02%	0.003%
35	6.677	1751	1753	1756	rBB4	788	401	0.02%	0.002%
36	6.703	1756	1761	1765	rBV6	1334	1341	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037138.D
 Acq On : 28 Aug 2024 18:04
 Operator : SY/MD
 Sample : P3734-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.744	1771	1774	1776	rBV4	902	491	0.02%	0.003%
38	6.844	1802	1805	1807	rVB3	1171	579	0.02%	0.003%
39	6.857	1807	1809	1811	rVB3	644	284	0.01%	0.002%
40	6.867	1811	1812	1815	rBV3	715	333	0.01%	0.002%
41	6.912	1815	1826	1857	rBV	269411	527323	21.81%	2.966%
42	7.239	1916	1928	1958	rBV	1083793	1926759	79.68%	10.838%
43	7.551	2016	2025	2049	rBV	177474	331526	13.71%	1.865%
44	8.027	2163	2173	2216	rBV2	442582	927895	38.37%	5.219%
45	8.690	2377	2379	2384	rVB6	754	492	0.02%	0.003%
46	8.731	2387	2392	2396	rBV7	1928	2138	0.09%	0.012%
47	8.780	2396	2407	2434	rBV	1018894	1686066	69.73%	9.484%
48	9.185	2529	2533	2537	rVB6	2501	1706	0.07%	0.010%
49	9.204	2537	2539	2542	rVB2	701	317	0.01%	0.002%
50	9.223	2542	2545	2547	rBV3	1783	1327	0.05%	0.007%
51	9.249	2551	2553	2557	rVV5	1446	831	0.03%	0.005%
52	9.313	2571	2573	2575	rBV2	1183	551	0.02%	0.003%
53	9.387	2595	2596	2600	rBV2	956	490	0.02%	0.003%
54	9.452	2613	2616	2618	rBV4	1297	926	0.04%	0.005%
55	9.487	2624	2627	2630	rBV4	1082	889	0.04%	0.005%
56	9.561	2648	2650	2651	rBV2	791	322	0.01%	0.002%
57	9.635	2671	2673	2674	rBV2	935	362	0.01%	0.002%
58	9.680	2685	2687	2691	rBV3	916	665	0.03%	0.004%
59	9.709	2694	2696	2703	rVB6	1597	1290	0.05%	0.007%
60	9.776	2715	2717	2719	rBV3	888	417	0.02%	0.002%
61	9.837	2733	2736	2737	rBV3	880	395	0.02%	0.002%
62	9.966	2772	2776	2783	rVB9	1275	1217	0.05%	0.007%
63	10.037	2795	2798	2799	rBV3	917	509	0.02%	0.003%
64	10.066	2803	2807	2809	rBV5	1845	1190	0.05%	0.007%
65	10.149	2820	2833	2853	rBV	663092	1053571	43.57%	5.926%
66	10.384	2903	2906	2907	rBV4	1404	706	0.03%	0.004%
67	10.493	2938	2940	2941	rBV2	1245	488	0.02%	0.003%
68	10.596	2969	2972	2977	rVB6	1761	1227	0.05%	0.007%
69	10.625	2977	2981	2983	rBV4	504	466	0.02%	0.003%
70	10.657	2988	2991	2992	rBV2	908	430	0.02%	0.002%
71	10.689	2999	3001	3002	rBV2	586	268	0.01%	0.002%
72	10.751	3018	3020	3023	rVV4	1084	584	0.02%	0.003%
73	10.789	3023	3032	3036	rVB4	2254	3375	0.14%	0.019%
74	10.850	3047	3051	3053	rBV4	1259	864	0.04%	0.005%
75	10.915	3068	3071	3073	rBV3	652	392	0.02%	0.002%
76	10.963	3082	3086	3089	rBV6	1454	1359	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
 Data File : VV037138.D
 Acq On : 28 Aug 2024 18:04
 Operator : SY/MD
 Sample : P3734-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	10.982	3089	3092	3095	rVV5	1648	1534	0.06%	0.009%
78	11.014	3099	3102	3105	rVB4	1428	738	0.03%	0.004%
79	11.037	3108	3109	3111	rBV2	831	318	0.01%	0.002%
80	11.075	3119	3121	3123	rBV2	1037	563	0.02%	0.003%
81	11.114	3130	3133	3134	rBV4	1856	1111	0.05%	0.006%
82	11.181	3143	3154	3181	rBV	1034102	1635724	67.65%	9.201%
83	11.554	3259	3270	3295	rBV	1041644	1678293	69.41%	9.440%
84	12.159	3456	3458	3462	rBV5	1522	1154	0.05%	0.006%
85	12.214	3471	3475	3478	rVB5	2140	1449	0.06%	0.008%
86	12.304	3495	3503	3504	rBV7	3962	4769	0.20%	0.027%
87	12.551	3578	3580	3582	rBV3	1045	460	0.02%	0.003%
88	12.628	3602	3604	3608	rBV4	1084	898	0.04%	0.005%
89	12.972	3708	3711	3714	rBV5	1251	723	0.03%	0.004%
90	13.001	3718	3720	3722	rVB2	1143	511	0.02%	0.003%
91	13.021	3722	3726	3728	rBV4	1018	718	0.03%	0.004%
92	13.050	3732	3735	3737	rBV2	1596	1051	0.04%	0.006%
93	13.130	3758	3760	3763	rVV4	1384	504	0.02%	0.003%
94	13.146	3763	3765	3769	rVB3	1032	808	0.03%	0.005%
95	13.204	3781	3783	3784	rBV	1411	660	0.03%	0.004%
96	13.394	3840	3842	3844	rBV3	1215	799	0.03%	0.004%
97	13.590	3901	3903	3904	rBV2	1541	517	0.02%	0.003%
98	13.622	3909	3913	3915	rBV5	1330	1027	0.04%	0.006%
99	14.030	4039	4040	4042	rBV2	1291	410	0.02%	0.002%
100	14.471	4174	4177	4178	rBV3	1723	1093	0.05%	0.006%




Sum of corrected areas: 17778462

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037138.D
Acq On : 28 Aug 2024 18:04
Operator : SY/MD
Sample : P3734-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44B0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

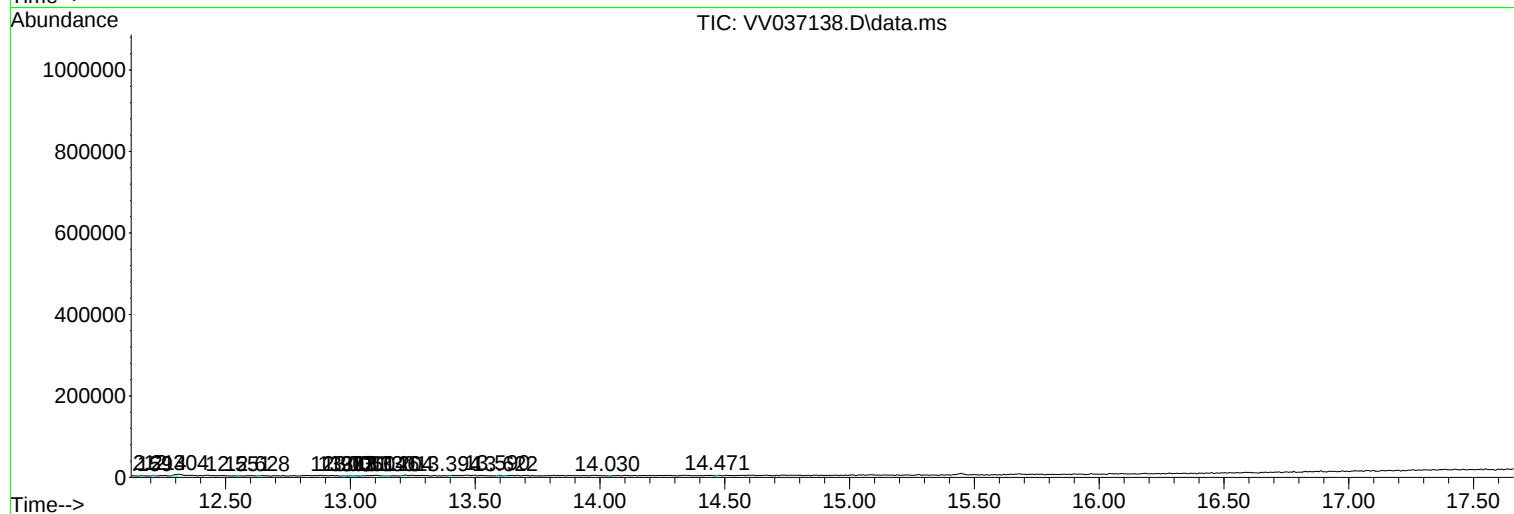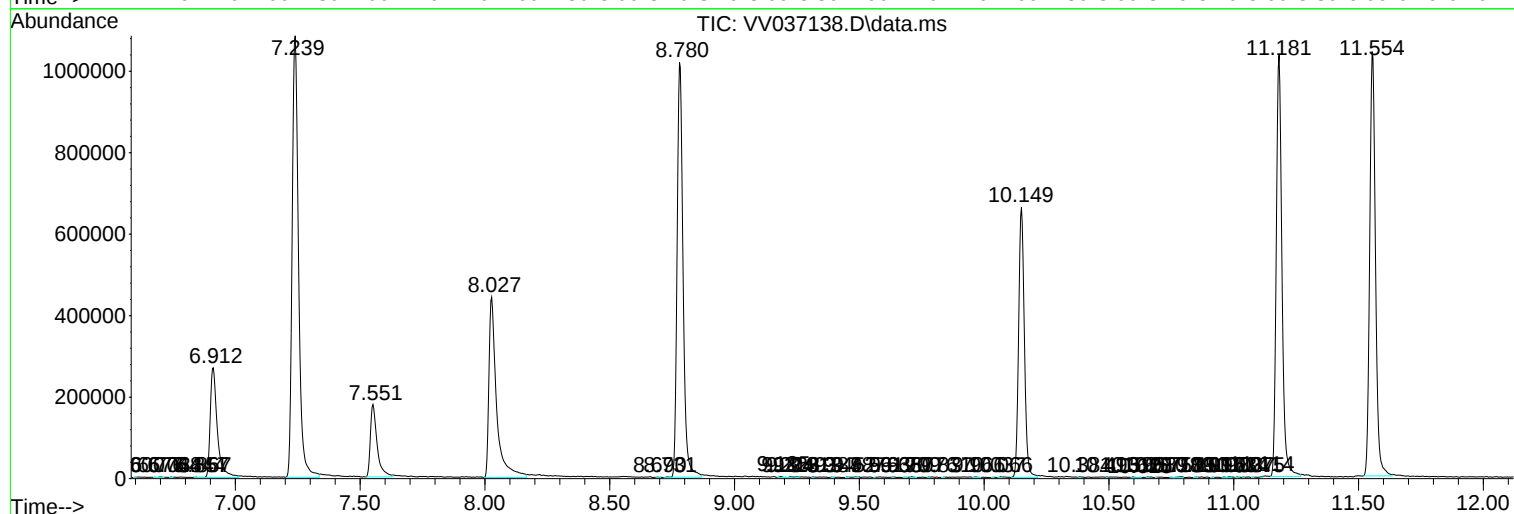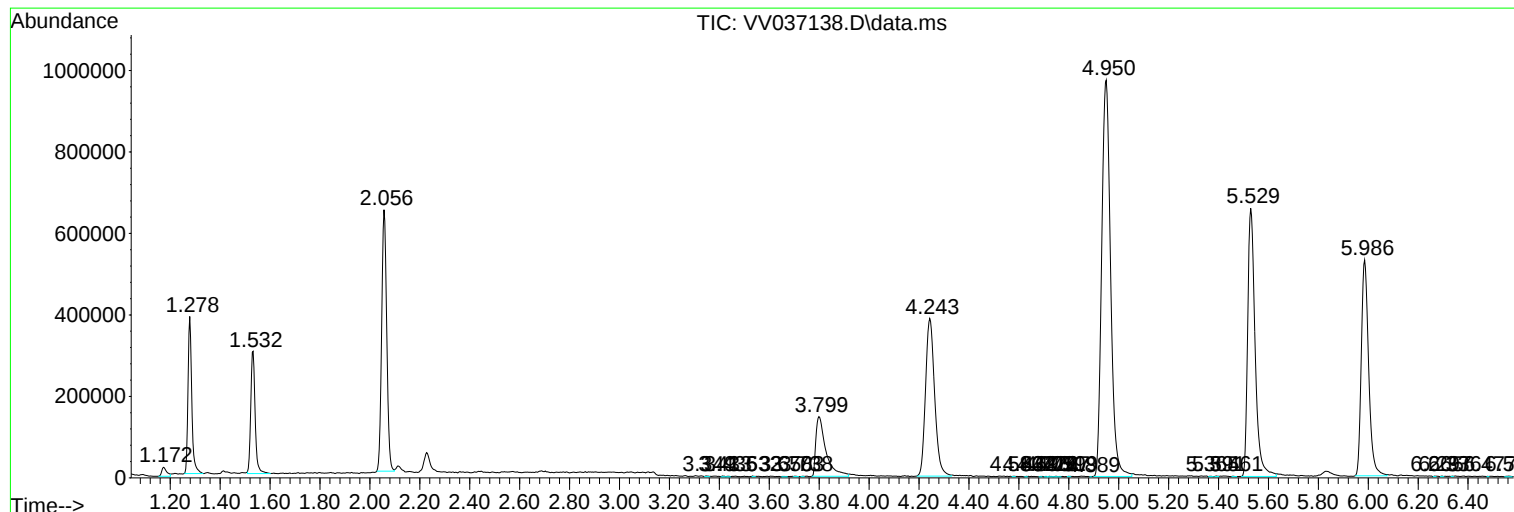

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037138.D
Acq On : 28 Aug 2024 18:04
Operator : SY/MD
Sample : P3734-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44B0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082824\
Data File : VV037138.D
Acq On : 28 Aug 2024 18:04
Operator : SY/MD
Sample : P3734-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44B0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------