

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037162.D
 Acq On : 29 Aug 2024 16:55
 Operator : SY/MD
 Sample : P3733-01
 Misc : 23.43G/10mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 29 23:44:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 29 23:38:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	638887	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	619767	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	296992	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	196795	33.673	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	67.340%		
7) Chloroethane-d5	1.503	69	85064	18.833	ug/L	-0.03
Spiked Amount 50.000	Range 70 - 130		Recovery =	37.660%#		
11) 1,1-Dichloroethene-d2	2.040	65	90301	36.762	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.520%		
21) 2-Butanone-d5	3.805	46	164653	72.752	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	72.750%		
24) Chloroform-d	4.240	84	343228	37.524	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.040%		
26) 1,2-Dichloroethane-d4	4.934	65	225935	39.224	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.440%		
32) Benzene-d6	4.947	84	710901	37.977	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.960%		
36) 1,2-Dichloropropane-d6	5.982	67	228656	38.999	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	78.000%		
41) Toluene-d8	7.236	98	619625	36.676	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.360%#		
43) trans-1,3-Dichloroprop...	7.551	79	90329	33.300	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.600%		
47) 2-Hexanone-d5	8.030	63	124740	77.955	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	77.950%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	269994	37.969	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	75.940%		
66) 1,2-Dichlorobenzene-d4	11.554	152	237019	39.847	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.700%#		
Target Compounds						Qvalue
15) Methyl Acetate	2.371	43	23206	5.703	ug/L	96
48) 2-Hexanone	8.030	43	15175	4.025	ug/L #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037162.D
Acq On : 29 Aug 2024 16:55
Operator : SY/MD
Sample : P3733-01
Misc : 23.43G/10mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 29 23:44:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 29 23:38:00 2024
Response via : Initial Calibration

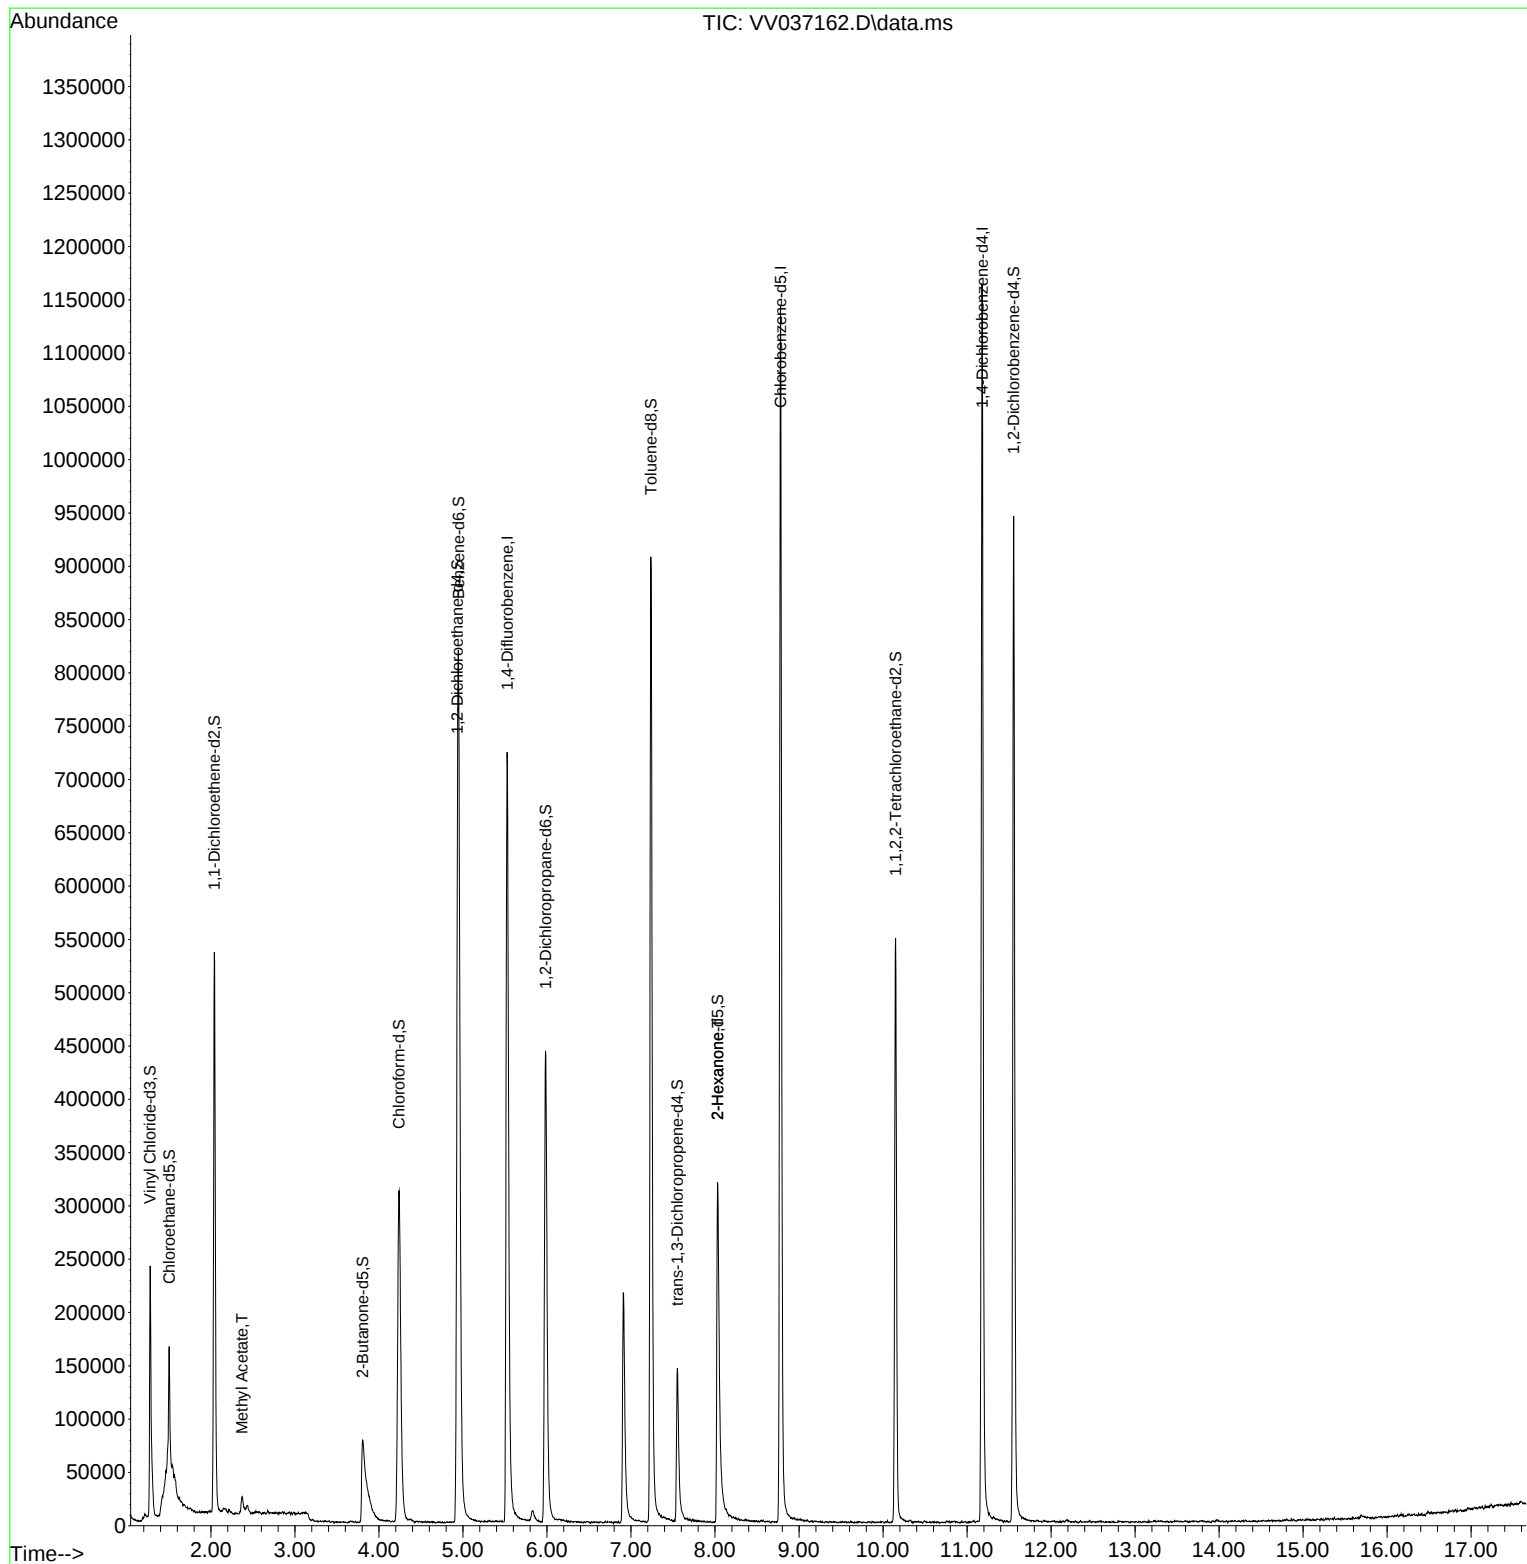

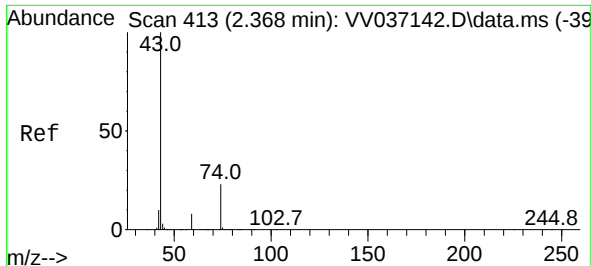

#15

Methyl Acetate

Concen: 5.703 ug/L

RT: 2.371 min Scan# 41

Delta R.T. 0.003 min

Lab File: VV037162.D

Acq: 29 Aug 2024 16:55

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 23206

Ion Ratio Lower Upper

43 100

74 20.8 18.4 27.6

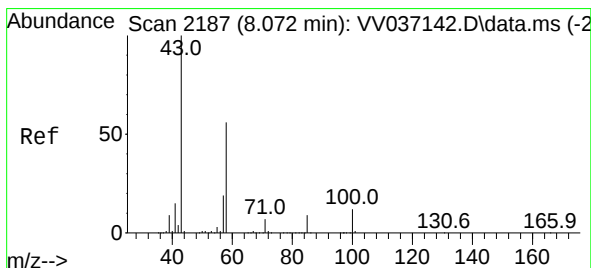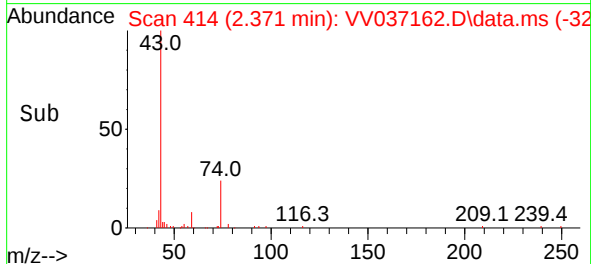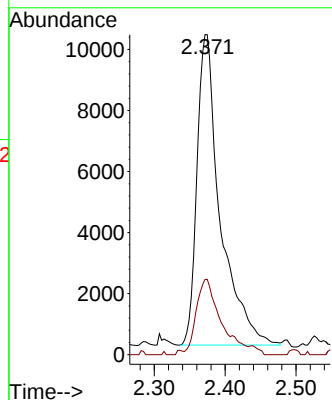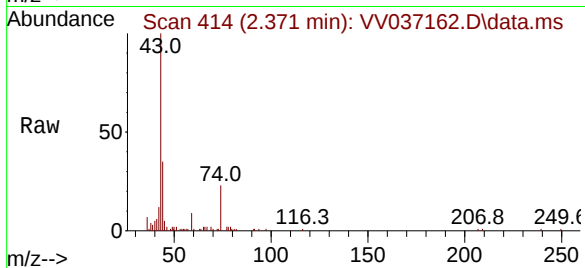

#48

2-Hexanone

Concen: 4.025 ug/L

RT: 8.030 min Scan# 2174

Delta R.T. -0.042 min

Lab File: VV037162.D

Acq: 29 Aug 2024 16:55

Tgt Ion: 43 Resp: 15175

Ion Ratio Lower Upper

43 100

58 35.7 46.0 69.0#

57 36.1 15.6 23.4#

100 0.6 10.6 16.0#

