

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037165.D
 Acq On : 29 Aug 2024 18:01
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 29 23:45:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 29 23:38:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	591840	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	570817	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	264400	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	227399	42.003	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	84.000%	
7) Chloroethane-d5	1.532	69	193697	46.292	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	92.580%	
11) 1,1-Dichloroethene-d2	2.056	65	99886	43.897	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	87.800%	
21) 2-Butanone-d5	3.796	46	217834	103.902	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	103.900%	
24) Chloroform-d	4.243	84	403094	47.573	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.140%	
26) 1,2-Dichloroethane-d4	4.937	65	264462	49.562	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.120%	
32) Benzene-d6	4.953	84	826910	47.962	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.920%	
36) 1,2-Dichloropropane-d6	5.986	67	270184	50.033	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	100.060%	
41) Toluene-d8	7.239	98	721796	46.388	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.780%	
43) trans-1,3-Dichloroprop...	7.551	79	107456	43.011	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	86.020%	
47) 2-Hexanone-d5	8.024	63	142723	96.841	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	96.840%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	322554	49.250	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.500%	
66) 1,2-Dichlorobenzene-d4	11.554	152	265947	50.222	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.440%	
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	2895	0.706	ug/L	# 25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037165.D
Acq On : 29 Aug 2024 18:01
Operator : SY/MD
Sample : VIBLK
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 29 23:45:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 29 23:38:00 2024
Response via : Initial Calibration

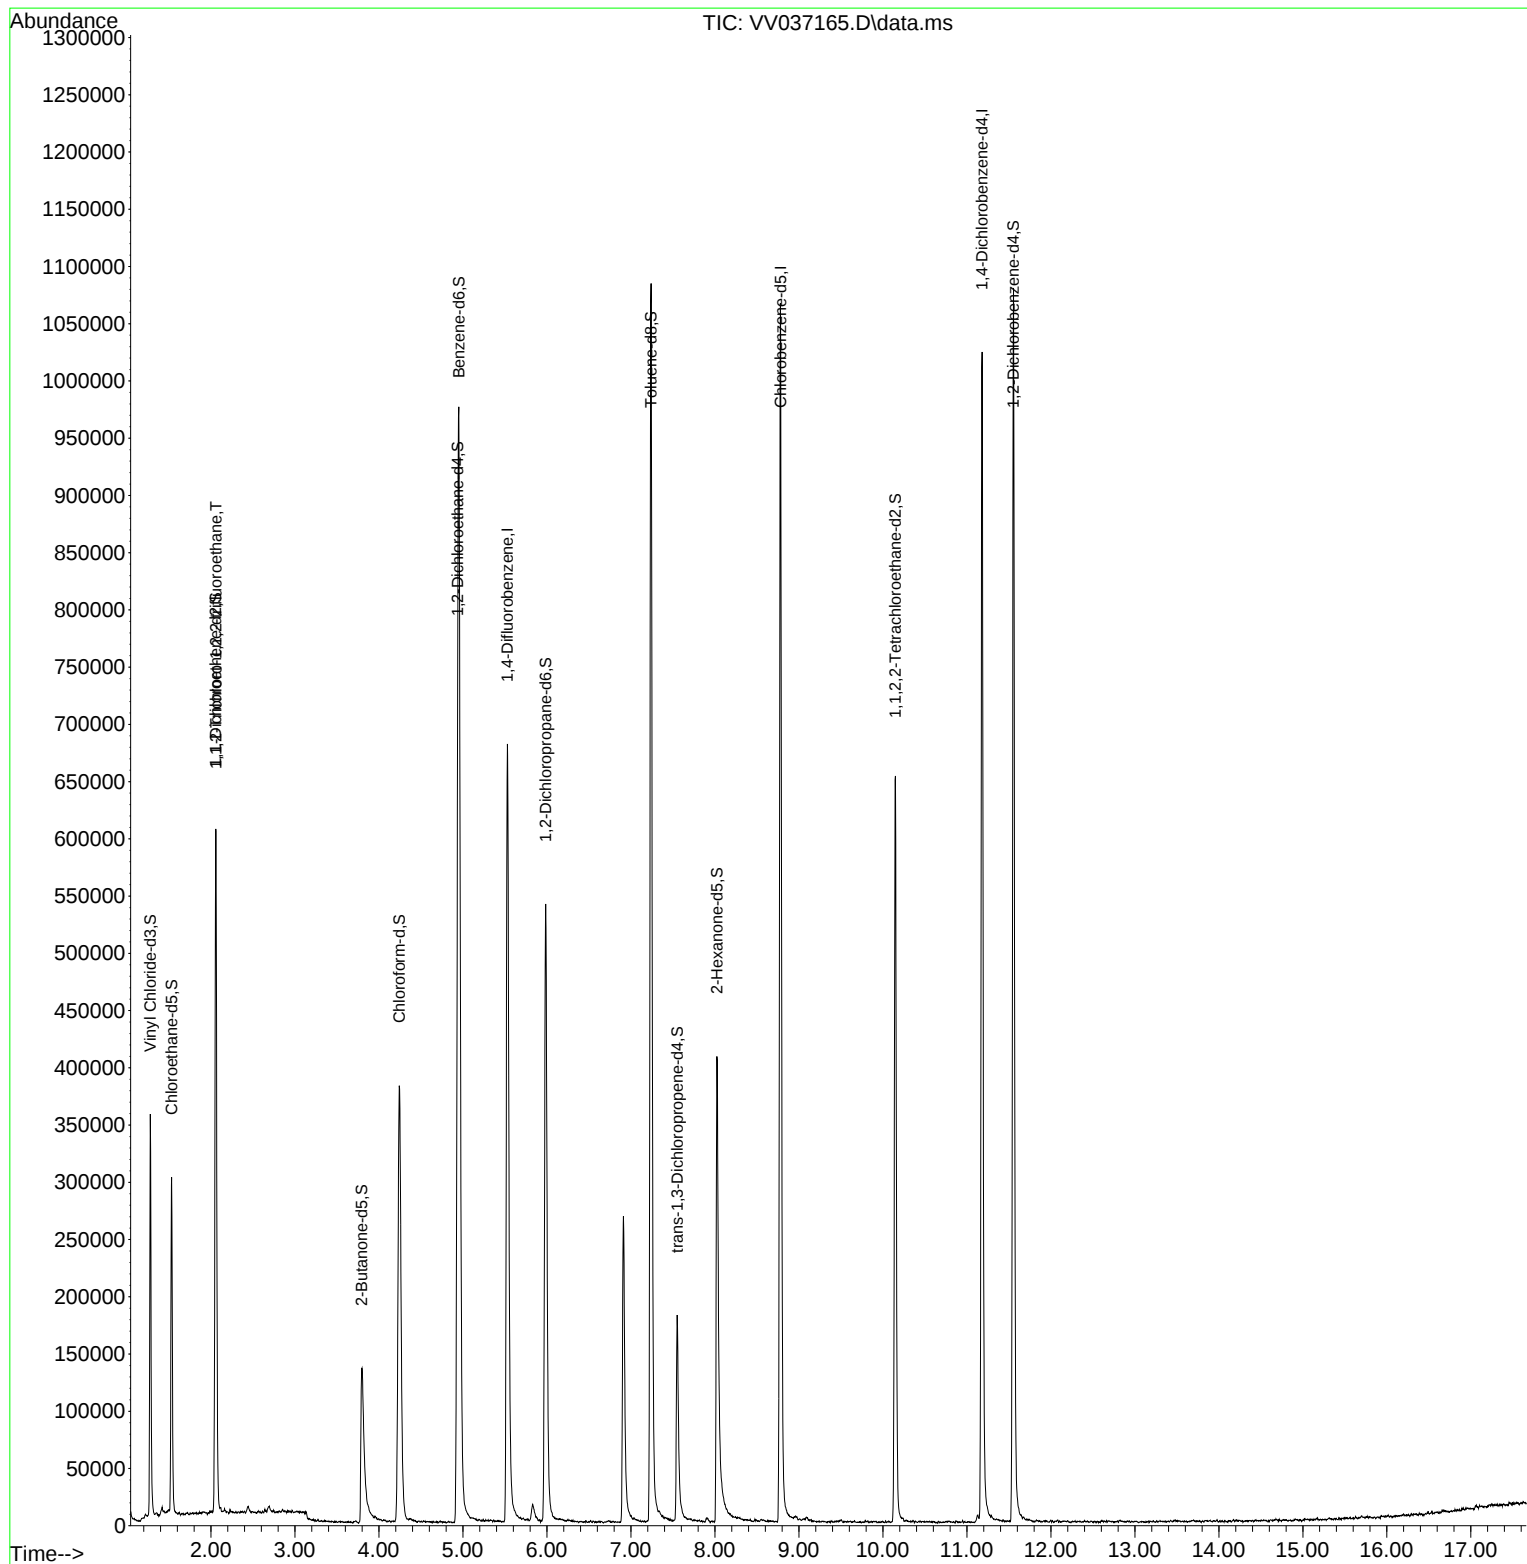

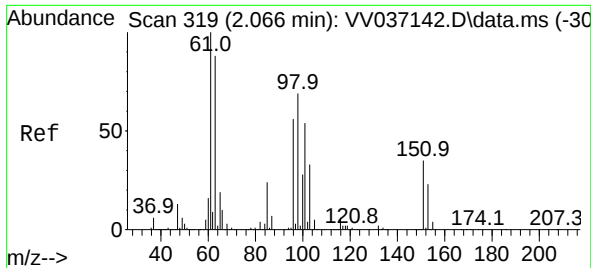

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.706 ug/L
RT: 2.060 min Scan# 317
Delta R.T. -0.007 min
Lab File: VV037165.D
Acq: 29 Aug 2024 18:01

Instrument :
MSVOA_V
ClientSampleId :

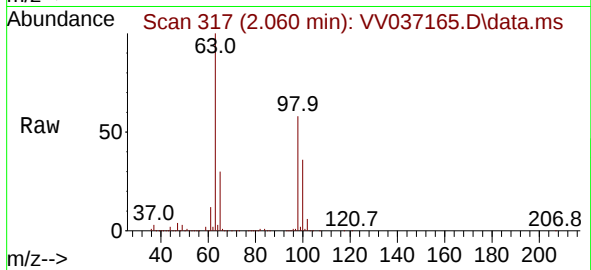

Tgt Ion:	101	Resp:	2895
Ion	Ratio	Lower	Upper
101	100		
85	5.6	35.6	53.4#
151	0.0	55.0	82.4#

