

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037167.D
 Acq On : 29 Aug 2024 19:28
 Operator : SY/MD
 Sample : VV0829MBL02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 30 01:20:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 30 01:20:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	581761	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	567404	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	254545	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	231386	43.480	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	86.960%	
7) Chloroethane-d5	1.532	69	193511	47.049	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	94.100%	
11) 1,1-Dichloroethene-d2	2.056	65	102094	45.644	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.280%	
21) 2-Butanone-d5	3.796	46	192343	93.333	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	93.330%	
24) Chloroform-d	4.243	84	399104	47.918	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.840%	
26) 1,2-Dichloroethane-d4	4.937	65	256618	48.925	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.860%	
32) Benzene-d6	4.953	84	827868	48.306	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.620%	
36) 1,2-Dichloropropane-d6	5.985	67	265677	49.495	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	98.980%	
41) Toluene-d8	7.239	98	717037	46.359	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.720%	
43) trans-1,3-Dichloroprop...	7.551	79	104069	41.906	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	83.820%	
47) 2-Hexanone-d5	8.024	63	132905	90.722	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	90.720%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	312159	47.950	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	95.900%	
66) 1,2-Dichlorobenzene-d4	11.554	152	264840	51.949	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	103.900%	
Target Compounds						
					Qvalue	
10) 1,1,2-Trichloro-1,2,2-...	2.056	101	3273	0.812	ug/L #	22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037167.D
Acq On : 29 Aug 2024 19:28
Operator : SY/MD
Sample : VV0829MBL02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 30 01:20:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 30 01:20:16 2024
Response via : Initial Calibration

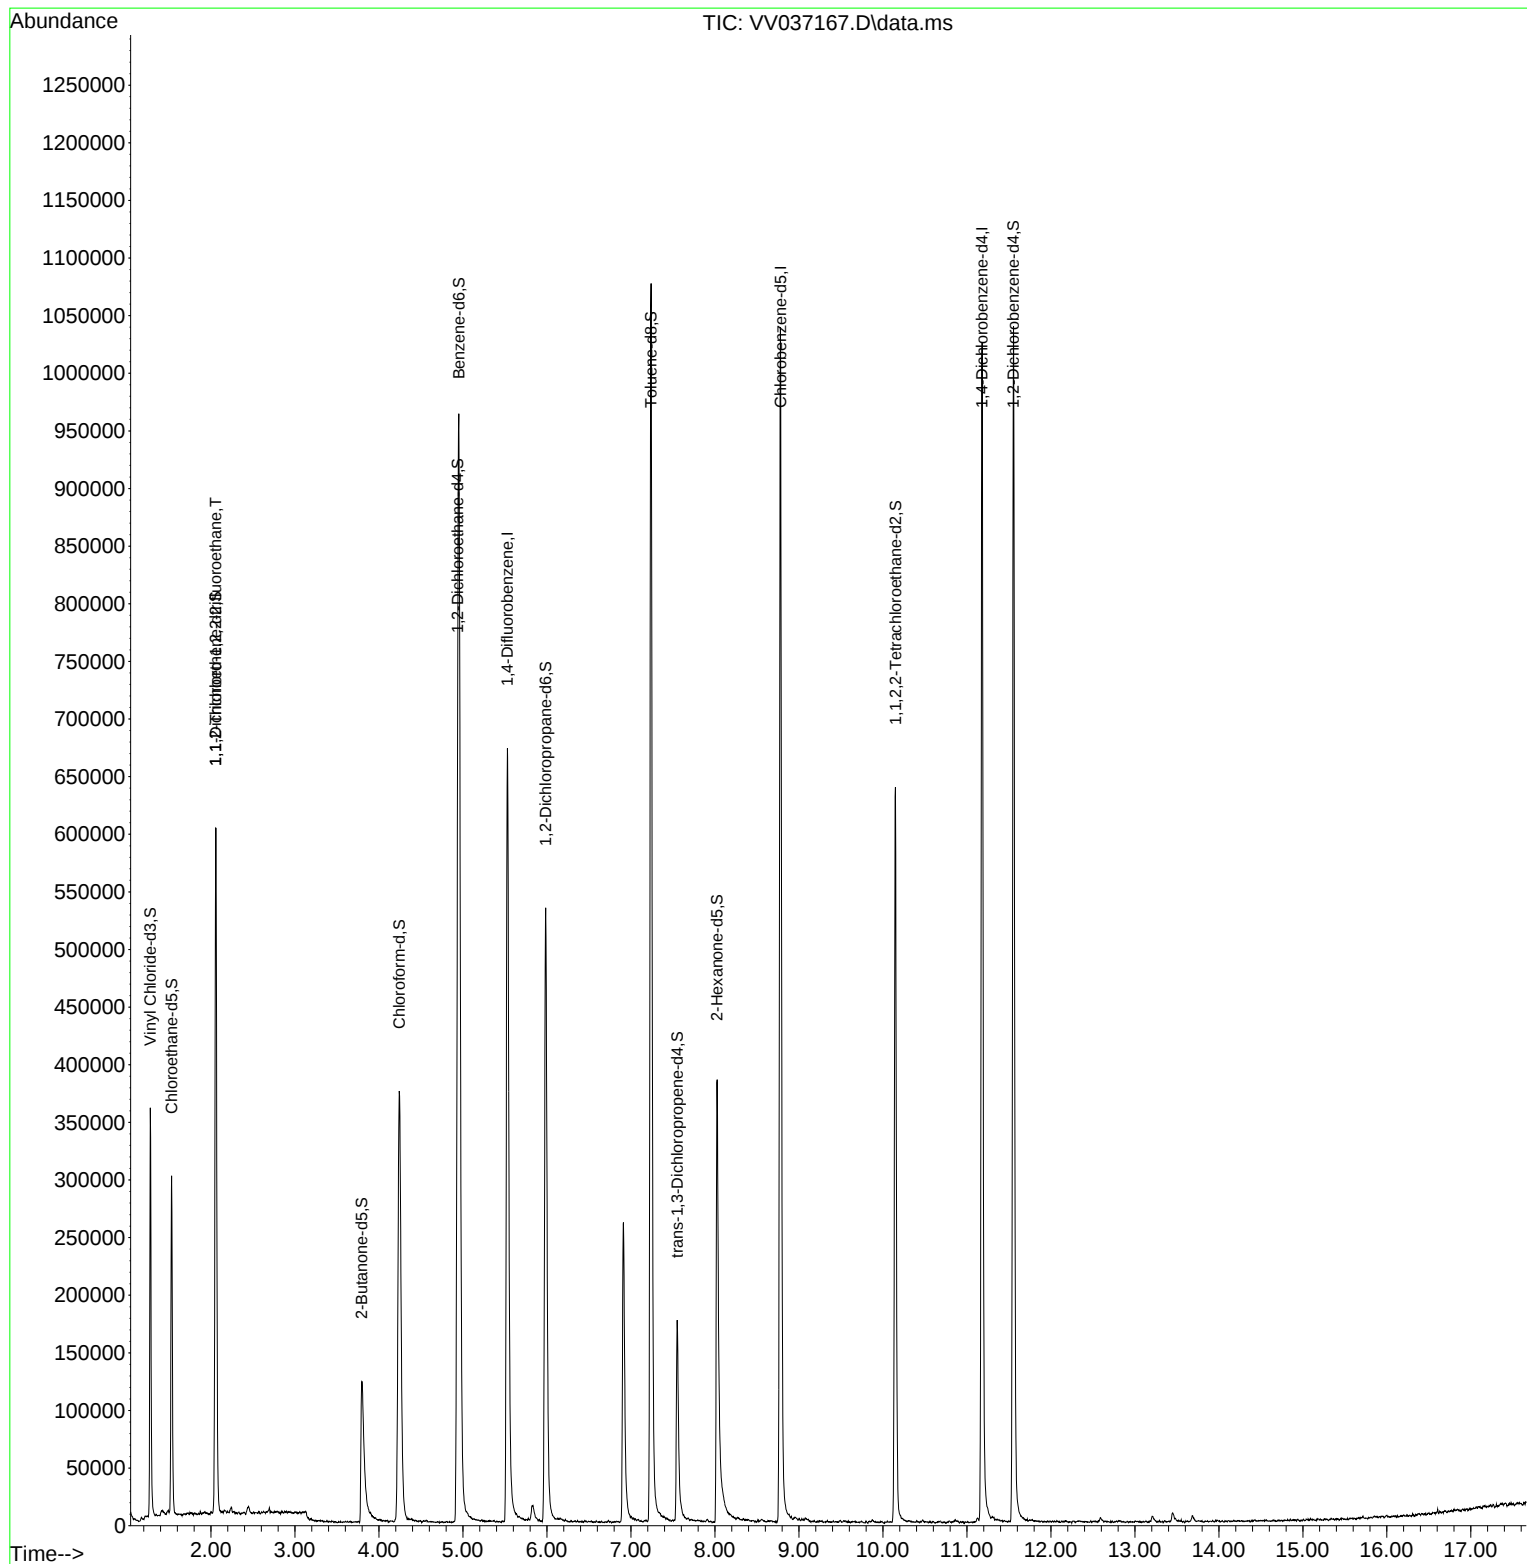

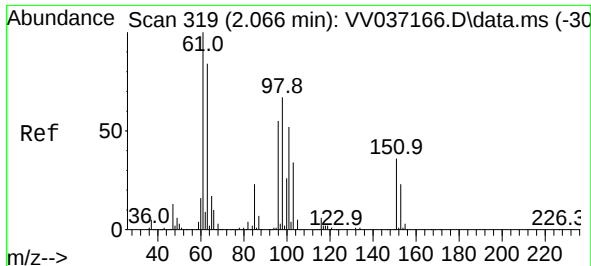

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.812 ug/L
 RT: 2.056 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV037167.D
 Acq: 29 Aug 2024 19:28

Instrument :
 MSVOA_V
 ClientSampleId :

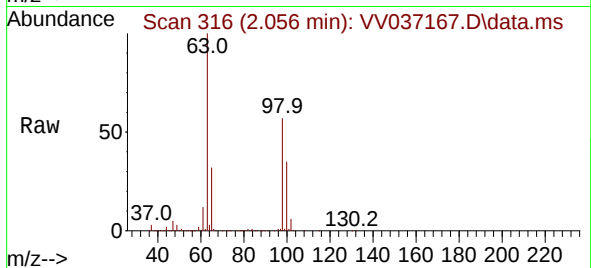

Tgt Ion:	101	Resp:	3273
Ion	Ratio	Lower	Upper
101	100		
85	0.0	35.6	53.4#
151	0.6	55.0	82.4#

