

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037178.D
 Acq On : 29 Aug 2024 23:36
 Operator : SY/MD
 Sample : P3692-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 30 01:44:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 30 01:20:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	562771	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	544272	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	250621	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	215536	41.868	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.740%
7) Chloroethane-d5	1.532	69	183317	46.075	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.140%
11) 1,1-Dichloroethene-d2	2.059	65	96973	44.818	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.640%
21) 2-Butanone-d5	3.796	46	179822	90.201	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.200%
24) Chloroform-d	4.243	84	385862	47.891	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.780%
26) 1,2-Dichloroethane-d4	4.937	65	245923	48.468	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.940%
32) Benzene-d6	4.953	84	784902	47.746	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.500%
36) 1,2-Dichloropropane-d6	5.985	67	257623	50.034	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.060%
41) Toluene-d8	7.239	98	684776	46.155	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.300%
43) trans-1,3-Dichloroprop...	7.551	79	96711	40.599	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.200%
47) 2-Hexanone-d5	8.024	63	113724	80.928	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	80.930%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	288660	46.225	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.440%
66) 1,2-Dichlorobenzene-d4	11.554	152	254735	50.750	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.500%
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.059	101	2900	0.744	ug/L	Qvalue # 25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037178.D
Acq On : 29 Aug 2024 23:36
Operator : SY/MD
Sample : P3692-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 30 01:44:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 30 01:20:16 2024
Response via : Initial Calibration

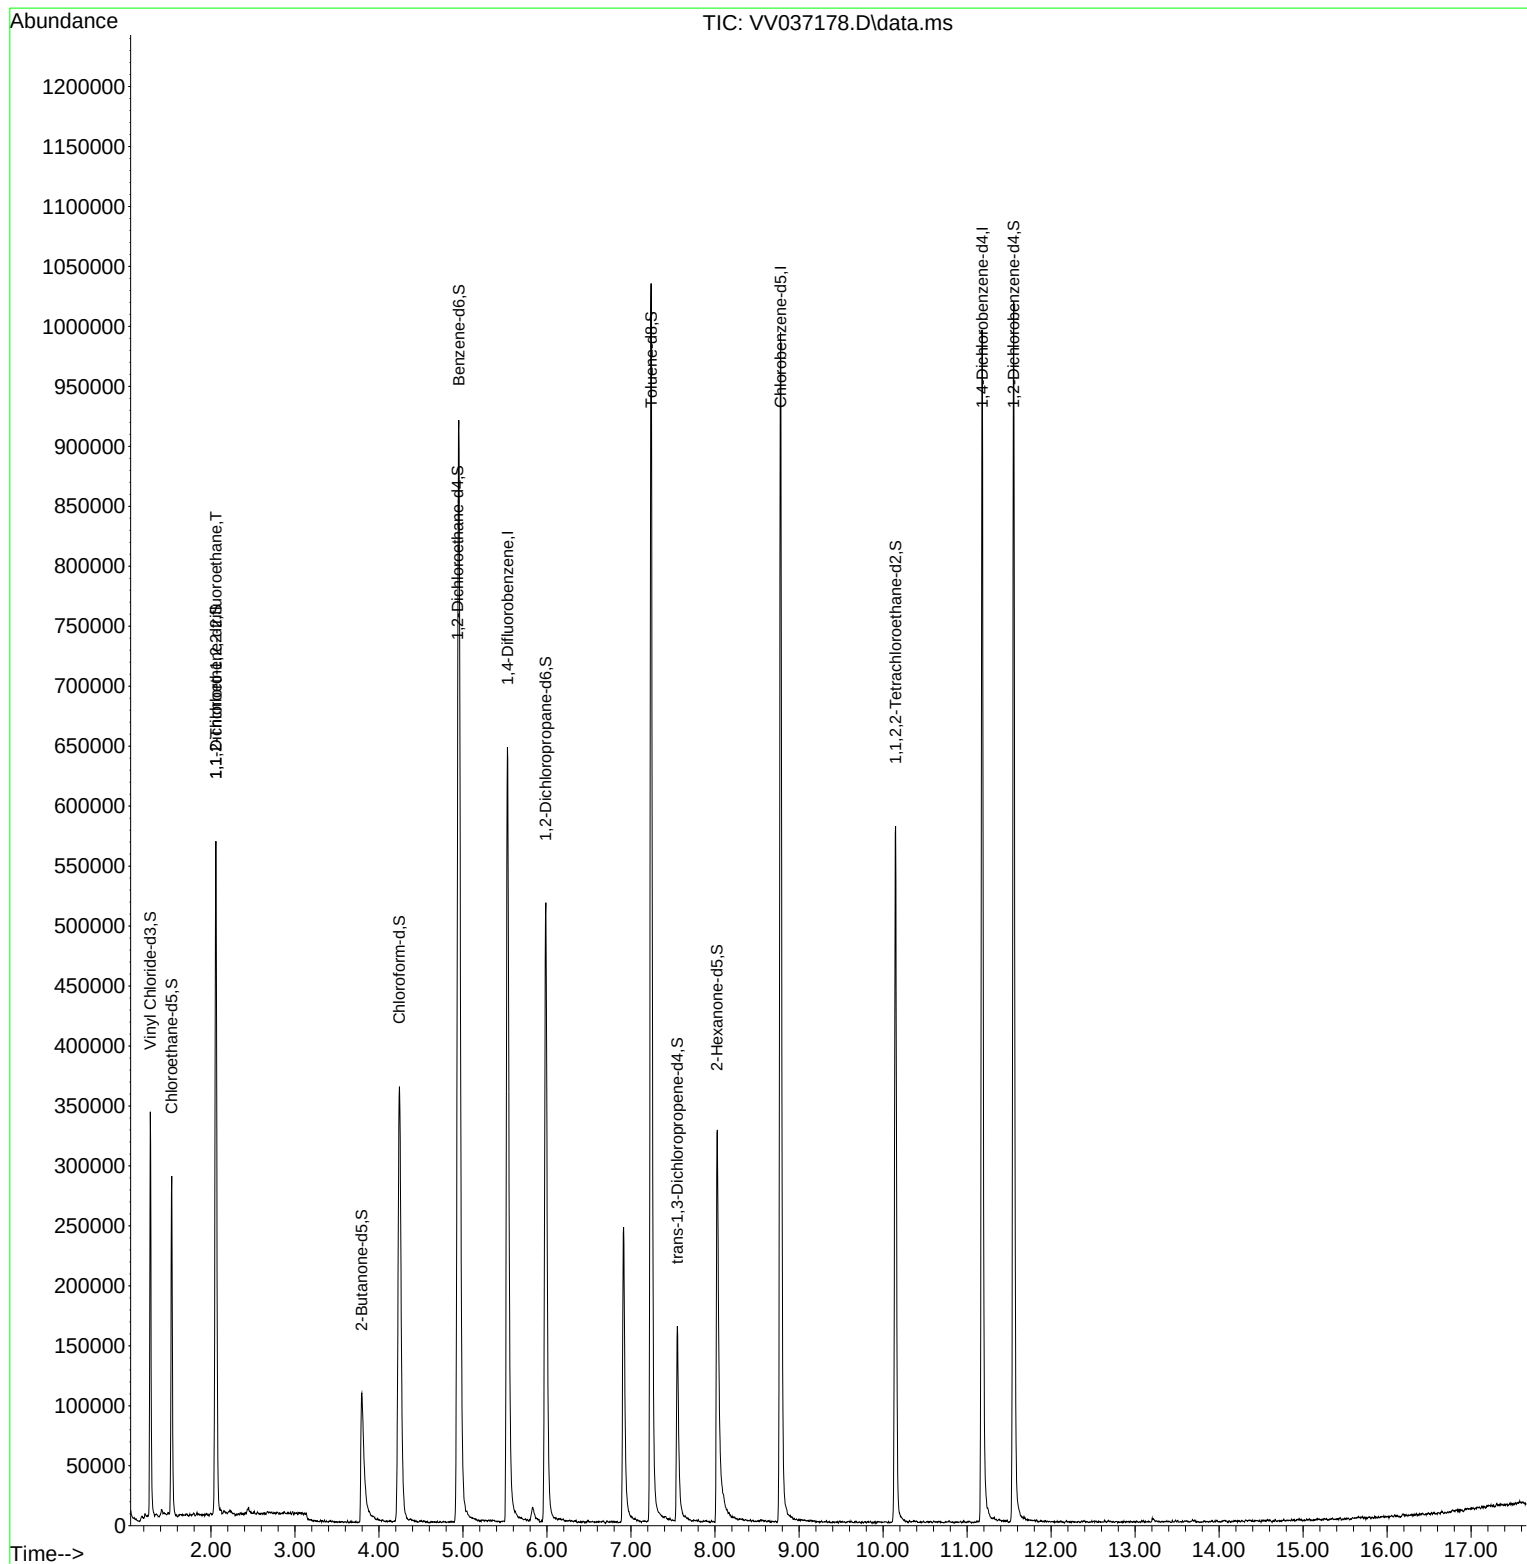

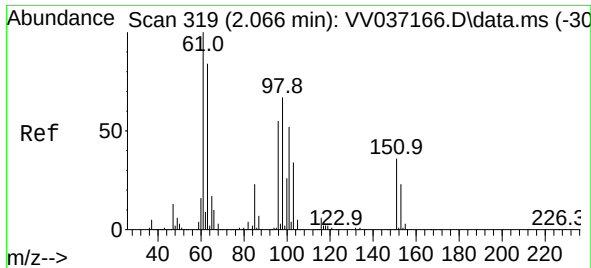

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.744 ug/L
 RT: 2.059 min Scan# 317
 Delta R.T. -0.007 min
 Lab File: VV037178.D
 Acq: 29 Aug 2024 23:36

Instrument :
 MSVOA_V
 ClientSampleId :

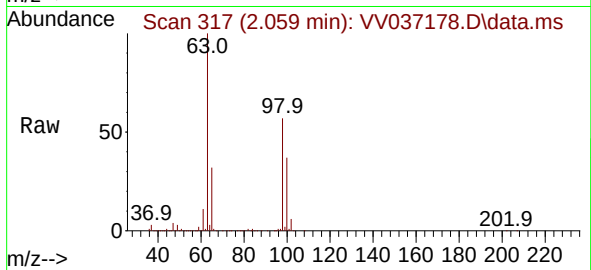

Tgt Ion:	101	Resp:	2900
Ion	Ratio	Lower	Upper
101	100		
85	4.3	35.6	53.4#
151	1.4	55.0	82.4#

