

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037145.D
 Acq On : 29 Aug 2024 10:45
 Operator : SY/MD
 Sample : P3734-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B2

Quant Time: Aug 29 23:39:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 29 23:38:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	577674	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	564627	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	262854	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	259535	49.114	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	98.220%	
7) Chloroethane-d5	1.532	69	208048	50.942	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	101.880%	
11) 1,1-Dichloroethene-d2	2.056	65	110788	49.882	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	99.760%	
21) 2-Butanone-d5	3.793	46	198116	96.814	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	96.810%	
24) Chloroform-d	4.240	84	419361	50.706	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.420%	
26) 1,2-Dichloroethane-d4	4.934	65	265161	50.911	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.820%	
32) Benzene-d6	4.950	84	850029	49.844	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.680%	
36) 1,2-Dichloropropane-d6	5.982	67	274308	51.354	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	102.700%	
41) Toluene-d8	7.236	98	740324	48.100	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.200%	
43) trans-1,3-Dichloroprop...	7.548	79	96774	39.160	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	78.320%	
47) 2-Hexanone-d5	8.024	63	120955	82.971	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	82.970%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	306423	47.300	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	94.600%	
66) 1,2-Dichlorobenzene-d4	11.554	152	266233	50.572	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	101.140%	
Target Compounds						
13) Acetone	2.111	43	15611	7.113	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037145.D
Acq On : 29 Aug 2024 10:45
Operator : SY/MD
Sample : P3734-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44B2

Quant Time: Aug 29 23:39:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 29 23:38:00 2024
Response via : Initial Calibration

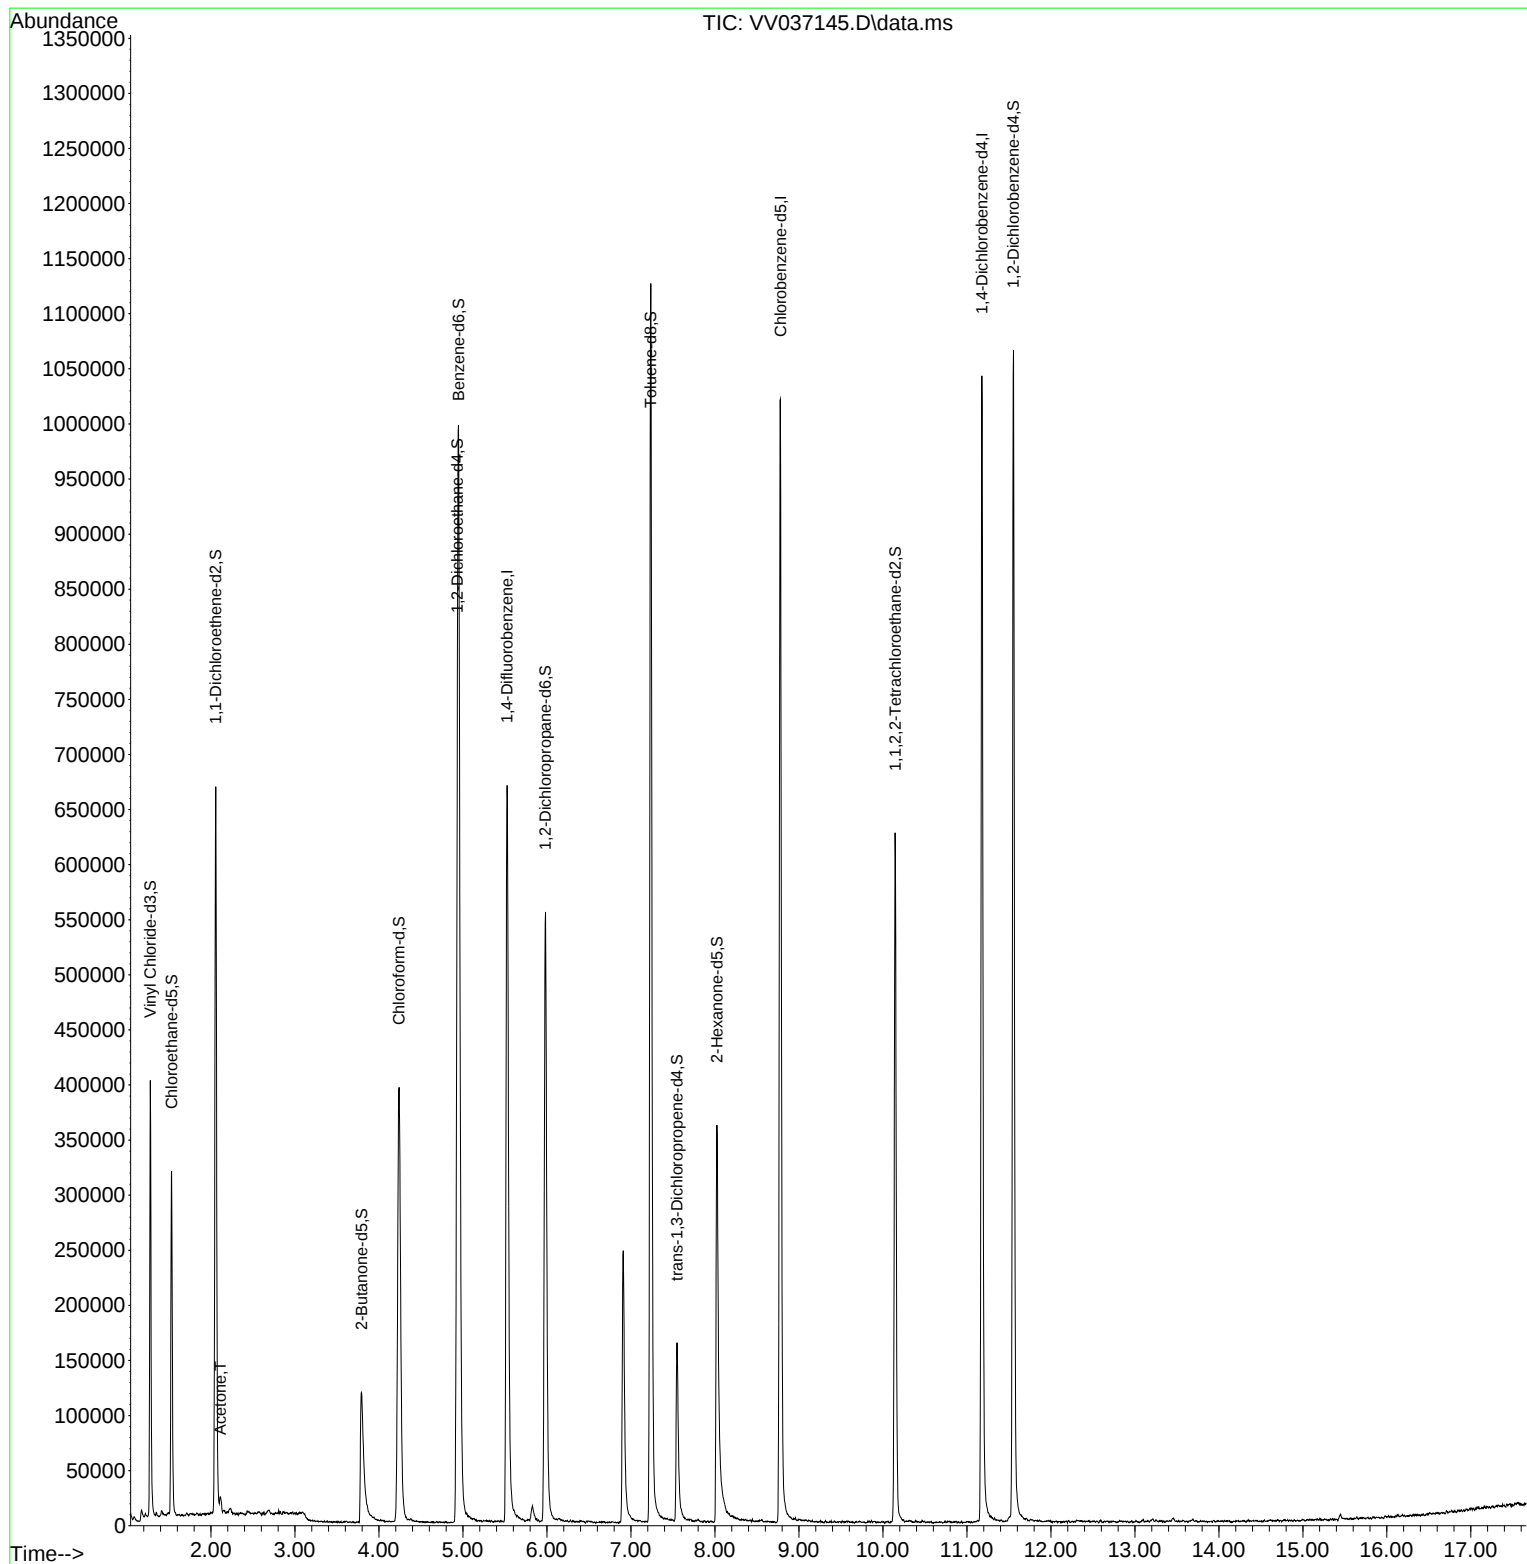

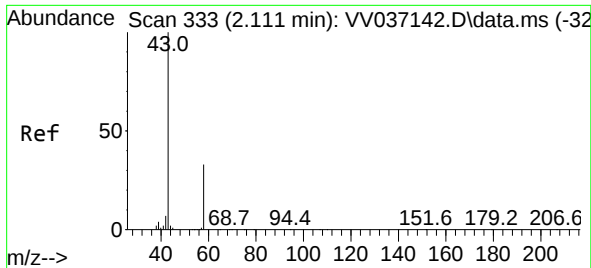

#13

Acetone

Concen: 7.113 ug/L

RT: 2.111 min Scan# 31

Delta R.T. -0.000 min

Lab File: VV037145.D


Acq: 29 Aug 2024 10:45

Instrument :

MSVOA_V

ClientSampleId :

A44B2

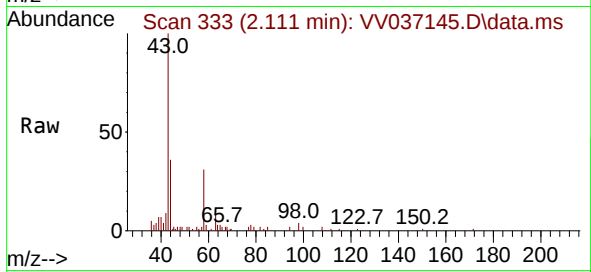

Tgt Ion: 43 Resp: 15611

Ion Ratio Lower Upper

43 100

58 34.0 0.0 64.8

