

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037157.D
 Acq On : 29 Aug 2024 15:06
 Operator : SY/MD
 Sample : VIBLK368
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK368

Quant Time: Aug 29 23:43:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 29 23:38:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	596541	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	572568	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	270910	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	242674	44.471	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	88.940%	
7) Chloroethane-d5	1.532	69	195659	46.393	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	92.780%	
11) 1,1-Dichloroethene-d2	2.056	65	104877	45.727	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.460%	
21) 2-Butanone-d5	3.796	46	217808	103.071	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	103.070%	
24) Chloroform-d	4.243	84	405298	47.456	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.920%	
26) 1,2-Dichloroethane-d4	4.937	65	261130	48.552	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.100%	
32) Benzene-d6	4.953	84	832612	48.145	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.300%	
36) 1,2-Dichloropropane-d6	5.986	67	269765	49.803	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	99.600%	
41) Toluene-d8	7.240	98	728464	46.673	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	93.340%	
43) trans-1,3-Dichloroprop...	7.551	79	107476	42.888	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	85.780%	
47) 2-Hexanone-d5	8.024	63	141548	95.750	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	95.750%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	318512	48.485	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	96.960%	
66) 1,2-Dichlorobenzene-d4	11.555	152	267129	49.233	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	98.460%	
Target Compounds						
20) cis-1,2-Dichloroethene	3.812	96	18653	4.178	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037157.D
Acq On : 29 Aug 2024 15:06
Operator : SY/MD
Sample : VIBLK368
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK368


Quant Time: Aug 29 23:43:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 29 23:38:00 2024
Response via : Initial Calibration

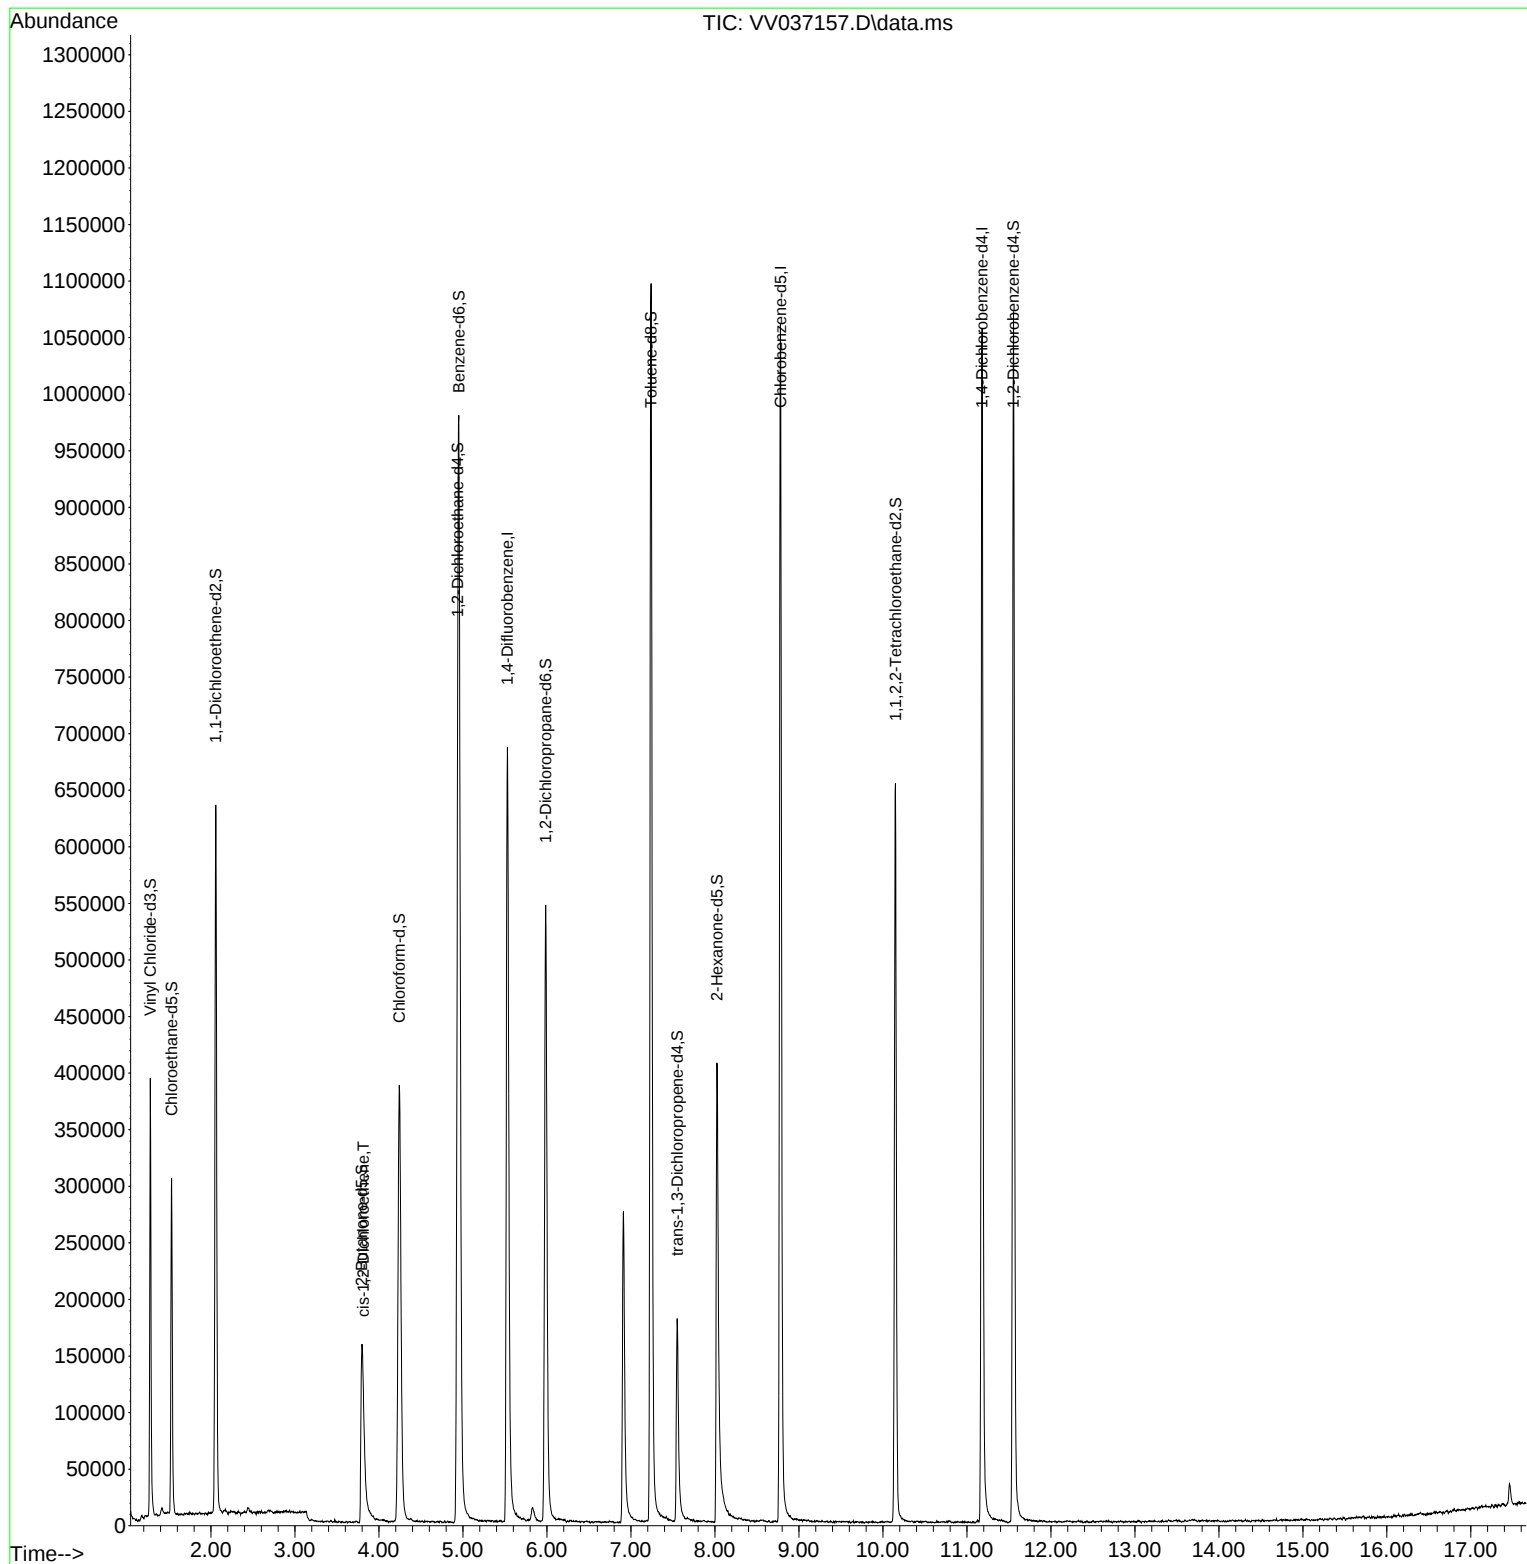

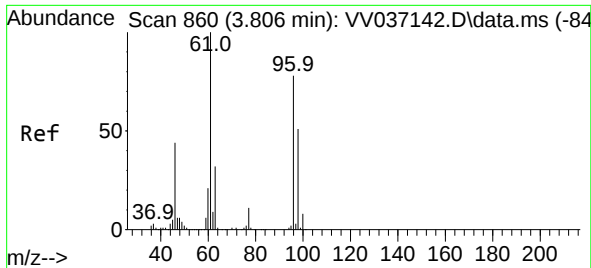

#20
 cis-1,2-Dichloroethene
 Concen: 4.178 ug/L
 RT: 3.812 min Scan# 80
 Delta R.T. 0.006 min
 Lab File: VV037157.D
 Acq: 29 Aug 2024 15:06

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK368

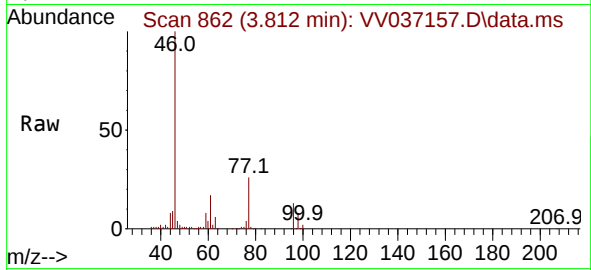

Tgt Ion:	96	Resp:	18653
Ion	Ratio	Lower	Upper
96	100		
61	132.0	89.9	166.9
98	63.3	44.8	83.2

