

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037161.D
 Acq On : 29 Aug 2024 16:34
 Operator : SY/MD
 Sample : P3733-20ME
 Misc : 16.56G/10mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B5ME

Quant Time: Aug 29 23:43:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 29 23:38:00 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	425592	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	412736	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	196012	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	356743	91.634	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 183.260%#		
7) Chloroethane-d5	1.500	69	115223	38.295	ug/L	-0.03
Spiked Amount	50.000	Range 70 - 130	Recovery	= 76.580%		
11) 1,1-Dichloroethene-d2	2.043	65	166422	101.706	ug/L	-0.01
Spiked Amount	50.000	Range 60 - 125	Recovery	= 203.420%#		
21) 2-Butanone-d5	3.793	46	353003	234.146	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 234.150%#		
24) Chloroform-d	4.236	84	623943	102.401	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 204.800%#		
26) 1,2-Dichloroethane-d4	4.931	65	405816	105.761	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 211.520%#		
32) Benzene-d6	4.947	84	1293510	103.761	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 207.520%#		
36) 1,2-Dichloropropane-d6	5.982	67	414562	106.173	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 212.340%#		
41) Toluene-d8	7.236	98	1146427	101.897	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 203.800%#		
43) trans-1,3-Dichloroprop...	7.548	79	172607	95.551	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 191.100%#		
47) 2-Hexanone-d5	8.024	63	252857	237.283	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 237.280%#		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	502045	106.017	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 212.040%#		
66) 1,2-Dichlorobenzene-d4	11.554	152	427340	108.856	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 217.720%#		
Target Compounds						Qvalue
15) Methyl Acetate	2.368	43	17866	6.591	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037161.D
Acq On : 29 Aug 2024 16:34
Operator : SY/MD
Sample : P3733-20ME
Misc : 16.56G/10mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44B5ME

Quant Time: Aug 29 23:43:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 29 23:38:00 2024
Response via : Initial Calibration

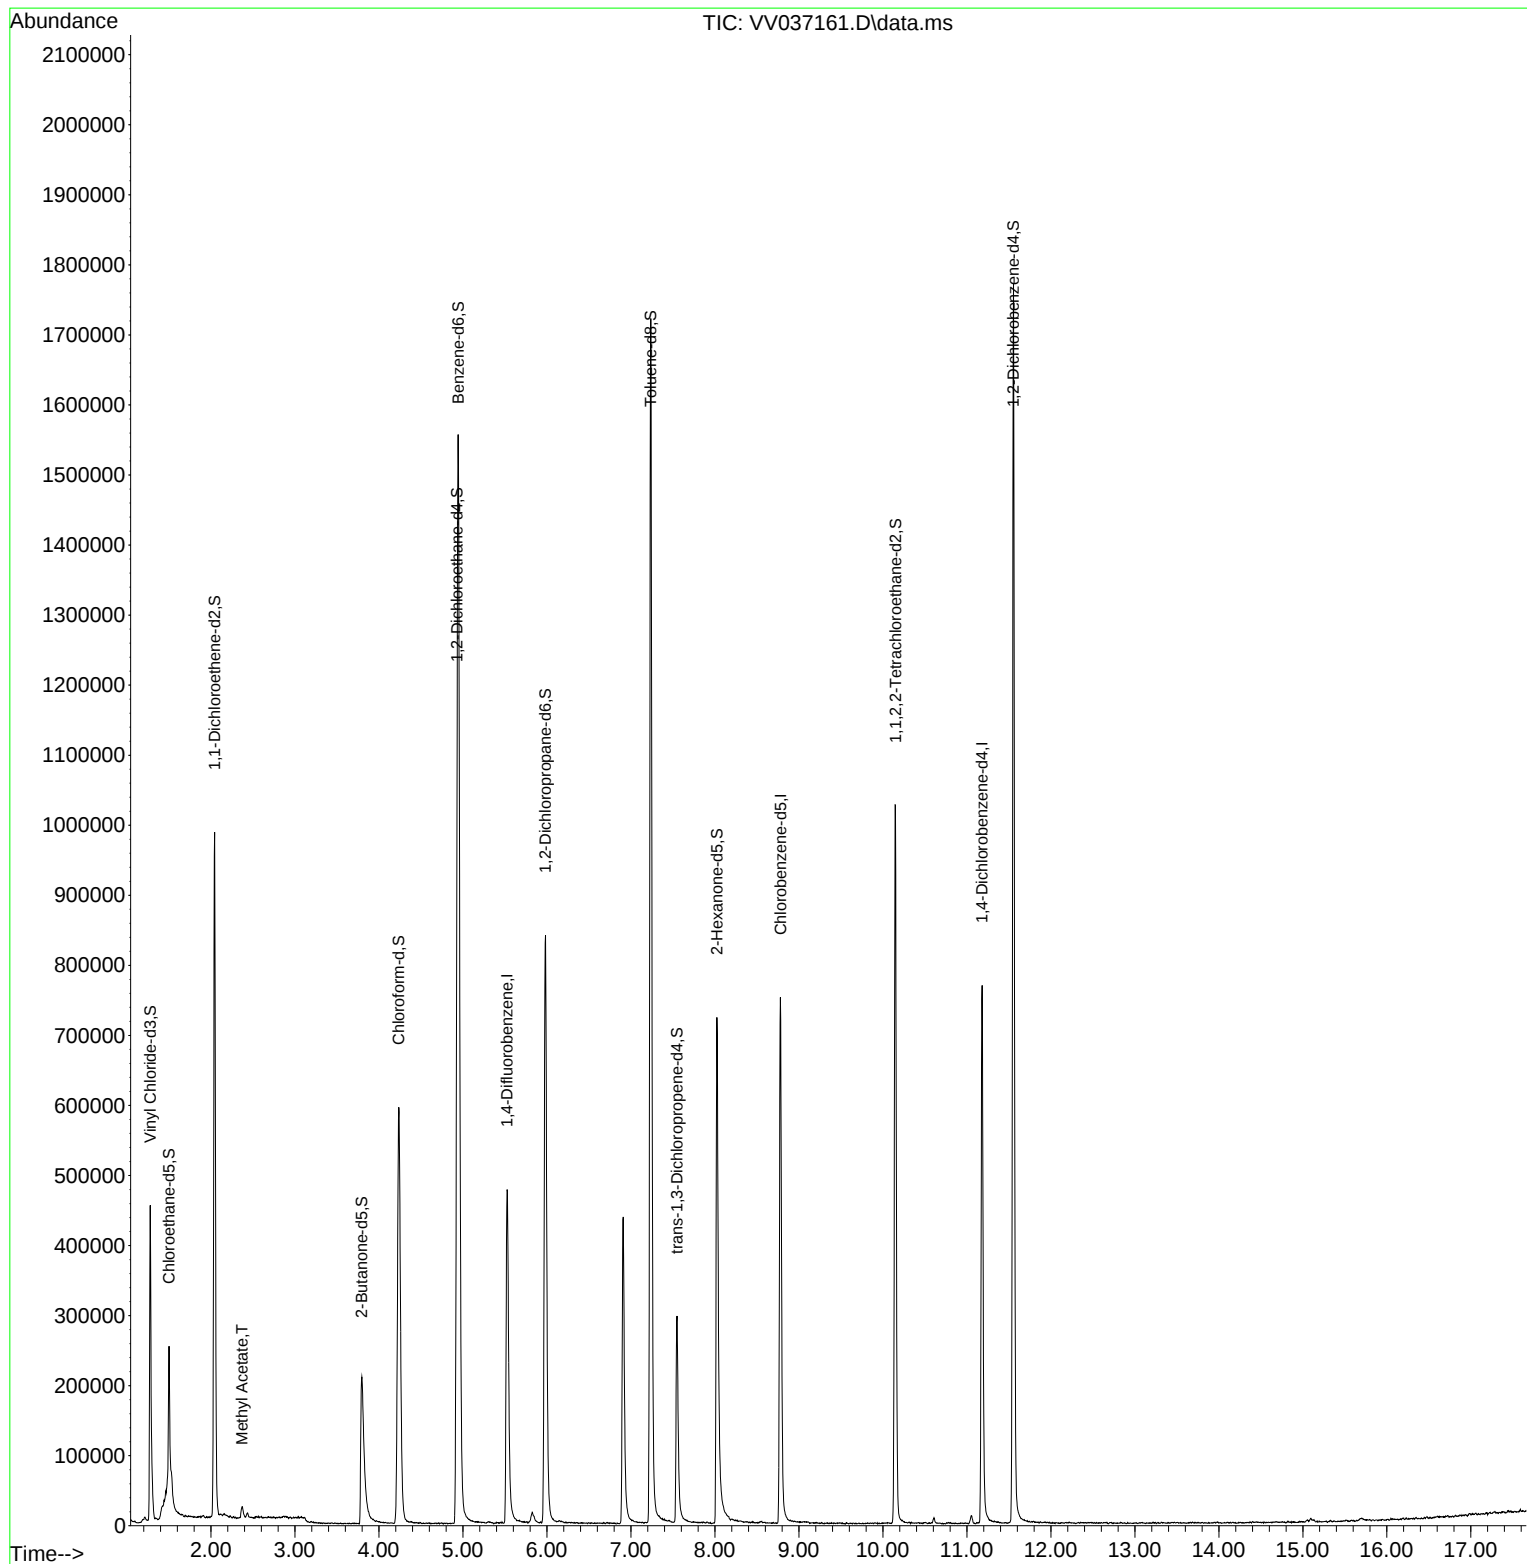

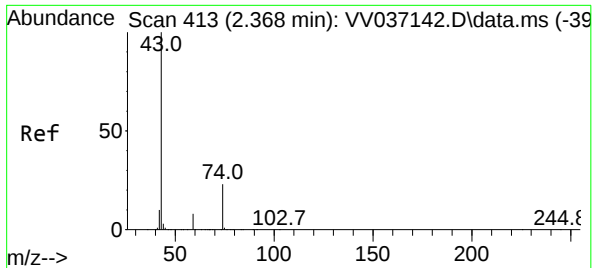

#15
Methyl Acetate
Concen: 6.591 ug/L
RT: 2.368 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV037161.D
Acq: 29 Aug 2024 16:34

Instrument :
MSVOA_V
ClientSampleId :
A44B5ME

Tgt Ion:	43	Resp:	17866
Ion	Ratio	Lower	Upper
43	100		
74	23.6	18.4	27.6

