

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037162.D
 Acq On : 29 Aug 2024 16:55
 Operator : SY/MD
 Sample : P3733-01
 Misc : 23.43G/10mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4495

Quant Time: Aug 29 23:44:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 29 23:38:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	638887	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	619767	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	296992	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	196795	33.673	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	67.340%
7) Chloroethane-d5	1.503	69	85064	18.833	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	37.660%#
11) 1,1-Dichloroethene-d2	2.040	65	90301	36.762	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.520%
21) 2-Butanone-d5	3.805	46	164653	72.752	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	72.750%
24) Chloroform-d	4.240	84	343228	37.524	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.040%
26) 1,2-Dichloroethane-d4	4.934	65	225935	39.224	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.440%
32) Benzene-d6	4.947	84	710901	37.977	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.960%
36) 1,2-Dichloropropane-d6	5.982	67	228656	38.999	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	78.000%
41) Toluene-d8	7.236	98	619625	36.676	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	73.360%#
43) trans-1,3-Dichloroprop...	7.551	79	90329	33.300	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.600%
47) 2-Hexanone-d5	8.030	63	124740	77.955	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.950%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	269994	37.969	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	75.940%
66) 1,2-Dichlorobenzene-d4	11.554	152	237019	39.847	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.700%#
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.371	43	23206	5.703	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037162.D
Acq On : 29 Aug 2024 16:55
Operator : SY/MD
Sample : P3733-01
Misc : 23.43G/10mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4495

Quant Time: Aug 29 23:44:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 29 23:38:00 2024
Response via : Initial Calibration

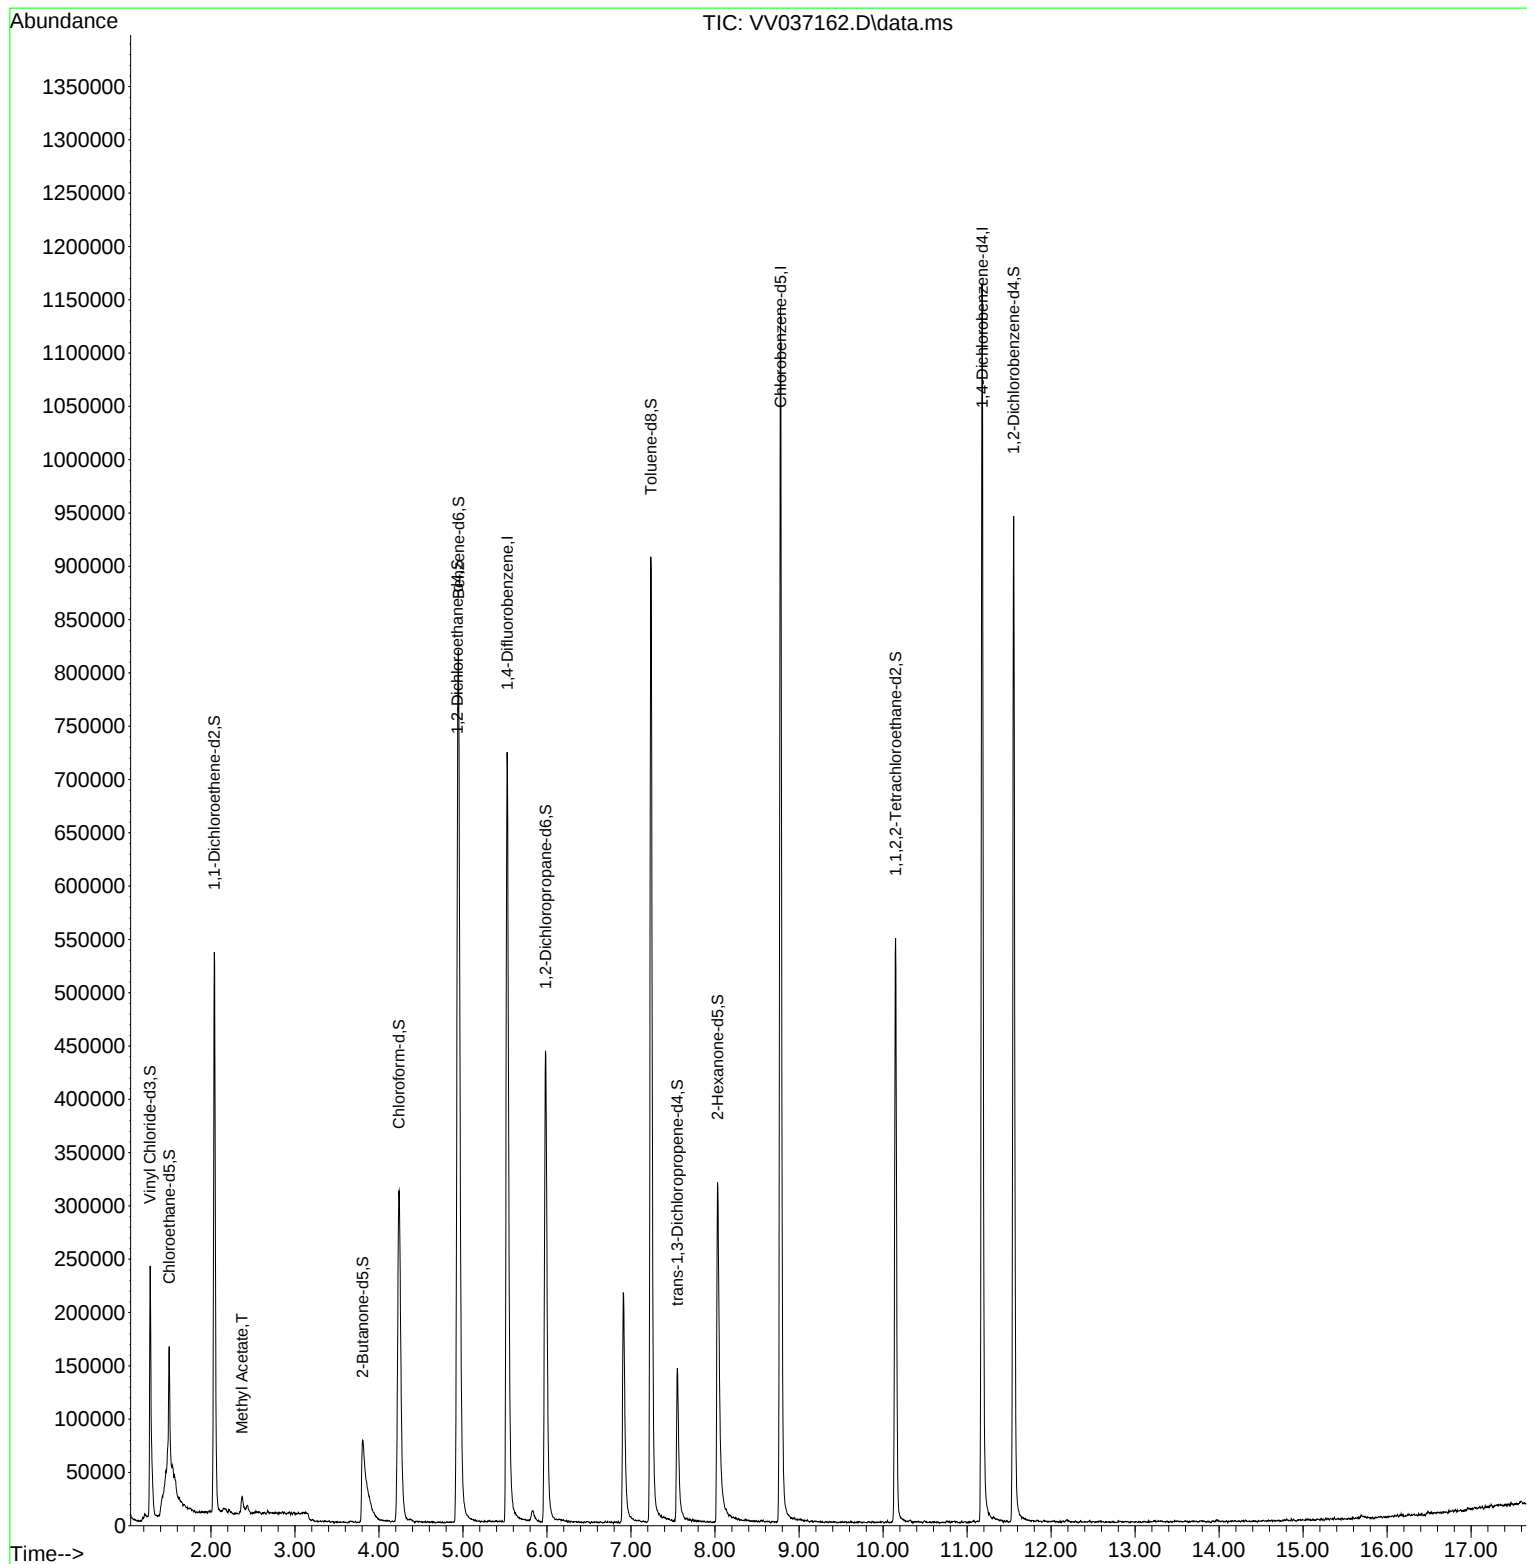

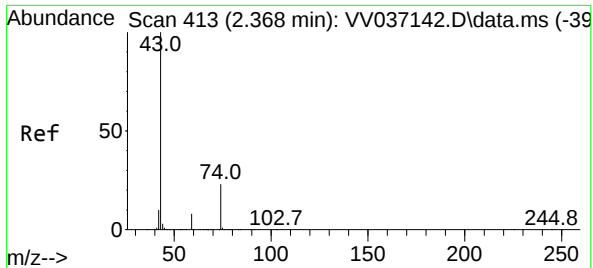

#15
Methyl Acetate
Concen: 5.703 ug/L
RT: 2.371 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV037162.D
Acq: 29 Aug 2024 16:55

Instrument :
MSVOA_V
ClientSampleId :
A4495

Tgt Ion: 43 Resp: 23206
Ion Ratio Lower Upper
43 100
74 20.8 18.4 27.6

