

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037145.D
 Acq On : 29 Aug 2024 10:45
 Operator : SY/MD
 Sample : P3734-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	37	41	51	rBV	8432	12487	0.50%	0.070%
2	1.278	67	74	89	rBV	394011	417033	16.73%	2.352%
3	1.532	145	153	170	rVB	312166	380472	15.27%	2.146%
4	2.056	307	316	329	rBV	657200	936594	37.58%	5.283%
5	3.455	748	751	753	rBV3	1281	675	0.03%	0.004%
6	3.494	761	763	766	rVB3	1274	566	0.02%	0.003%
7	3.584	785	791	793	rBV5	1207	1172	0.05%	0.007%
8	3.728	834	836	837	rBV2	729	299	0.01%	0.002%
9	3.754	843	844	847	rVB3	1245	452	0.02%	0.003%
10	3.793	847	856	887	rBV	118350	345144	13.85%	1.947%
11	4.240	980	995	1020	rBV	392392	992438	39.82%	5.598%
12	4.571	1096	1098	1103	rVB4	844	564	0.02%	0.003%
13	4.622	1112	1114	1116	rBV3	780	461	0.02%	0.003%
14	4.671	1127	1129	1130	rBV2	408	143	0.01%	0.001%
15	4.699	1136	1138	1140	rVB3	758	286	0.01%	0.002%
16	4.796	1164	1168	1170	rBV4	850	590	0.02%	0.003%
17	4.822	1174	1176	1178	rBV3	707	438	0.02%	0.002%
18	4.851	1183	1185	1188	rBV3	624	422	0.02%	0.002%
19	4.947	1199	1215	1242	rBV2	995242	2492211	100.00%	14.057%
20	5.526	1384	1395	1430	rBV	667989	1386361	55.63%	7.819%
21	5.982	1524	1537	1562	rBV	552665	1131911	45.42%	6.384%
22	6.391	1663	1664	1665	rBV	902	227	0.01%	0.001%
23	6.478	1685	1691	1693	rBV7	2044	2099	0.08%	0.012%
24	6.532	1705	1708	1714	rVB6	1399	1396	0.06%	0.008%
25	6.590	1723	1726	1728	rBV4	1112	609	0.02%	0.003%
26	6.648	1742	1744	1746	rVB3	1033	425	0.02%	0.002%
27	6.667	1746	1750	1753	rBV7	1263	1043	0.04%	0.006%
28	6.725	1767	1768	1769	rBV	641	168	0.01%	0.001%
29	6.831	1799	1801	1802	rBV2	493	190	0.01%	0.001%
30	6.860	1808	1810	1811	rBV2	1052	397	0.02%	0.002%
31	6.870	1811	1813	1814	rVV2	1131	420	0.02%	0.002%
32	6.908	1814	1825	1856	rVV	246673	487081	19.54%	2.747%
33	7.236	1915	1927	1960	rBV	1124323	1986215	79.70%	11.203%
34	7.548	2016	2024	2049	rBV	160636	296550	11.90%	1.673%
35	7.860	2120	2121	2123	rBV	1054	461	0.02%	0.003%
36	8.024	2163	2172	2208	rBV2	359887	782409	31.39%	4.413%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037145.D
 Acq On : 29 Aug 2024 10:45
 Operator : SY/MD
 Sample : P3734-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.445	2300	2303	2305	rBV4	2535	1408	0.06%	0.008%
38	8.702	2381	2383	2389	rVB7	1025	878	0.04%	0.005%
39	8.725	2389	2390	2392	rBV2	575	236	0.01%	0.001%
40	8.780	2396	2407	2433	rBV	1018302	1704303	68.39%	9.613%
41	9.239	2547	2550	2552	rBV3	884	626	0.03%	0.004%
42	9.317	2569	2574	2577	rBV6	2194	1886	0.08%	0.011%
43	9.426	2604	2608	2610	rVB5	1332	882	0.04%	0.005%
44	9.481	2622	2625	2626	rBV2	933	576	0.02%	0.003%
45	9.516	2632	2636	2638	rBV5	1865	1201	0.05%	0.007%
46	9.545	2643	2645	2647	rBV2	953	440	0.02%	0.002%
47	9.648	2675	2677	2681	rVB3	1120	749	0.03%	0.004%
48	9.670	2681	2684	2686	rBV4	1398	1006	0.04%	0.006%
49	9.722	2698	2700	2702	rBV3	826	382	0.02%	0.002%
50	9.812	2723	2728	2729	rBV3	815	646	0.03%	0.004%
51	9.821	2729	2731	2734	rVV4	1948	1060	0.04%	0.006%
52	9.841	2735	2737	2741	rVB4	1402	784	0.03%	0.004%
53	9.886	2749	2751	2754	rBV4	1212	1025	0.04%	0.006%
54	9.931	2762	2765	2767	rBV3	1156	638	0.03%	0.004%
55	9.944	2767	2769	2771	rVV3	837	384	0.02%	0.002%
56	9.956	2771	2773	2777	rVB5	541	294	0.01%	0.002%
57	10.024	2793	2794	2795	rBV	427	152	0.01%	0.001%
58	10.037	2795	2798	2801	rVV3	1358	995	0.04%	0.006%
59	10.146	2820	2832	2860	rBV	625375	998712	40.07%	5.633%
60	10.387	2904	2907	2910	rBV3	1766	955	0.04%	0.005%
61	10.403	2910	2912	2914	rVB3	1369	580	0.02%	0.003%
62	10.452	2924	2927	2929	rBV4	782	478	0.02%	0.003%
63	10.464	2929	2931	2933	rBV2	1607	830	0.03%	0.005%
64	10.580	2966	2967	2969	rVB2	1074	262	0.01%	0.001%
65	10.612	2973	2977	2980	rBV5	744	636	0.03%	0.004%
66	10.738	3014	3016	3017	rBV2	925	192	0.01%	0.001%
67	10.747	3017	3019	3022	rVB4	1427	764	0.03%	0.004%
68	10.773	3025	3027	3029	rBV	1012	472	0.02%	0.003%
69	10.834	3044	3046	3049	rBV4	801	360	0.01%	0.002%
70	10.850	3049	3051	3054	rVV4	948	437	0.02%	0.002%
71	10.873	3054	3058	3062	rVB5	1567	1677	0.07%	0.009%
72	10.892	3062	3064	3065	rBV2	784	324	0.01%	0.002%
73	10.927	3072	3075	3077	rBV3	1010	639	0.03%	0.004%
74	10.937	3077	3078	3081	rVB	1781	576	0.02%	0.003%
75	10.953	3081	3083	3086	rBV3	1093	850	0.03%	0.005%
76	11.053	3111	3114	3118	rBV4	1487	1013	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037145.D
 Acq On : 29 Aug 2024 10:45
 Operator : SY/MD
 Sample : P3734-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A44B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.085	3118	3124	3127	rBV4	1403	1359	0.05%	0.008%
78	11.178	3143	3153	3176	rBV	1039142	1626354	65.26%	9.173%
79	11.554	3259	3270	3297	rBV	1058221	1688760	67.76%	9.525%
80	11.995	3406	3407	3410	rVB2	1936	726	0.03%	0.004%
81	12.011	3410	3412	3414	rBV3	1092	476	0.02%	0.003%
82	12.024	3414	3416	3422	rBV6	1197	1117	0.04%	0.006%
83	12.136	3449	3451	3453	rBV2	934	474	0.02%	0.003%
84	12.214	3470	3475	3479	rBV6	2144	2363	0.09%	0.013%
85	12.281	3493	3496	3500	rBV4	1026	862	0.03%	0.005%
86	12.304	3500	3503	3505	rBV3	1791	1286	0.05%	0.007%
87	12.590	3585	3592	3593	rBV5	2504	2329	0.09%	0.013%
88	12.625	3598	3603	3604	rBV4	846	661	0.03%	0.004%
89	12.706	3624	3628	3629	rBV4	1450	1048	0.04%	0.006%
90	12.796	3653	3656	3657	rBV3	877	491	0.02%	0.003%
91	12.943	3698	3702	3704	rBV3	1094	1022	0.04%	0.006%
92	12.988	3712	3716	3720	rBV6	1197	1045	0.04%	0.006%
93	13.127	3755	3759	3761	rBV5	1023	912	0.04%	0.005%
94	13.342	3823	3826	3830	rBV4	1676	1326	0.05%	0.007%
95	13.644	3917	3920	3922	rBV3	1274	985	0.04%	0.006%
96	13.934	4006	4010	4012	rBV5	1918	1538	0.06%	0.009%
97	14.066	4048	4051	4054	rBV4	1541	1078	0.04%	0.006%
98	14.146	4073	4076	4078	rBV3	945	509	0.02%	0.003%
99	14.336	4133	4135	4137	rBV2	1392	732	0.03%	0.004%
100	14.541	4194	4199	4202	rBV7	1841	1504	0.06%	0.008%




Sum of corrected areas: 17729674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037145.D
Acq On : 29 Aug 2024 10:45
Operator : SY/MD
Sample : P3734-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44B2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

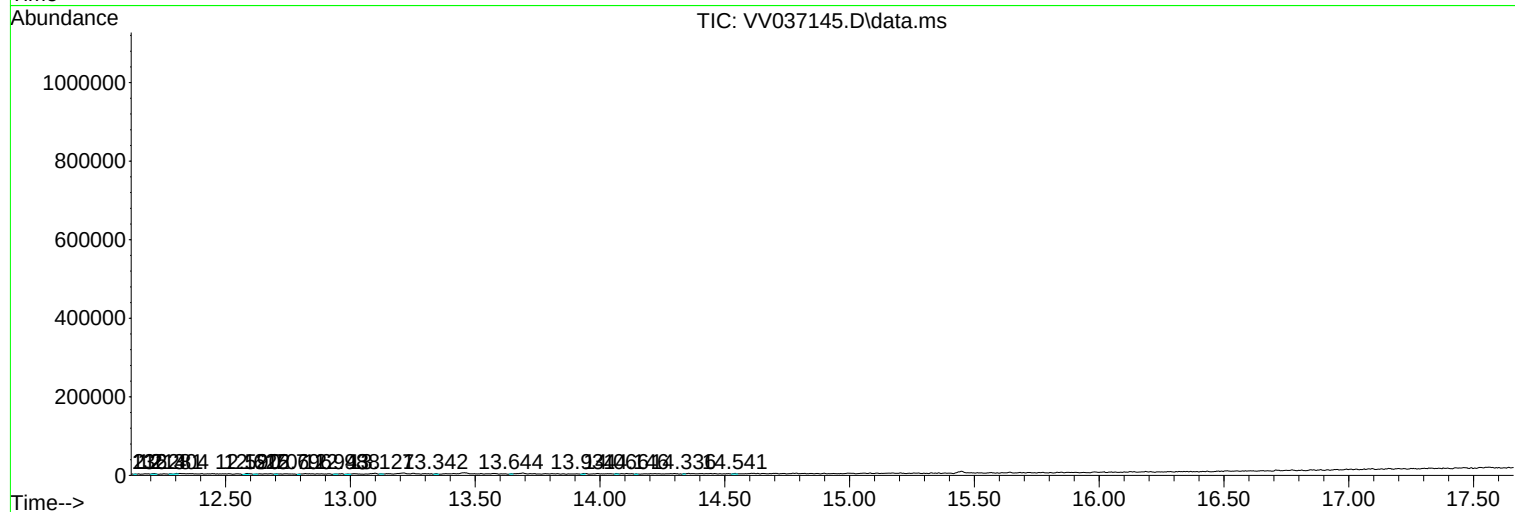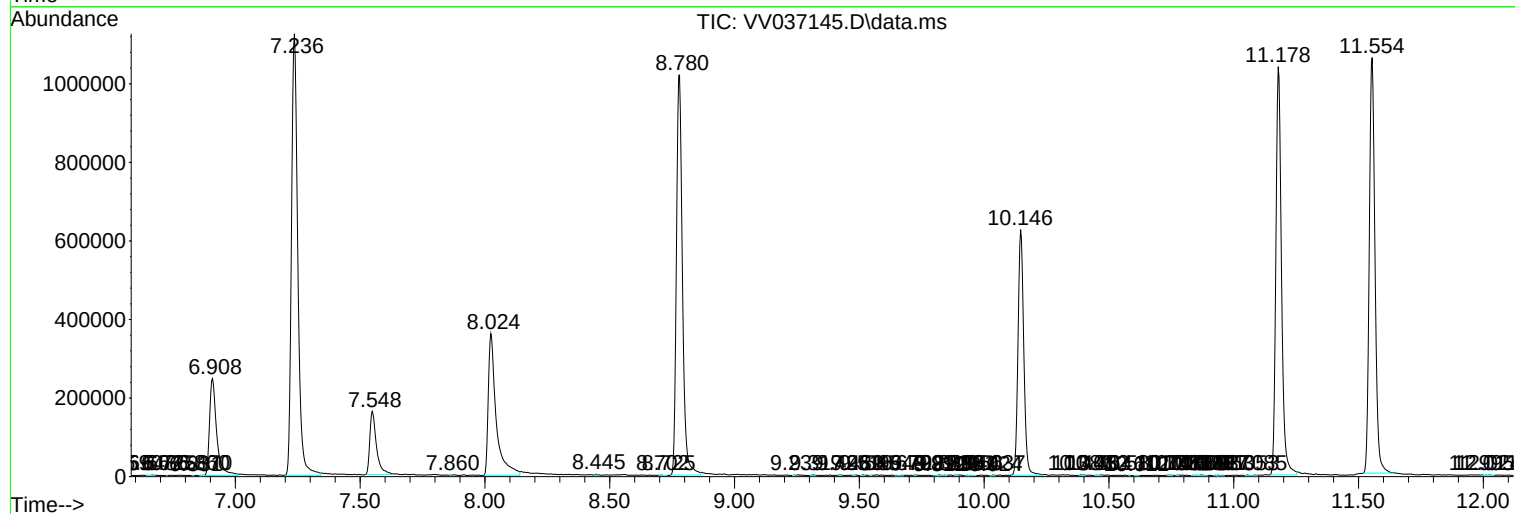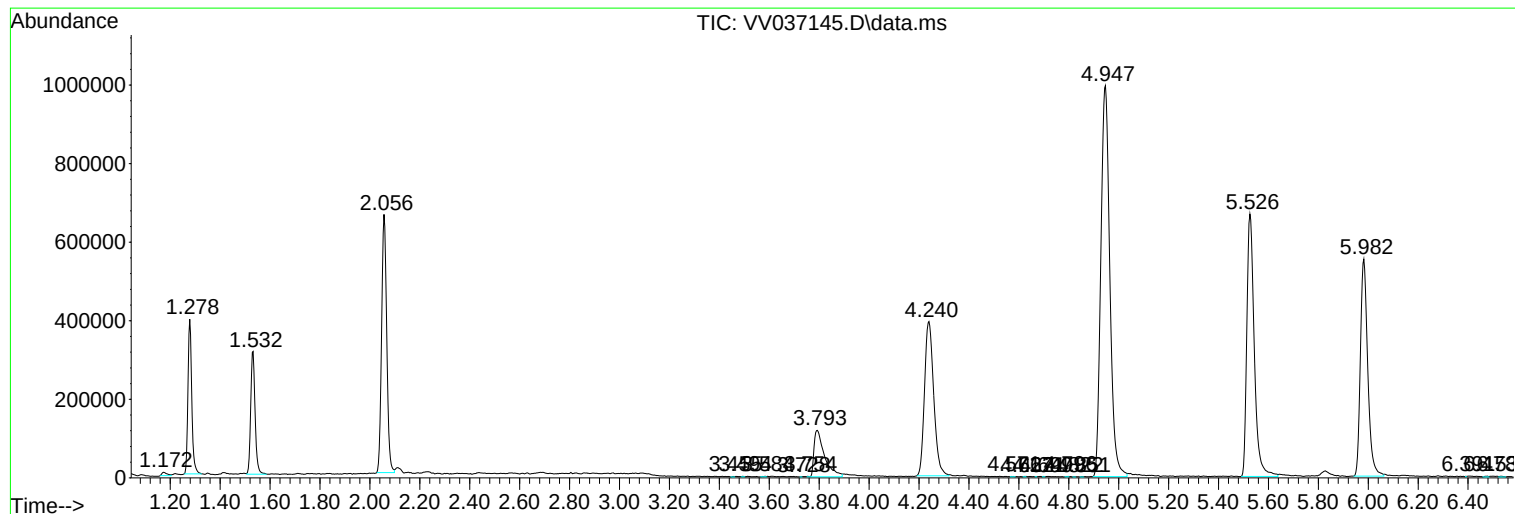

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037145.D
Acq On : 29 Aug 2024 10:45
Operator : SY/MD
Sample : P3734-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44B2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037145.D
Acq On : 29 Aug 2024 10:45
Operator : SY/MD
Sample : P3734-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A44B2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc