

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037151.D
 Acq On : 29 Aug 2024 12:55
 Operator : SY/MD
 Sample : VIBLK365
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	51	rBV	6698	10785	0.43%	0.059%
2	1.278	68	74	92	rVB	385415	406938	16.33%	2.245%
3	1.532	146	153	171	rVB	307468	366259	14.69%	2.020%
4	2.060	308	317	342	rVB	633907	921079	36.95%	5.081%
5	3.330	709	712	713	rBV3	817	448	0.02%	0.002%
6	3.384	726	729	730	rBV3	1469	811	0.03%	0.004%
7	3.535	775	776	779	rBV2	749	408	0.02%	0.002%
8	3.600	793	796	799	rBV5	1184	706	0.03%	0.004%
9	3.696	821	826	829	rBV5	1334	1273	0.05%	0.007%
10	3.799	848	858	895	rBV2	126843	366874	14.72%	2.024%
11	4.134	960	962	967	rBV5	1401	920	0.04%	0.005%
12	4.246	978	997	1027	rBV	386354	998020	40.04%	5.505%
13	4.555	1091	1093	1098	rVB5	1381	793	0.03%	0.004%
14	4.577	1098	1100	1102	rBV3	1150	537	0.02%	0.003%
15	4.735	1145	1149	1152	rBV5	688	625	0.03%	0.003%
16	4.757	1154	1156	1159	rBV3	871	562	0.02%	0.003%
17	4.879	1192	1194	1196	rVB2	1513	578	0.02%	0.003%
18	4.896	1197	1199	1201	rBV3	918	392	0.02%	0.002%
19	4.950	1201	1216	1252	rBV2	991910	2492698	100.00%	13.750%
20	5.368	1343	1346	1349	rBV4	1260	818	0.03%	0.005%
21	5.529	1385	1396	1430	rBV	685942	1427809	57.28%	7.876%
22	5.934	1520	1522	1524	rBV3	1241	624	0.03%	0.003%
23	5.986	1526	1538	1566	rVV	552393	1126428	45.19%	6.214%
24	6.291	1629	1633	1635	rBV5	1341	1081	0.04%	0.006%
25	6.323	1640	1643	1646	rBV5	1138	898	0.04%	0.005%
26	6.384	1660	1662	1665	rBV3	1125	602	0.02%	0.003%
27	6.458	1683	1685	1689	rBV5	840	544	0.02%	0.003%
28	6.558	1714	1716	1719	rVB2	1134	521	0.02%	0.003%
29	6.613	1731	1733	1736	rBV3	1227	891	0.04%	0.005%
30	6.629	1736	1738	1741	rVV4	1240	615	0.02%	0.003%
31	6.645	1741	1743	1747	rVB4	1110	567	0.02%	0.003%
32	6.670	1747	1751	1754	rBV6	1311	1004	0.04%	0.006%
33	6.686	1754	1756	1758	rBV3	1015	482	0.02%	0.003%
34	6.719	1762	1766	1769	rBV6	939	827	0.03%	0.005%
35	6.767	1778	1781	1785	rVB6	1358	1141	0.05%	0.006%
36	6.789	1786	1788	1792	rBV5	1026	619	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037151.D
 Acq On : 29 Aug 2024 12:55
 Operator : SY/MD
 Sample : VIBLK365
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.809	1792	1794	1798	rVV4	1279	808	0.03%	0.004%
38	6.828	1798	1800	1807	rVB8	936	689	0.03%	0.004%
39	6.912	1815	1826	1853	rBV	284708	542453	21.76%	2.992%
40	7.239	1916	1928	1960	rBV	1119882	1979554	79.41%	10.920%
41	7.551	2016	2025	2052	rBV	183218	345341	13.85%	1.905%
42	7.793	2098	2100	2108	rVB7	2611	2412	0.10%	0.013%
43	7.905	2133	2135	2136	rBV2	1467	792	0.03%	0.004%
44	7.950	2147	2149	2151	rVB2	1217	515	0.02%	0.003%
45	7.966	2151	2154	2156	rBV2	1282	777	0.03%	0.004%
46	7.979	2156	2158	2160	rBV4	885	549	0.02%	0.003%
47	8.024	2164	2172	2215	rBV	382644	821060	32.94%	4.529%
48	8.654	2366	2368	2372	rBV6	1229	857	0.03%	0.005%
49	8.780	2396	2407	2438	rBV	1071916	1773992	71.17%	9.786%
50	9.291	2564	2566	2567	rBV2	909	392	0.02%	0.002%
51	9.329	2576	2578	2581	rBV4	1142	541	0.02%	0.003%
52	9.346	2581	2583	2586	rVB4	1159	610	0.02%	0.003%
53	9.458	2615	2618	2619	rBV	1225	727	0.03%	0.004%
54	9.490	2624	2628	2632	rVV7	1562	1208	0.05%	0.007%
55	9.522	2632	2638	2642	rVV7	1302	1489	0.06%	0.008%
56	9.542	2642	2644	2647	rVB3	1356	676	0.03%	0.004%
57	9.606	2661	2664	2667	rBV6	916	579	0.02%	0.003%
58	9.638	2668	2674	2675	rBV4	799	734	0.03%	0.004%
59	9.699	2688	2693	2695	rBV5	901	698	0.03%	0.004%
60	9.780	2716	2718	2720	rBV3	762	390	0.02%	0.002%
61	9.805	2724	2726	2728	rVV3	817	480	0.02%	0.003%
62	9.834	2731	2735	2740	rVB6	2020	1964	0.08%	0.011%
63	9.873	2742	2747	2751	rVB7	1360	1252	0.05%	0.007%
64	9.889	2751	2752	2755	rVB3	1102	458	0.02%	0.003%
65	9.911	2755	2759	2761	rBV5	1000	876	0.04%	0.005%
66	10.027	2792	2795	2797	rBV4	1555	1064	0.04%	0.006%
67	10.056	2801	2804	2806	rBV2	1380	822	0.03%	0.005%
68	10.095	2813	2816	2818	rBV4	1024	660	0.03%	0.004%
69	10.149	2821	2833	2851	rVV	640587	1029831	41.31%	5.681%
70	10.419	2914	2917	2921	rVB4	1163	942	0.04%	0.005%
71	10.442	2921	2924	2927	rBV3	1181	920	0.04%	0.005%
72	10.474	2932	2934	2935	rBV3	1056	479	0.02%	0.003%
73	10.484	2935	2937	2939	rVB3	1464	718	0.03%	0.004%
74	10.571	2961	2964	2969	rBV6	1175	983	0.04%	0.005%
75	10.590	2969	2970	2975	rVB3	1494	978	0.04%	0.005%
76	10.616	2975	2978	2979	rBV3	649	393	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037151.D
 Acq On : 29 Aug 2024 12:55
 Operator : SY/MD
 Sample : VIBLK365
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	10.651	2986	2989	2991	rBV3	721	454	0.02%	0.003%
78	10.773	3025	3027	3028	rBV2	682	388	0.02%	0.002%
79	10.876	3056	3059	3060	rBV3	707	394	0.02%	0.002%
80	10.924	3072	3074	3076	rBV2	1004	440	0.02%	0.002%
81	10.972	3086	3089	3093	rBV5	709	643	0.03%	0.004%
82	11.014	3099	3102	3105	rBV4	663	607	0.02%	0.003%
83	11.030	3105	3107	3108	rVV2	976	378	0.02%	0.002%
84	11.069	3114	3119	3121	rBV5	781	615	0.02%	0.003%
85	11.114	3130	3133	3134	rBV3	1111	526	0.02%	0.003%
86	11.178	3143	3153	3181	rBV	1066849	1716345	68.85%	9.468%
87	11.554	3259	3270	3293	rBV	1077127	1743017	69.92%	9.615%
88	11.911	3379	3381	3382	rBV2	1664	704	0.03%	0.004%
89	12.143	3451	3453	3455	rBV3	997	420	0.02%	0.002%
90	12.329	3508	3511	3512	rBV3	1158	707	0.03%	0.004%
91	12.394	3529	3531	3534	rVB4	2125	974	0.04%	0.005%
92	12.416	3535	3538	3541	rVB3	985	503	0.02%	0.003%
93	12.452	3547	3549	3551	rBV3	1149	559	0.02%	0.003%
94	12.943	3700	3702	3707	rVB6	1423	798	0.03%	0.004%
95	13.069	3739	3741	3744	rVB2	1168	411	0.02%	0.002%
96	13.599	3904	3906	3909	rBV4	932	463	0.02%	0.003%
97	13.619	3909	3912	3914	rBV4	930	619	0.02%	0.003%
98	13.866	3987	3989	3993	rBV5	1069	665	0.03%	0.004%
99	14.226	4099	4101	4103	rBV3	1126	416	0.02%	0.002%
100	14.426	4161	4163	4164	rBV	1040	396	0.02%	0.002%




Sum of corrected areas: 18128282

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037151.D
Acq On : 29 Aug 2024 12:55
Operator : SY/MD
Sample : VIBLK365
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

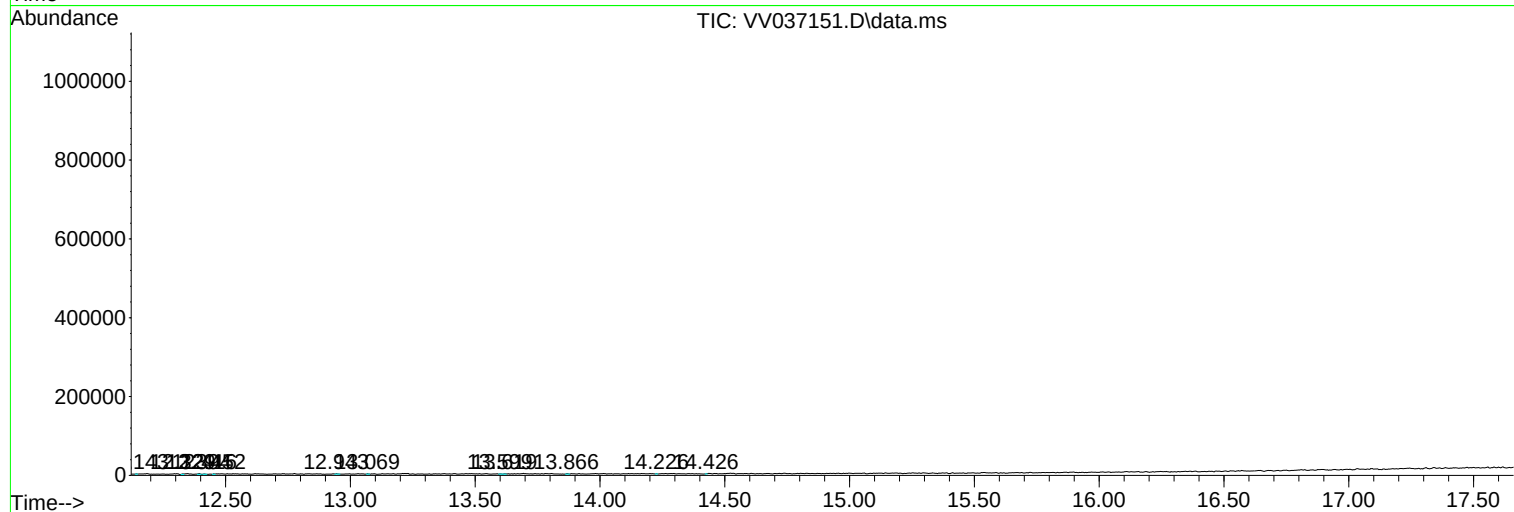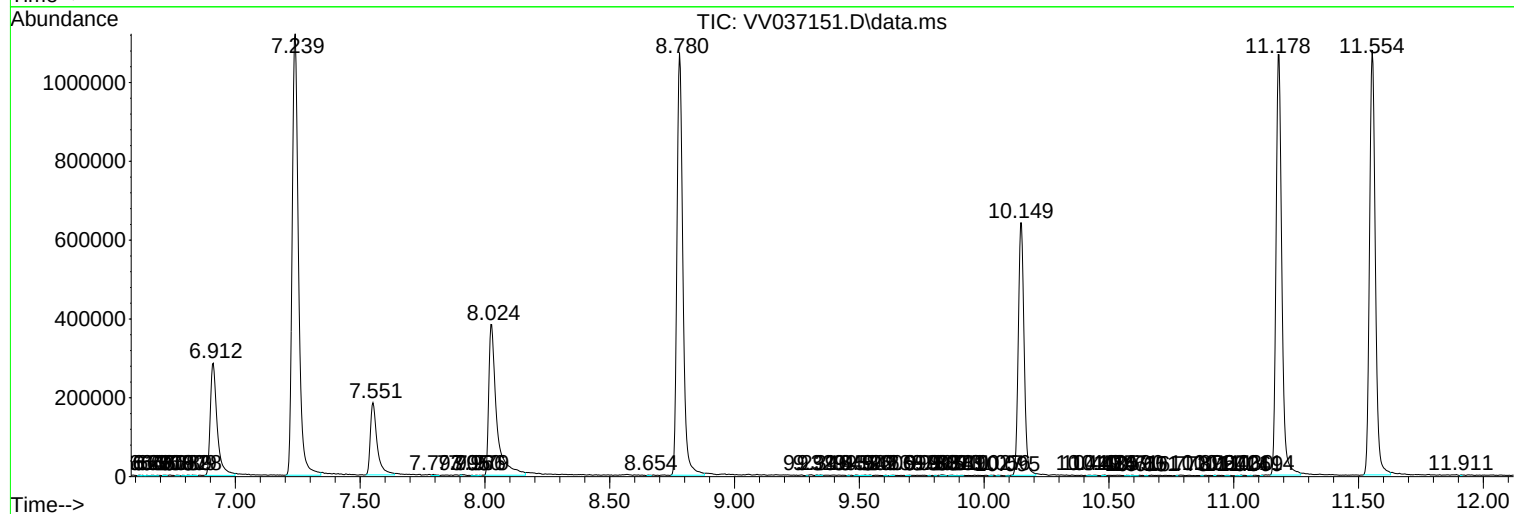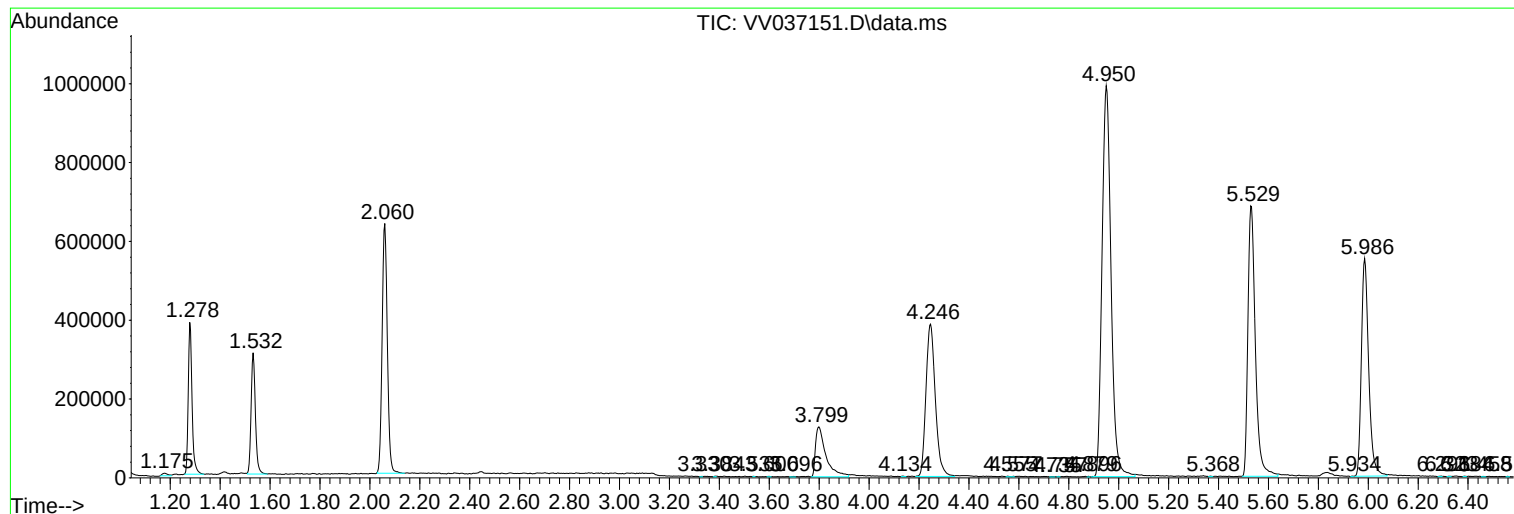

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037151.D
Acq On : 29 Aug 2024 12:55
Operator : SY/MD
Sample : VIBLK365
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037151.D
Acq On : 29 Aug 2024 12:55
Operator : SY/MD
Sample : VIBLK365
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------