

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037153.D
 Acq On : 29 Aug 2024 13:39
 Operator : SY/MD
 Sample : VIBLK366
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	356654	377942	15.39%	2.133%
2	1.532	146	153	167	rVB	294325	346257	14.10%	1.955%
3	2.059	308	317	337	rVB	608160	871779	35.50%	4.921%
4	3.516	767	770	771	rBV3	869	454	0.02%	0.003%
5	3.609	796	799	800	rBV2	1193	639	0.03%	0.004%
6	3.712	826	831	834	rBV5	1362	1252	0.05%	0.007%
7	3.731	834	837	839	rBV4	853	483	0.02%	0.003%
8	3.757	843	845	847	rBV2	1033	389	0.02%	0.002%
9	3.799	849	858	883	rBV	130504	357213	14.55%	2.016%
10	4.246	982	997	1027	rBV	380066	961776	39.17%	5.429%
11	4.542	1084	1089	1091	rBV5	1278	1250	0.05%	0.007%
12	4.696	1135	1137	1138	rBV2	1394	623	0.03%	0.004%
13	4.725	1144	1146	1148	rBV2	1006	582	0.02%	0.003%
14	4.796	1166	1168	1170	rVB2	955	367	0.01%	0.002%
15	4.818	1173	1175	1176	rBV2	619	318	0.01%	0.002%
16	4.892	1196	1198	1200	rBV3	561	258	0.01%	0.001%
17	4.950	1200	1216	1250	rBV3	984149	2455630	100.00%	13.861%
18	5.532	1385	1397	1429	rBV	663835	1379788	56.19%	7.789%
19	5.985	1526	1538	1568	rBV	536970	1115019	45.41%	6.294%
20	6.394	1661	1665	1668	rBV4	1079	977	0.04%	0.006%
21	6.458	1683	1685	1686	rBV2	1129	336	0.01%	0.002%
22	6.522	1701	1705	1712	rBV7	2018	2595	0.11%	0.015%
23	6.673	1750	1752	1755	rVB4	1613	616	0.03%	0.003%
24	6.686	1755	1756	1760	rBV2	424	261	0.01%	0.001%
25	6.712	1762	1764	1765	rBV2	1179	543	0.02%	0.003%
26	6.834	1799	1802	1803	rBV3	795	460	0.02%	0.003%
27	6.911	1816	1826	1855	rBV	272017	530142	21.59%	2.993%
28	7.239	1917	1928	1966	rBV	1077256	1920617	78.21%	10.841%
29	7.551	2016	2025	2045	rBV	180704	331449	13.50%	1.871%
30	7.953	2145	2150	2153	rBV6	1335	1218	0.05%	0.007%
31	8.027	2164	2173	2216	rBV2	402333	850187	34.62%	4.799%
32	8.625	2357	2359	2363	rVB3	1005	565	0.02%	0.003%
33	8.644	2363	2365	2367	rBV3	1205	531	0.02%	0.003%
34	8.715	2385	2387	2392	rVB6	1837	1289	0.05%	0.007%
35	8.738	2392	2394	2395	rBV2	783	364	0.01%	0.002%
36	8.779	2396	2407	2434	rBV	1037893	1725050	70.25%	9.737%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037153.D
 Acq On : 29 Aug 2024 13:39
 Operator : SY/MD
 Sample : VIBLK366
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.236	2547	2549	2550	rBV3	853	327	0.01%	0.002%
38	9.352	2580	2585	2589	rBV6	1051	1050	0.04%	0.006%
39	9.387	2593	2596	2603	rVB6	1466	1406	0.06%	0.008%
40	9.439	2606	2612	2617	rBV9	2314	2816	0.11%	0.016%
41	9.464	2617	2620	2622	rBV4	1003	676	0.03%	0.004%
42	9.522	2636	2638	2640	rBV2	702	429	0.02%	0.002%
43	9.590	2656	2659	2662	rBV4	1257	861	0.04%	0.005%
44	9.638	2671	2674	2677	rVB6	1610	962	0.04%	0.005%
45	9.654	2677	2679	2681	rBV2	1519	491	0.02%	0.003%
46	9.699	2691	2693	2696	rVB3	708	449	0.02%	0.003%
47	9.718	2696	2699	2701	rVB4	1311	547	0.02%	0.003%
48	9.738	2701	2705	2709	rBV5	1779	1794	0.07%	0.010%
49	9.760	2709	2712	2714	rBV3	1131	611	0.02%	0.003%
50	9.818	2729	2730	2732	rBV2	932	296	0.01%	0.002%
51	9.834	2732	2735	2739	rBV6	1128	1033	0.04%	0.006%
52	9.902	2754	2756	2758	rBV2	601	213	0.01%	0.001%
53	9.927	2761	2764	2765	rBV2	707	453	0.02%	0.003%
54	9.937	2765	2767	2772	rVB5	1248	668	0.03%	0.004%
55	9.963	2772	2775	2776	rBV2	900	270	0.01%	0.002%
56	9.979	2777	2780	2781	rBV2	719	358	0.01%	0.002%
57	10.056	2800	2804	2807	rVB6	965	633	0.03%	0.004%
58	10.072	2807	2809	2810	rBV2	423	163	0.01%	0.001%
59	10.082	2810	2812	2814	rBV3	824	338	0.01%	0.002%
60	10.095	2814	2816	2817	rBV	722	227	0.01%	0.001%
61	10.149	2821	2833	2860	rVV	654769	1044501	42.53%	5.896%
62	10.291	2876	2877	2879	rBV2	1018	354	0.01%	0.002%
63	10.422	2914	2918	2922	rBV5	1763	1387	0.06%	0.008%
64	10.464	2927	2931	2937	rBV8	1032	1267	0.05%	0.007%
65	10.493	2937	2940	2944	rBV6	1203	1113	0.05%	0.006%
66	10.709	3002	3007	3012	rVB6	1277	1624	0.07%	0.009%
67	10.731	3012	3014	3015	rBV2	697	245	0.01%	0.001%
68	10.750	3018	3020	3021	rBV2	643	256	0.01%	0.001%
69	10.770	3025	3026	3028	rBV2	837	304	0.01%	0.002%
70	10.812	3037	3039	3041	rBV3	1107	575	0.02%	0.003%
71	10.866	3054	3056	3057	rBV2	945	365	0.01%	0.002%
72	10.908	3067	3069	3071	rBV3	767	290	0.01%	0.002%
73	10.947	3079	3081	3086	rVB4	1446	973	0.04%	0.005%
74	10.969	3086	3088	3090	rBV2	931	367	0.01%	0.002%
75	10.982	3090	3092	3093	rVB2	1039	322	0.01%	0.002%
76	10.988	3093	3094	3096	rVB2	377	143	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037153.D
 Acq On : 29 Aug 2024 13:39
 Operator : SY/MD
 Sample : VIBLK366
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.011	3096	3101	3102	rBV3	1346	1011	0.04%	0.006%
78	11.046	3109	3112	3115	rVB5	933	596	0.02%	0.003%
79	11.078	3115	3122	3126	rBV6	1467	2078	0.08%	0.012%
80	11.101	3126	3129	3131	rBV3	974	649	0.03%	0.004%
81	11.181	3143	3154	3185	rBV	1055108	1671512	68.07%	9.435%
82	11.554	3259	3270	3299	rBV	1066022	1714322	69.81%	9.677%
83	11.966	3394	3398	3400	rBV3	2313	1633	0.07%	0.009%
84	12.082	3431	3434	3439	rBV6	1746	1159	0.05%	0.007%
85	12.139	3451	3452	3455	rBV4	757	381	0.02%	0.002%
86	12.249	3483	3486	3489	rBV4	966	834	0.03%	0.005%
87	12.274	3489	3494	3501	rVV9	1874	2719	0.11%	0.015%
88	12.448	3544	3548	3550	rBV3	1256	913	0.04%	0.005%
89	12.619	3599	3601	3608	rVB6	1492	1292	0.05%	0.007%
90	12.657	3608	3613	3614	rBV4	1217	930	0.04%	0.005%
91	12.789	3652	3654	3656	rVB3	898	286	0.01%	0.002%
92	12.953	3703	3705	3707	rVB2	950	382	0.02%	0.002%
93	12.982	3712	3714	3717	rBV4	903	492	0.02%	0.003%
94	13.014	3720	3724	3725	rBV3	1208	781	0.03%	0.004%
95	13.024	3725	3727	3730	rBV4	956	597	0.02%	0.003%
96	13.117	3750	3756	3760	rBV6	1580	1752	0.07%	0.010%
97	13.525	3882	3883	3887	rVB4	754	385	0.02%	0.002%
98	13.676	3928	3930	3931	rBV2	1447	558	0.02%	0.003%




Sum of corrected areas: 17715638

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037153.D
Acq On : 29 Aug 2024 13:39
Operator : SY/MD
Sample : VIBLK366
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

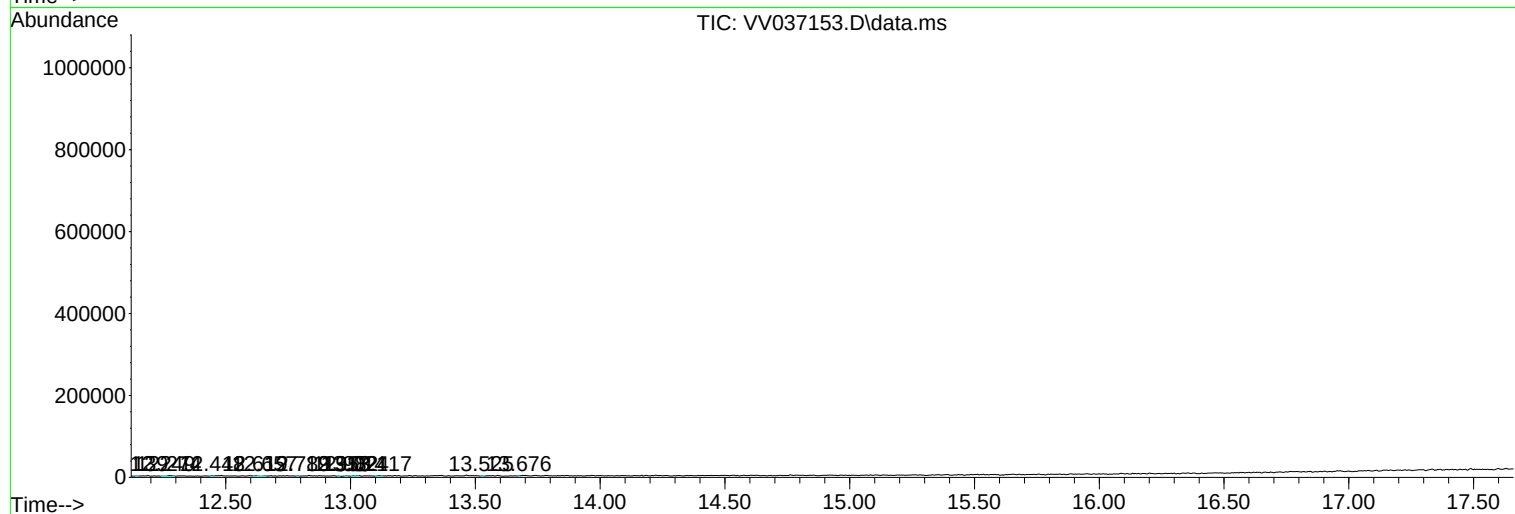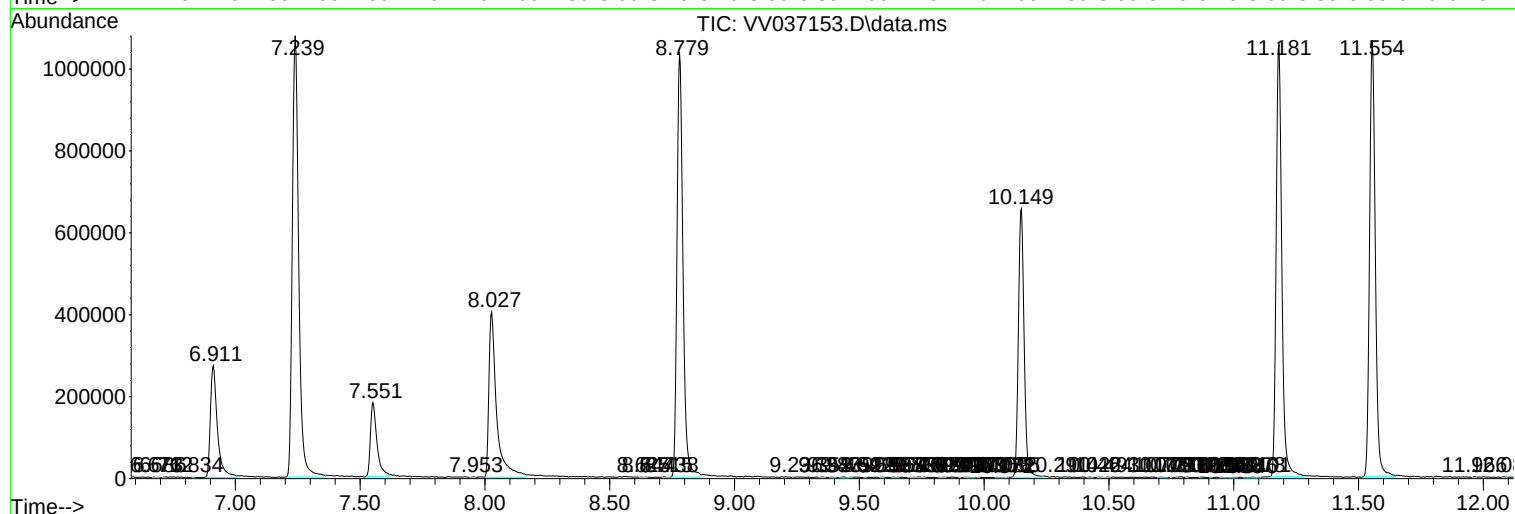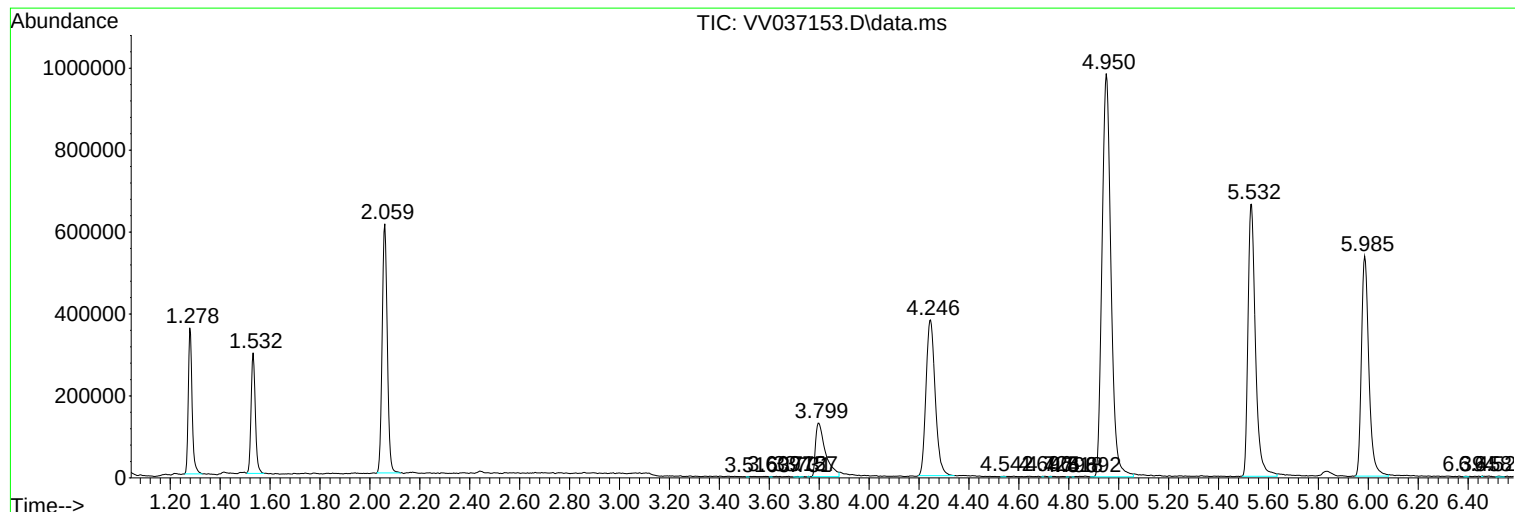

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037153.D
Acq On : 29 Aug 2024 13:39
Operator : SY/MD
Sample : VIBLK366
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037153.D
Acq On : 29 Aug 2024 13:39
Operator : SY/MD
Sample : VIBLK366
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc