

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037155.D
 Acq On : 29 Aug 2024 14:22
 Operator : SY/MD
 Sample : VIBLK367
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK367

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	372641	403938	15.77%	2.194%
2	1.532	146	153	169	rVB	320810	374666	14.63%	2.035%
3	2.059	308	317	334	rBV	651553	926366	36.16%	5.031%
4	3.400	732	734	739	rVB4	783	471	0.02%	0.003%
5	3.497	761	764	768	rBV4	1544	1032	0.04%	0.006%
6	3.516	768	770	773	rVV4	1076	784	0.03%	0.004%
7	3.548	776	780	784	rBV6	1102	1044	0.04%	0.006%
8	3.612	798	800	804	rVB5	1380	750	0.03%	0.004%
9	3.712	827	831	834	rBV5	1131	953	0.04%	0.005%
10	3.731	834	837	840	rBV4	957	818	0.03%	0.004%
11	3.799	849	858	883	rBV	130882	356278	13.91%	1.935%
12	4.111	952	955	956	rBV3	1352	614	0.02%	0.003%
13	4.246	979	997	1028	rBV	392037	1007362	39.33%	5.471%
14	4.465	1063	1065	1067	rVB3	1341	526	0.02%	0.003%
15	4.477	1067	1069	1071	rVB2	1229	501	0.02%	0.003%
16	4.490	1071	1073	1075	rBV4	890	489	0.02%	0.003%
17	4.506	1075	1078	1082	rBV4	1167	764	0.03%	0.004%
18	4.638	1116	1119	1121	rBV4	892	579	0.02%	0.003%
19	4.680	1129	1132	1135	rBV3	1003	789	0.03%	0.004%
20	4.731	1145	1148	1154	rVB6	1252	1050	0.04%	0.006%
21	4.809	1168	1172	1174	rBV4	1029	883	0.03%	0.005%
22	4.857	1181	1187	1189	rBV6	1577	1528	0.06%	0.008%
23	4.950	1199	1216	1250	rBV2	1009017	2561571	100.00%	13.913%
24	5.262	1311	1313	1315	rBV2	1406	777	0.03%	0.004%
25	5.297	1322	1324	1327	rVB4	1709	690	0.03%	0.004%
26	5.529	1385	1396	1423	rBV	705753	1445042	56.41%	7.849%
27	5.985	1525	1538	1564	rBV	553504	1143923	44.66%	6.213%
28	6.346	1648	1650	1652	rBV3	1586	811	0.03%	0.004%
29	6.439	1676	1679	1682	rBV4	786	593	0.02%	0.003%
30	6.458	1682	1685	1689	rVV6	1108	747	0.03%	0.004%
31	6.481	1689	1692	1694	rVV4	1631	854	0.03%	0.005%
32	6.538	1703	1710	1714	rBV6	1843	2579	0.10%	0.014%
33	6.625	1734	1737	1742	rVB6	1218	1036	0.04%	0.006%
34	6.648	1742	1744	1747	rBV2	1930	1085	0.04%	0.006%
35	6.776	1782	1784	1790	rVB4	2326	1389	0.05%	0.008%
36	6.802	1790	1792	1794	rBV3	821	442	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037155.D
 Acq On : 29 Aug 2024 14:22
 Operator : SY/MD
 Sample : VIBLK367
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK367

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.821	1796	1798	1805	rVB7	1839	1730	0.07%	0.009%
38	6.854	1805	1808	1811	rBV5	848	704	0.03%	0.004%
39	6.911	1811	1826	1851	rBV	285388	546911	21.35%	2.970%
40	7.153	1898	1901	1902	rBV3	1003	493	0.02%	0.003%
41	7.239	1917	1928	1959	rBV	1134845	1991835	77.76%	10.818%
42	7.551	2016	2025	2054	rBV	186248	342128	13.36%	1.858%
43	7.773	2092	2094	2097	rBV4	1340	1035	0.04%	0.006%
44	8.027	2164	2173	2221	rBV2	408759	871195	34.01%	4.732%
45	8.779	2393	2407	2435	rBV	1093417	1803420	70.40%	9.795%
46	9.191	2533	2535	2537	rBV3	1391	718	0.03%	0.004%
47	9.262	2555	2557	2560	rBV4	1002	576	0.02%	0.003%
48	9.304	2568	2570	2572	rBV4	1043	601	0.02%	0.003%
49	9.390	2595	2597	2601	rBV5	1390	1009	0.04%	0.005%
50	9.413	2601	2604	2606	rBV5	1107	715	0.03%	0.004%
51	9.480	2621	2625	2628	rBV4	1292	1083	0.04%	0.006%
52	9.644	2674	2676	2678	rBV2	1273	517	0.02%	0.003%
53	9.683	2684	2688	2689	rBV3	931	616	0.02%	0.003%
54	9.715	2696	2698	2702	rVB4	1858	1144	0.04%	0.006%
55	9.734	2702	2704	2706	rBV3	1512	802	0.03%	0.004%
56	9.773	2712	2716	2717	rBV4	794	555	0.02%	0.003%
57	9.857	2736	2742	2745	rBV8	2225	2125	0.08%	0.012%
58	9.889	2749	2752	2754	rVB3	811	488	0.02%	0.003%
59	9.908	2754	2758	2761	rBV4	1232	925	0.04%	0.005%
60	9.931	2761	2765	2767	rBV6	1122	931	0.04%	0.005%
61	10.017	2789	2792	2793	rBV3	1138	666	0.03%	0.004%
62	10.082	2809	2812	2816	rBV5	1086	967	0.04%	0.005%
63	10.149	2821	2833	2854	rBV	651632	1051049	41.03%	5.709%
64	10.342	2891	2893	2899	rBV7	944	818	0.03%	0.004%
65	10.374	2899	2903	2904	rBV4	1149	707	0.03%	0.004%
66	10.413	2910	2915	2916	rBV5	1042	788	0.03%	0.004%
67	10.471	2927	2933	2934	rBV4	1268	1119	0.04%	0.006%
68	10.538	2953	2954	2958	rBV4	963	513	0.02%	0.003%
69	10.615	2976	2978	2981	rVB3	1129	521	0.02%	0.003%
70	10.657	2986	2991	2992	rBV4	1381	979	0.04%	0.005%
71	10.712	3006	3008	3010	rBV2	957	429	0.02%	0.002%
72	10.779	3025	3029	3030	rBV4	1171	679	0.03%	0.004%
73	10.863	3053	3055	3060	rBV5	1432	1127	0.04%	0.006%
74	10.943	3077	3080	3082	rVB3	865	466	0.02%	0.003%
75	10.959	3082	3085	3090	rBV5	1344	1149	0.04%	0.006%
76	11.021	3099	3104	3105	rBV5	1237	931	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037155.D
 Acq On : 29 Aug 2024 14:22
 Operator : SY/MD
 Sample : VIBLK367
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK367

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.101	3126	3129	3131	rBV3	860	521	0.02%	0.003%
78	11.181	3143	3154	3182	rBV	1079189	1714090	66.92%	9.310%
79	11.554	3258	3270	3297	rBV	1103821	1751530	68.38%	9.513%
80	11.918	3380	3383	3385	rBV5	934	543	0.02%	0.003%
81	11.930	3385	3387	3391	rVV5	1339	937	0.04%	0.005%
82	12.053	3423	3425	3428	rVB3	1260	651	0.03%	0.004%
83	12.217	3474	3476	3480	rBV3	1136	1065	0.04%	0.006%
84	12.242	3482	3484	3487	rVB3	1400	680	0.03%	0.004%
85	12.307	3501	3504	3508	rBV3	1365	1519	0.06%	0.008%
86	12.368	3520	3523	3527	rBV5	1785	1358	0.05%	0.007%
87	12.400	3531	3533	3536	rBV4	680	437	0.02%	0.002%
88	12.564	3581	3584	3586	rBV4	1355	944	0.04%	0.005%
89	12.693	3618	3624	3627	rBV8	1100	1216	0.05%	0.007%
90	12.738	3635	3638	3641	rBV3	1332	956	0.04%	0.005%
91	12.783	3650	3652	3655	rBV2	967	631	0.02%	0.003%
92	12.979	3710	3713	3714	rBV2	1115	600	0.02%	0.003%
93	13.117	3752	3756	3759	rBV6	1246	894	0.03%	0.005%
94	13.162	3765	3770	3773	rBV7	1313	1210	0.05%	0.007%
95	13.236	3790	3793	3794	rBV2	1016	588	0.02%	0.003%
96	13.310	3814	3816	3819	rVB2	1006	442	0.02%	0.002%
97	13.355	3822	3830	3843	rBV4	12598	30933	1.21%	0.168%
98	13.651	3912	3922	3927	rBV5	9903	18541	0.72%	0.101%
99	14.027	4036	4039	4042	rBV3	1697	1606	0.06%	0.009%
100	14.348	4136	4139	4140	rBV2	1267	804	0.03%	0.004%




Sum of corrected areas: 18411584

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037155.D
Acq On : 29 Aug 2024 14:22
Operator : SY/MD
Sample : VIBLK367
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK367

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

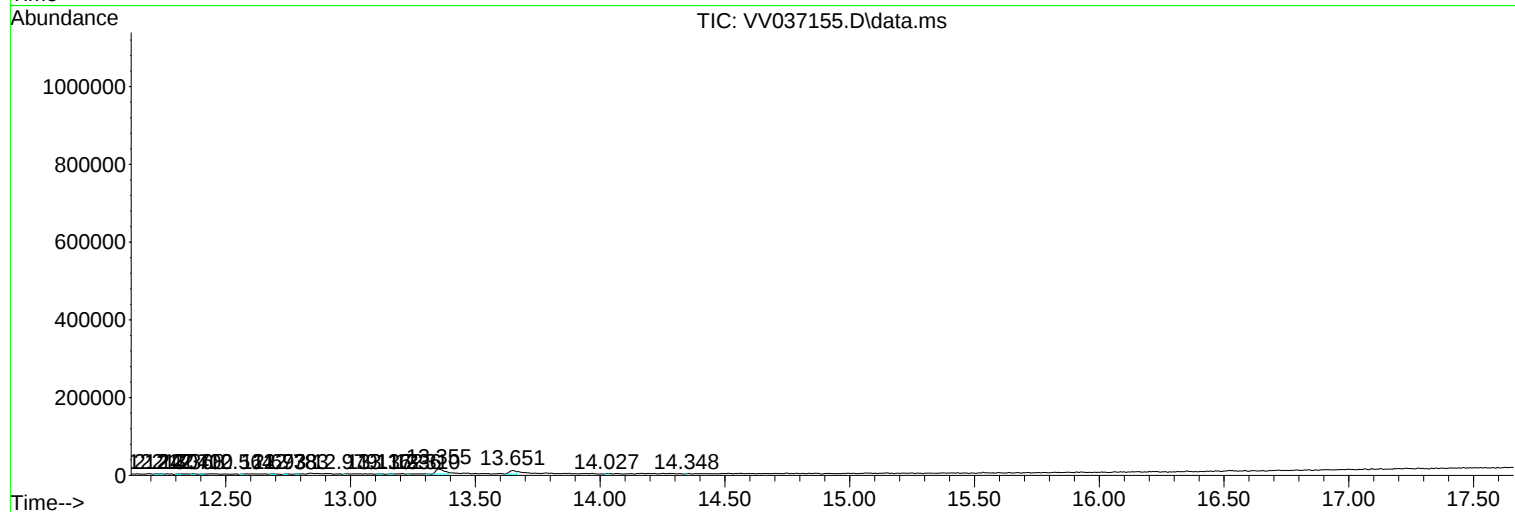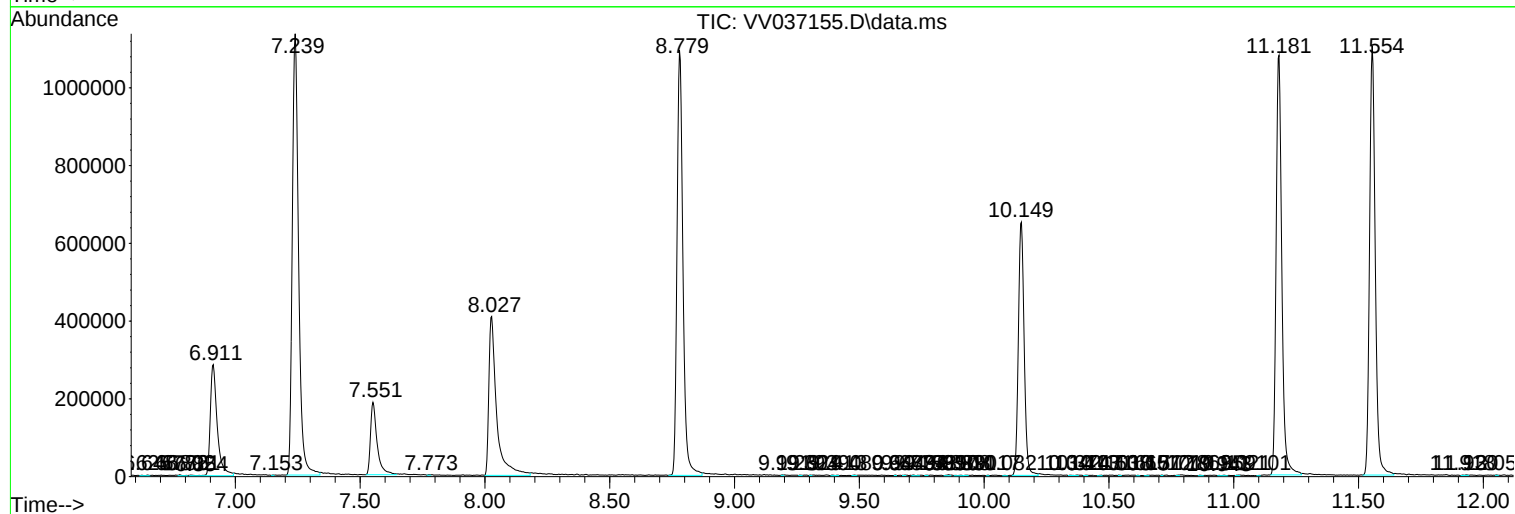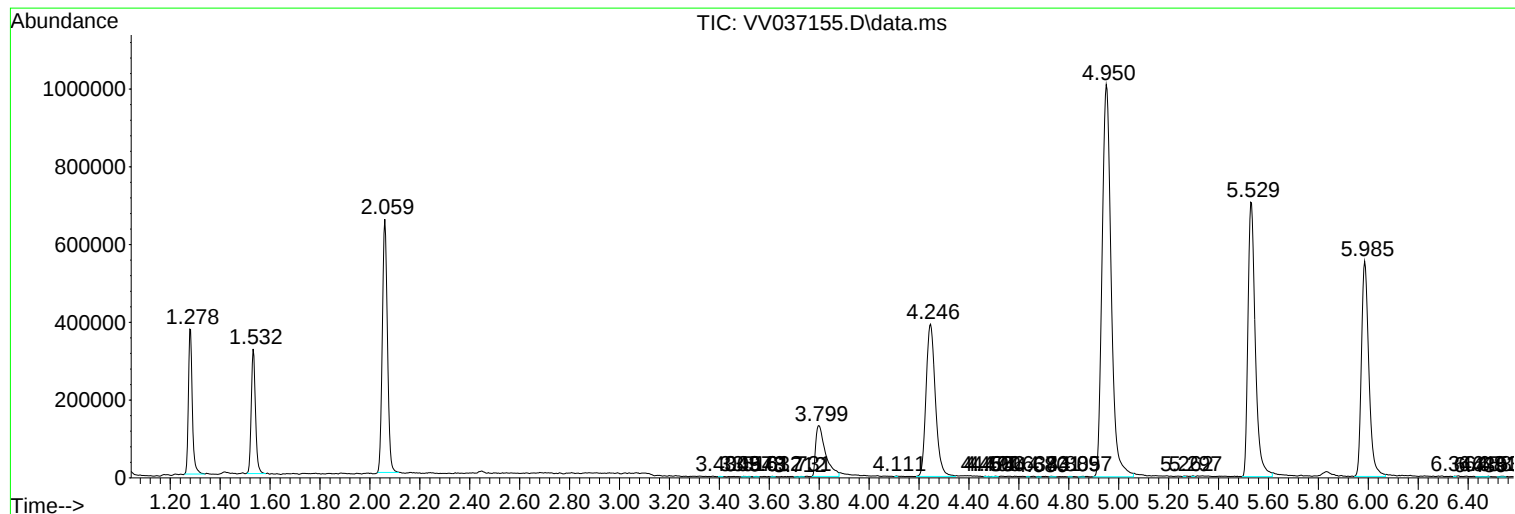

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037155.D
Acq On : 29 Aug 2024 14:22
Operator : SY/MD
Sample : VIBLK367
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK367

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037155.D
Acq On : 29 Aug 2024 14:22
Operator : SY/MD
Sample : VIBLK367
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK367

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc