

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037156.D
 Acq On : 29 Aug 2024 14:44
 Operator : SY/MD
 Sample : P3692-20
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037156.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	94	rBV2	722016	803926	2.97%	1.774%
2	1.532	146	153	169	rVB	300646	356381	1.32%	0.786%
3	2.060	308	317	340	rVB	636291	934007	3.45%	2.061%
4	2.690	505	513	536	rVB	196203	331922	1.23%	0.732%
5	3.246	683	686	688	rBV4	1159	823	0.00%	0.002%
6	3.384	726	729	731	rBV4	1346	930	0.00%	0.002%
7	3.423	736	741	744	rBV3	1092	1088	0.00%	0.002%
8	3.577	783	789	793	rBV6	1061	1049	0.00%	0.002%
9	3.593	793	794	796	rVB	563	176	0.00%	0.000%
10	3.603	796	797	798	rBV	405	129	0.00%	0.000%
11	3.619	799	802	804	rBV3	727	458	0.00%	0.001%
12	3.648	809	811	814	rVV4	1229	668	0.00%	0.001%
13	3.664	814	816	818	rVB4	739	240	0.00%	0.001%
14	3.805	842	860	913	rBV	11694717	27074434	100.00%	59.746%
15	4.243	983	996	1024	rVB	382063	958331	3.54%	2.115%
16	4.950	1200	1216	1246	rBV2	977656	2455234	9.07%	5.418%
17	5.458	1372	1374	1375	rBV2	1174	467	0.00%	0.001%
18	5.529	1385	1396	1422	rBV	674249	1384970	5.12%	3.056%
19	5.985	1525	1538	1572	rBV	542592	1122910	4.15%	2.478%
20	6.288	1629	1632	1638	rVB7	1067	1161	0.00%	0.003%
21	6.313	1638	1640	1645	rBV5	1095	841	0.00%	0.002%
22	6.490	1691	1695	1696	rBV3	1054	869	0.00%	0.002%
23	6.632	1736	1739	1742	rBV5	1628	1094	0.00%	0.002%
24	6.667	1748	1750	1752	rBV3	888	354	0.00%	0.001%
25	6.696	1756	1759	1761	rBV3	585	345	0.00%	0.001%
26	6.719	1761	1766	1769	rBV6	1810	1537	0.01%	0.003%
27	6.767	1779	1781	1784	rVB4	1207	586	0.00%	0.001%
28	6.786	1784	1787	1789	rBV2	1095	683	0.00%	0.002%
29	6.818	1795	1797	1804	rVB7	1606	1466	0.01%	0.003%
30	6.847	1804	1806	1807	rBV2	691	301	0.00%	0.001%
31	6.873	1811	1814	1815	rBV4	572	392	0.00%	0.001%
32	6.911	1815	1826	1857	rBV	274288	538289	1.99%	1.188%
33	7.239	1917	1928	1954	rBV	1109502	1930985	7.13%	4.261%
34	7.551	2016	2025	2049	rBV	179938	335616	1.24%	0.741%
35	8.027	2164	2173	2211	rBV	409006	846636	3.13%	1.868%
36	8.712	2383	2386	2389	rVB4	1128	868	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037156.D
 Acq On : 29 Aug 2024 14:44
 Operator : SY/MD
 Sample : P3692-20
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.731	2391	2392	2393	rBV	784	211	0.00%	0.000%
38	8.780	2396	2407	2436	rBV	1039372	1724689	6.37%	3.806%
39	9.220	2541	2544	2547	rBV4	1066	1007	0.00%	0.002%
40	9.345	2581	2583	2584	rBV2	1558	588	0.00%	0.001%
41	9.371	2590	2591	2592	rBV	860	273	0.00%	0.001%
42	9.400	2598	2600	2603	rBV3	1127	664	0.00%	0.001%
43	9.455	2614	2617	2620	rBV5	1196	833	0.00%	0.002%
44	9.506	2632	2633	2636	rVB3	858	342	0.00%	0.001%
45	9.529	2638	2640	2643	rBV3	1921	1422	0.01%	0.003%
46	9.580	2655	2656	2657	rBV	889	209	0.00%	0.000%
47	9.686	2687	2689	2691	rBV2	877	312	0.00%	0.001%
48	9.722	2698	2700	2702	rBV4	933	492	0.00%	0.001%
49	9.773	2707	2716	2719	rBV9	1253	1677	0.01%	0.004%
50	9.979	2778	2780	2782	rVB3	694	331	0.00%	0.001%
51	9.998	2782	2786	2789	rVB4	1425	766	0.00%	0.002%
52	10.014	2789	2791	2794	rBV5	1124	796	0.00%	0.002%
53	10.043	2798	2800	2801	rBV2	1190	434	0.00%	0.001%
54	10.149	2821	2833	2857	rBV	660089	1053339	3.89%	2.324%
55	10.619	2976	2979	2980	rBV2	471	230	0.00%	0.001%
56	10.664	2990	2993	2997	rVB5	2417	1742	0.01%	0.004%
57	10.689	2997	3001	3002	rBV4	1345	831	0.00%	0.002%
58	10.789	3026	3032	3037	rBV8	2261	2527	0.01%	0.006%
59	10.818	3037	3041	3043	rVB3	1430	789	0.00%	0.002%
60	10.834	3043	3046	3047	rBV3	1363	591	0.00%	0.001%
61	10.886	3059	3062	3065	rBV5	1018	614	0.00%	0.001%
62	10.918	3070	3072	3075	rBV4	1169	929	0.00%	0.002%
63	10.969	3086	3088	3090	rBV2	583	312	0.00%	0.001%
64	11.056	3111	3115	3116	rBV4	834	656	0.00%	0.001%
65	11.117	3131	3134	3135	rBV2	2806	1715	0.01%	0.004%
66	11.181	3143	3154	3190	rBV	1024397	1668466	6.16%	3.682%
67	11.554	3257	3270	3300	rBV	1078926	1735320	6.41%	3.829%
68	11.879	3366	3371	3375	rBV7	2152	2219	0.01%	0.005%
69	11.995	3404	3407	3410	rBV5	1259	1012	0.00%	0.002%
70	12.011	3410	3412	3414	rVV3	1099	408	0.00%	0.001%
71	12.043	3421	3422	3423	rVB	650	125	0.00%	0.000%
72	12.130	3447	3449	3450	rBV2	595	227	0.00%	0.001%
73	12.146	3450	3454	3455	rBV3	959	426	0.00%	0.001%
74	12.156	3455	3457	3458	rBV2	727	200	0.00%	0.000%
75	12.165	3458	3460	3463	rBV4	1087	791	0.00%	0.002%
76	12.451	3547	3549	3551	rBV2	1150	765	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037156.D
 Acq On : 29 Aug 2024 14:44
 Operator : SY/MD
 Sample : P3692-20
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	12.503	3561	3565	3566	rBV3	985	726	0.00%	0.002%
78	12.548	3577	3579	3580	rBV2	947	330	0.00%	0.001%
79	12.641	3606	3608	3616	rBV8	1249	863	0.00%	0.002%
80	12.709	3627	3629	3632	rBV3	884	578	0.00%	0.001%
81	12.731	3634	3636	3640	rVB5	1395	713	0.00%	0.002%
82	12.766	3645	3647	3648	rBV2	666	224	0.00%	0.000%
83	12.776	3648	3650	3653	rBV3	1387	895	0.00%	0.002%
84	12.860	3673	3676	3678	rBV4	1196	701	0.00%	0.002%
85	12.911	3687	3692	3693	rBV4	1538	1097	0.00%	0.002%
86	13.046	3733	3734	3737	rVB2	591	210	0.00%	0.000%
87	13.255	3797	3799	3801	rBV2	1318	648	0.00%	0.001%
88	13.291	3808	3810	3813	rBV4	885	413	0.00%	0.001%
89	13.657	3917	3924	3926	rBV9	4631	5399	0.02%	0.012%
90	13.795	3965	3967	3968	rBV2	953	355	0.00%	0.001%
91	13.885	3992	3995	3998	rBV3	1431	1120	0.00%	0.002%
92	14.056	4046	4048	4049	rBV2	1249	612	0.00%	0.001%
93	14.509	4184	4189	4192	rBV6	1994	1448	0.01%	0.003%




Sum of corrected areas: 45315778

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037156.D
Acq On : 29 Aug 2024 14:44
Operator : SY/MD
Sample : P3692-20
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

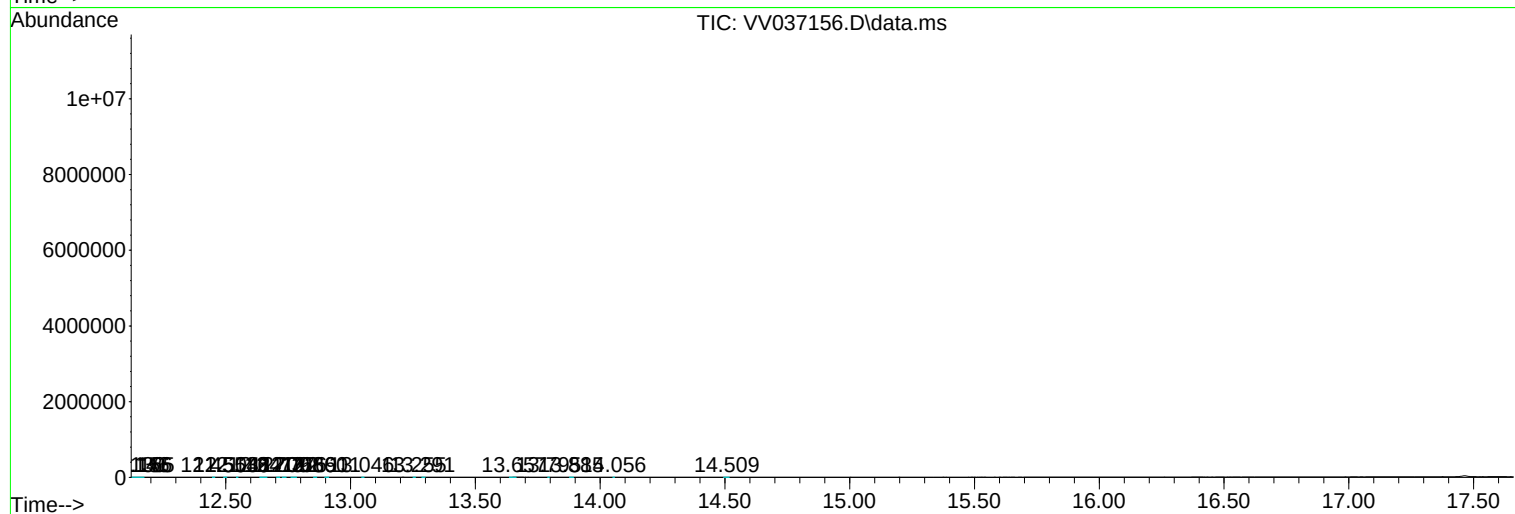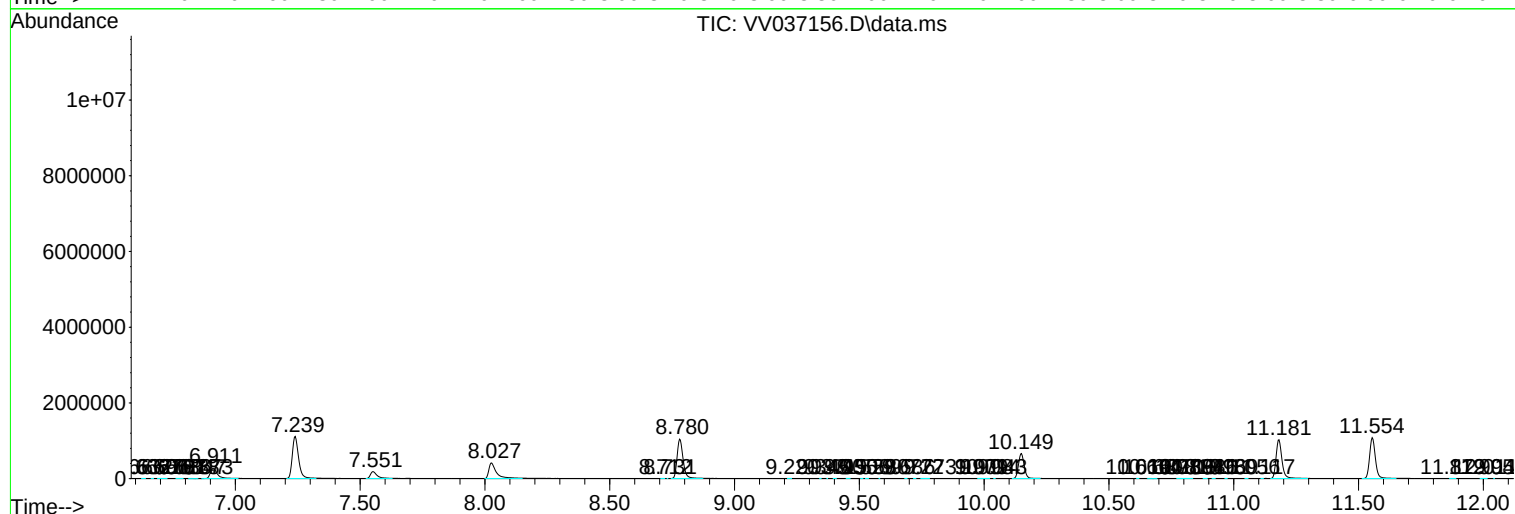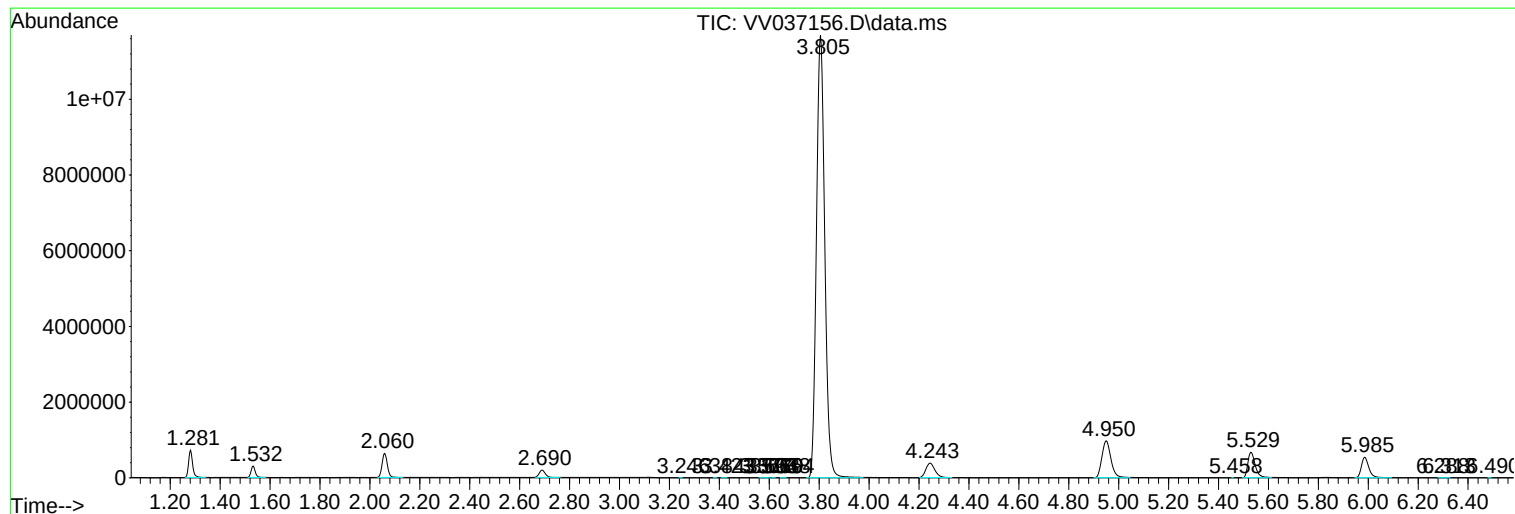

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037156.D
Acq On : 29 Aug 2024 14:44
Operator : SY/MD
Sample : P3692-20
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037156.D
Acq On : 29 Aug 2024 14:44
Operator : SY/MD
Sample : P3692-20
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc