

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037157.D
 Acq On : 29 Aug 2024 15:06
 Operator : SY/MD
 Sample : VIBLK368
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK368

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	386166	397050	16.11%	2.208%
2	1.532	146	153	169	rVB	296865	355595	14.43%	1.977%
3	2.056	307	316	339	rVB	625163	901739	36.59%	5.014%
4	3.423	736	741	742	rBV5	1341	1057	0.04%	0.006%
5	3.474	755	757	759	rVB3	2261	844	0.03%	0.005%
6	3.523	770	772	779	rVB6	1473	1319	0.05%	0.007%
7	3.561	779	784	786	rBV5	1133	988	0.04%	0.005%
8	3.587	790	792	796	rBV4	406	238	0.01%	0.001%
9	3.609	796	799	803	rVB6	1404	1090	0.04%	0.006%
10	3.635	803	807	808	rBV4	806	597	0.02%	0.003%
11	3.706	826	829	830	rBV2	671	344	0.01%	0.002%
12	3.757	843	845	848	rVB3	521	321	0.01%	0.002%
13	3.799	848	858	889	rBV	157945	451373	18.31%	2.510%
14	4.185	973	978	979	rBV2	1404	1205	0.05%	0.007%
15	4.243	982	996	1027	rVV	384592	975032	39.56%	5.421%
16	4.699	1136	1138	1142	rBV6	1075	693	0.03%	0.004%
17	4.757	1154	1156	1159	rBV2	634	346	0.01%	0.002%
18	4.783	1161	1164	1166	rVB4	1491	957	0.04%	0.005%
19	4.841	1180	1182	1185	rBV4	1073	704	0.03%	0.004%
20	4.950	1197	1216	1248	rBV2	978880	2464758	100.00%	13.704%
21	5.378	1346	1349	1351	rBV4	1125	743	0.03%	0.004%
22	5.404	1355	1357	1360	rVB4	1343	591	0.02%	0.003%
23	5.529	1385	1396	1427	rBV	683897	1415484	57.43%	7.870%
24	5.986	1526	1538	1564	rBV	543295	1109165	45.00%	6.167%
25	6.391	1662	1664	1667	rVB5	1071	522	0.02%	0.003%
26	6.510	1699	1701	1703	rVB2	1021	321	0.01%	0.002%
27	6.526	1703	1706	1707	rBV3	1000	632	0.03%	0.004%
28	6.561	1713	1717	1719	rBV4	1049	751	0.03%	0.004%
29	6.654	1744	1746	1747	rBV2	844	366	0.01%	0.002%
30	6.690	1755	1757	1762	rVB5	965	662	0.03%	0.004%
31	6.744	1769	1774	1777	rBV5	1428	1157	0.05%	0.006%
32	6.802	1791	1792	1794	rBV2	537	239	0.01%	0.001%
33	6.825	1797	1799	1803	rBV3	494	328	0.01%	0.002%
34	6.844	1803	1805	1808	rVB3	1103	536	0.02%	0.003%
35	6.860	1808	1810	1811	rBV2	936	488	0.02%	0.003%
36	6.912	1814	1826	1854	rBV	275264	535217	21.71%	2.976%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037157.D
Acq On : 29 Aug 2024 15:06
Operator : SY/MD
Sample : VIBLK368
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK368

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis

37	7.130	1891	1894	1896	rBV4	1453	742	0.03%	0.004%
38	7.240	1917	1928	1959	rBV	1093379	1934706	78.49%	10.757%
39	7.551	2016	2025	2059	rBV	178356	332997	13.51%	1.852%
40	7.995	2162	2163	2164	rBV	919	280	0.01%	0.002%
41	8.024	2164	2172	2210	rVV2	405927	857017	34.77%	4.765%
42	8.696	2376	2381	2382	rBV4	1255	802	0.03%	0.004%
43	8.780	2396	2407	2433	rBV	1058036	1746937	70.88%	9.713%
44	9.362	2586	2588	2590	rBV3	721	407	0.02%	0.002%
45	9.413	2602	2604	2606	rBV4	1379	548	0.02%	0.003%
46	9.436	2606	2611	2613	rBV6	1548	1262	0.05%	0.007%
47	9.452	2613	2616	2619	rBV5	1135	816	0.03%	0.005%
48	9.513	2634	2635	2637	rBV2	875	441	0.02%	0.002%
49	9.603	2658	2663	2664	rBV4	1342	916	0.04%	0.005%
50	9.625	2667	2670	2671	rBV2	868	529	0.02%	0.003%
51	9.674	2682	2685	2688	rBV3	1016	667	0.03%	0.004%
52	9.731	2699	2703	2706	rBV6	1128	920	0.04%	0.005%
53	9.748	2706	2708	2709	rBV2	696	290	0.01%	0.002%
54	9.757	2709	2711	2712	rBV2	767	380	0.02%	0.002%
55	9.799	2717	2724	2732	rBV10	1316	2272	0.09%	0.013%
56	9.831	2732	2734	2736	rBV3	1208	639	0.03%	0.004%
57	9.873	2745	2747	2749	rVB3	1282	550	0.02%	0.003%
58	9.883	2749	2750	2754	rVB4	1026	404	0.02%	0.002%
59	9.956	2771	2773	2776	rBV4	584	393	0.02%	0.002%
60	9.973	2776	2778	2780	rBV3	743	297	0.01%	0.002%
61	10.098	2814	2817	2819	rBV	857	559	0.02%	0.003%
62	10.149	2821	2833	2850	rBV	652084	1030237	41.80%	5.728%
63	10.371	2900	2902	2903	rBV2	953	378	0.02%	0.002%
64	10.468	2930	2932	2934	rBV3	1420	815	0.03%	0.005%
65	10.638	2982	2985	2987	rVB3	1422	600	0.02%	0.003%
66	10.751	3018	3020	3021	rBV2	864	365	0.01%	0.002%
67	10.786	3029	3031	3035	rBV5	1379	841	0.03%	0.005%
68	10.821	3040	3042	3045	rBV4	576	320	0.01%	0.002%
69	10.850	3049	3051	3053	rBV3	1019	437	0.02%	0.002%
70	10.870	3055	3057	3061	rBV4	714	383	0.02%	0.002%
71	10.892	3061	3064	3069	rBV6	1053	738	0.03%	0.004%
72	10.937	3076	3078	3081	rBV4	741	403	0.02%	0.002%
73	10.950	3081	3082	3087	rVB4	1490	857	0.03%	0.005%
74	10.976	3087	3090	3093	rBV3	1489	967	0.04%	0.005%
75	11.018	3099	3103	3105	rBV3	1092	737	0.03%	0.004%
76	11.063	3113	3117	3118	rBV3	753	426	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037157.D
 Acq On : 29 Aug 2024 15:06
 Operator : SY/MD
 Sample : VIBLK368
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK368

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.072	3118	3120	3124	rVB5	1257	849	0.03%	0.005%
78	11.114	3128	3133	3135	rBV6	1541	1324	0.05%	0.007%
79	11.127	3135	3137	3142	rVB5	1939	1255	0.05%	0.007%
80	11.182	3142	3154	3195	rBV	1055208	1698404	68.91%	9.443%
81	11.468	3241	3243	3249	rVB7	1578	1306	0.05%	0.007%
82	11.555	3259	3270	3303	rBV	1069308	1720729	69.81%	9.568%
83	11.915	3378	3382	3385	rBV6	1293	1259	0.05%	0.007%
84	12.262	3488	3490	3492	rBV2	1009	422	0.02%	0.002%
85	12.275	3492	3494	3497	rBV3	873	553	0.02%	0.003%
86	12.352	3517	3518	3521	rBV3	1050	415	0.02%	0.002%
87	12.397	3528	3532	3535	rBV5	1048	838	0.03%	0.005%
88	12.419	3537	3539	3541	rVV3	1243	564	0.02%	0.003%
89	12.435	3542	3544	3547	rVB4	1246	625	0.03%	0.003%
90	12.477	3555	3557	3560	rBV3	738	393	0.02%	0.002%
91	12.500	3560	3564	3570	rVV6	1417	1500	0.06%	0.008%
92	12.625	3601	3603	3605	rBV3	1186	646	0.03%	0.004%
93	12.747	3637	3641	3645	rBV6	1819	1888	0.08%	0.010%
94	12.886	3681	3684	3686	rBV3	1169	614	0.02%	0.003%
95	12.960	3705	3707	3710	rBV4	860	405	0.02%	0.002%
96	13.030	3727	3729	3730	rBV2	1281	535	0.02%	0.003%
97	13.085	3744	3746	3747	rBV2	1420	626	0.03%	0.003%
98	13.230	3789	3791	3792	rBV3	1185	400	0.02%	0.002%
99	14.079	4053	4055	4060	rBV5	1239	939	0.04%	0.005%
100	14.686	4242	4244	4248	rVB5	1936	834	0.03%	0.005%




Sum of corrected areas: 17985050

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037157.D
Acq On : 29 Aug 2024 15:06
Operator : SY/MD
Sample : VIBLK368
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK368

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

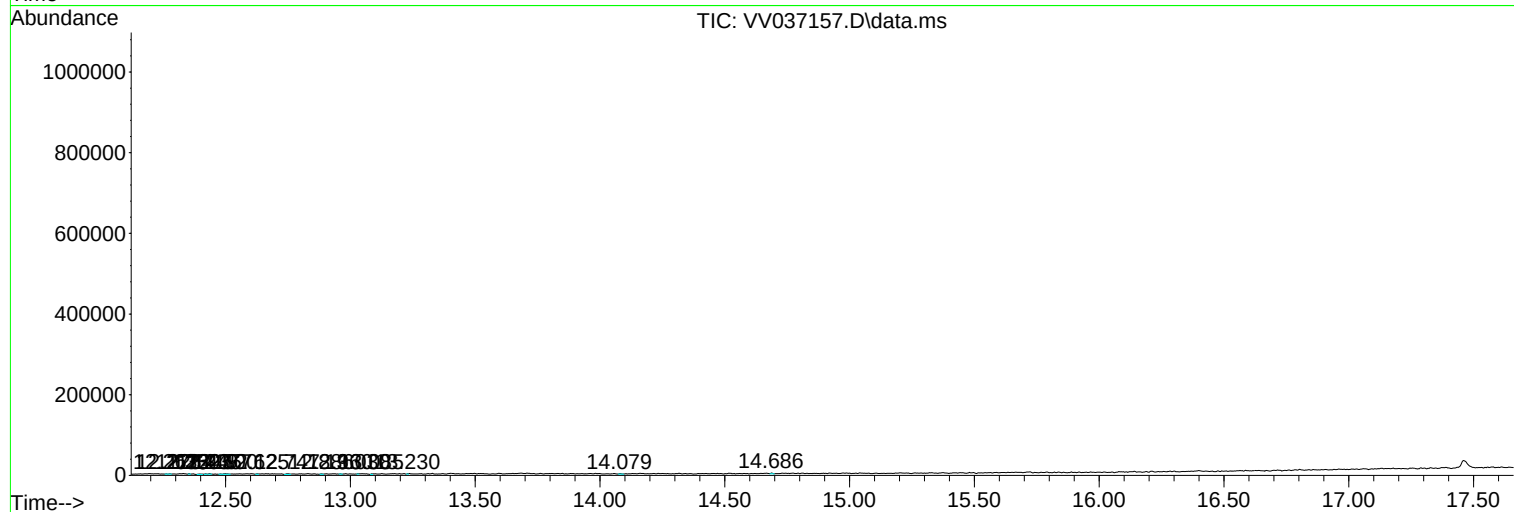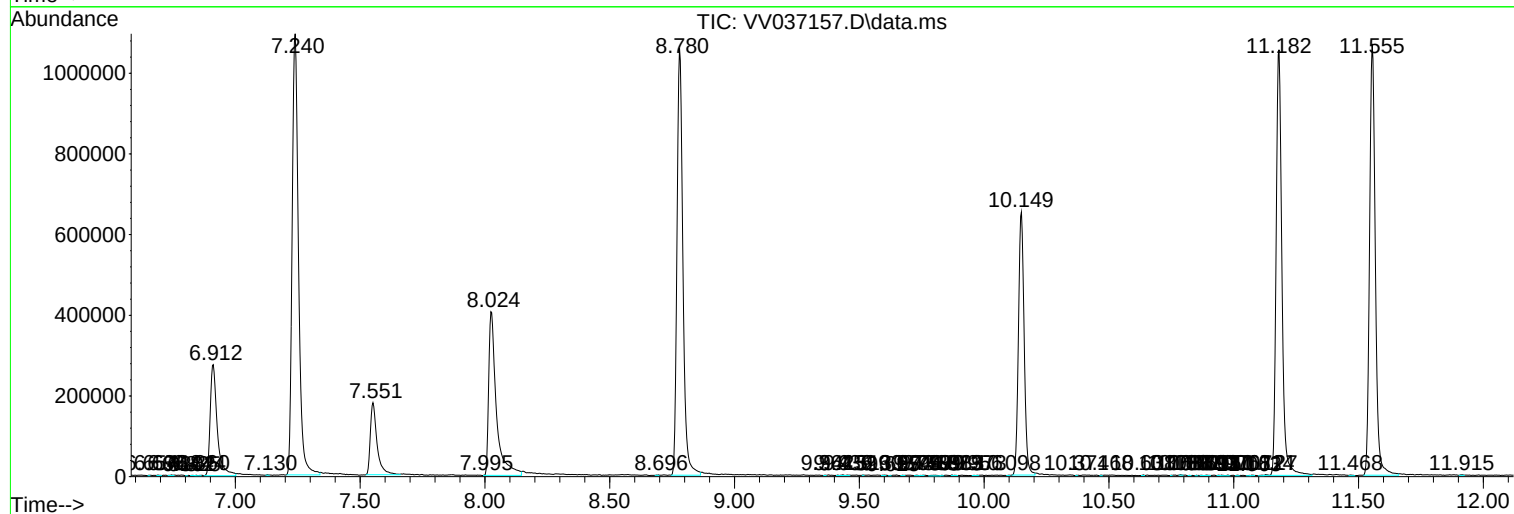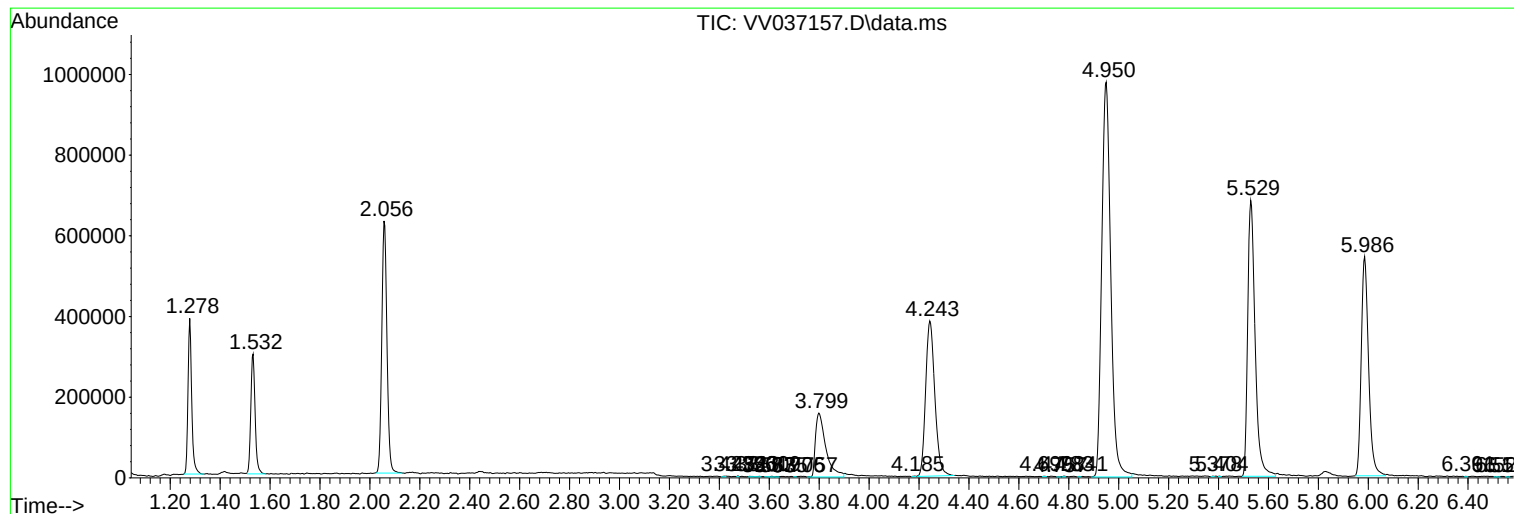

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037157.D
Acq On : 29 Aug 2024 15:06
Operator : SY/MD
Sample : VIBLK368
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK368

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037157.D
Acq On : 29 Aug 2024 15:06
Operator : SY/MD
Sample : VIBLK368
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK368

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc