

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037158.D
 Acq On : 29 Aug 2024 15:28
 Operator : SY/MD
 Sample : P3692-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	36	41	51	rBV	9256	18473	0.17%	0.059%
2	1.282	67	75	101	rVB2	1619600	1768048	15.96%	5.635%
3	1.532	146	153	170	rVB	309391	366233	3.31%	1.167%
4	2.060	307	317	331	rBV2	712539	1095655	9.89%	3.492%
5	3.307	703	705	709	rVB5	1696	947	0.01%	0.003%
6	3.394	730	732	735	rVB4	1059	553	0.00%	0.002%
7	3.478	756	758	763	rVB4	1209	955	0.01%	0.003%
8	3.500	763	765	767	rBV2	1299	754	0.01%	0.002%
9	3.577	787	789	790	rBV2	830	308	0.00%	0.001%
10	3.625	802	804	807	rVB3	1186	591	0.01%	0.002%
11	3.642	807	809	812	rBV2	554	286	0.00%	0.001%
12	3.680	818	821	824	rBV6	1178	803	0.01%	0.003%
13	3.722	831	834	835	rBV2	1099	594	0.01%	0.002%
14	3.806	843	860	909	rBV	4702687	11075766	100.00%	35.299%
15	4.243	980	996	1024	rBV	387881	984467	8.89%	3.138%
16	4.732	1144	1148	1151	rBV4	1274	988	0.01%	0.003%
17	4.863	1185	1189	1192	rBV5	1613	1188	0.01%	0.004%
18	4.886	1192	1196	1198	rBV3	764	541	0.00%	0.002%
19	4.950	1200	1216	1254	rBV2	987363	2486292	22.45%	7.924%
20	5.529	1384	1396	1430	rBV	680172	1411984	12.75%	4.500%
21	5.828	1478	1489	1516	rBV	522022	1054883	9.52%	3.362%
22	5.986	1527	1538	1564	rBV	544067	1096089	9.90%	3.493%
23	6.526	1702	1706	1708	rBV4	1289	992	0.01%	0.003%
24	6.539	1708	1710	1712	rVB3	1134	443	0.00%	0.001%
25	6.625	1735	1737	1738	rBV2	961	499	0.00%	0.002%
26	6.693	1754	1758	1759	rBV4	1341	841	0.01%	0.003%
27	6.719	1764	1766	1767	rBV2	797	286	0.00%	0.001%
28	6.776	1781	1784	1785	rBV3	1194	513	0.00%	0.002%
29	6.802	1790	1792	1794	rVB2	1026	410	0.00%	0.001%
30	6.815	1794	1796	1800	rVB5	1222	670	0.01%	0.002%
31	6.834	1800	1802	1804	rBV2	692	364	0.00%	0.001%
32	6.860	1808	1810	1814	rVB5	981	604	0.01%	0.002%
33	6.908	1814	1825	1852	rBV	279970	542263	4.90%	1.728%
34	7.169	1904	1906	1910	rBV4	977	630	0.01%	0.002%
35	7.239	1916	1928	1957	rBV	1114619	1967725	17.77%	6.271%
36	7.551	2016	2025	2053	rBV	186012	344546	3.11%	1.098%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037158.D
 Acq On : 29 Aug 2024 15:28
 Operator : SY/MD
 Sample : P3692-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.024	2164	2172	2217	rBV	422713	882324	7.97%	2.812%
38	8.648	2361	2366	2369	rVB4	1800	1602	0.01%	0.005%
39	8.667	2369	2372	2376	rBV6	1586	1432	0.01%	0.005%
40	8.780	2396	2407	2441	rBV	1058608	1741168	15.72%	5.549%
41	9.259	2554	2556	2562	rVB7	1321	1078	0.01%	0.003%
42	9.288	2562	2565	2568	rBV5	1398	1232	0.01%	0.004%
43	9.342	2579	2582	2584	rBV4	1193	740	0.01%	0.002%
44	9.387	2594	2596	2597	rBV2	1033	432	0.00%	0.001%
45	9.481	2622	2625	2626	rBV3	803	328	0.00%	0.001%
46	9.519	2634	2637	2638	rBV2	720	427	0.00%	0.001%
47	9.548	2642	2646	2653	rBV10	2229	2731	0.02%	0.009%
48	9.580	2653	2656	2657	rBV2	1039	499	0.00%	0.002%
49	9.628	2666	2671	2676	rVB8	1648	1647	0.01%	0.005%
50	9.680	2685	2687	2689	rVB3	507	266	0.00%	0.001%
51	9.706	2689	2695	2696	rBV2	1916	1302	0.01%	0.004%
52	9.812	2725	2728	2729	rBV3	978	467	0.00%	0.001%
53	9.870	2744	2746	2749	rBV4	1135	665	0.01%	0.002%
54	9.969	2775	2777	2780	rVB4	949	470	0.00%	0.001%
55	9.985	2780	2782	2784	rBV2	779	375	0.00%	0.001%
56	10.005	2787	2788	2790	rBV2	545	177	0.00%	0.001%
57	10.018	2790	2792	2795	rBV4	1774	1076	0.01%	0.003%
58	10.040	2797	2799	2801	rBV3	625	298	0.00%	0.001%
59	10.085	2810	2813	2814	rBV2	715	377	0.00%	0.001%
60	10.146	2821	2832	2852	rBV	673418	1064208	9.61%	3.392%
61	10.452	2925	2927	2929	rVB3	1561	510	0.00%	0.002%
62	10.477	2933	2935	2937	rBV3	835	505	0.00%	0.002%
63	10.564	2958	2962	2963	rBV2	1397	907	0.01%	0.003%
64	10.619	2977	2979	2980	rBV	567	245	0.00%	0.001%
65	10.638	2980	2985	2987	rVV5	1061	1053	0.01%	0.003%
66	10.699	3002	3004	3007	rVB4	1094	486	0.00%	0.002%
67	10.712	3007	3008	3011	rBV3	925	521	0.00%	0.002%
68	10.751	3018	3020	3023	rBV2	486	263	0.00%	0.001%
69	10.773	3025	3027	3028	rVB2	625	142	0.00%	0.000%
70	10.786	3028	3031	3033	rBV4	1863	1222	0.01%	0.004%
71	10.841	3045	3048	3050	rBV3	728	396	0.00%	0.001%
72	10.905	3064	3068	3072	rVB6	1553	1300	0.01%	0.004%
73	10.921	3072	3073	3077	rVB4	1009	480	0.00%	0.002%
74	10.950	3077	3082	3083	rBV4	1382	977	0.01%	0.003%
75	11.021	3102	3104	3108	rVB4	1211	838	0.01%	0.003%
76	11.053	3108	3114	3119	rBV7	1330	1637	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037158.D
 Acq On : 29 Aug 2024 15:28
 Operator : SY/MD
 Sample : P3692-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.079	3119	3122	3123	rVB2	545	288	0.00%	0.001%
78	11.098	3123	3128	3129	rBV4	1476	1018	0.01%	0.003%
79	11.178	3142	3153	3183	rBV	1035791	1681390	15.18%	5.359%
80	11.554	3256	3270	3296	rBV	1085048	1736055	15.67%	5.533%
81	11.879	3369	3371	3373	rBV2	1064	464	0.00%	0.001%
82	11.998	3406	3408	3410	rBV3	875	403	0.00%	0.001%
83	12.117	3442	3445	3447	rBV4	1641	979	0.01%	0.003%
84	12.175	3459	3463	3464	rBV4	1122	885	0.01%	0.003%
85	12.304	3501	3503	3506	rVB2	1382	735	0.01%	0.002%
86	12.419	3534	3539	3542	rBV6	1629	1605	0.01%	0.005%
87	12.503	3563	3565	3568	rVB3	1533	726	0.01%	0.002%
88	12.522	3568	3571	3573	rBV3	765	413	0.00%	0.001%
89	12.558	3576	3582	3585	rBV6	1871	2067	0.02%	0.007%
90	12.715	3624	3631	3634	rBV5	1990	1887	0.02%	0.006%
91	12.841	3668	3670	3672	rVB2	688	213	0.00%	0.001%
92	12.853	3672	3674	3675	rBV2	975	384	0.00%	0.001%
93	12.911	3690	3692	3693	rBV2	1126	496	0.00%	0.002%
94	13.124	3756	3758	3760	rBV2	1097	534	0.00%	0.002%
95	13.165	3769	3771	3772	rBV	1048	502	0.00%	0.002%
96	13.204	3780	3783	3785	rBV4	1384	848	0.01%	0.003%
97	13.632	3913	3916	3918	rBV3	1546	897	0.01%	0.003%
98	13.677	3927	3930	3931	rBV3	1123	622	0.01%	0.002%




Sum of corrected areas: 31377398

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037158.D
Acq On : 29 Aug 2024 15:28
Operator : SY/MD
Sample : P3692-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

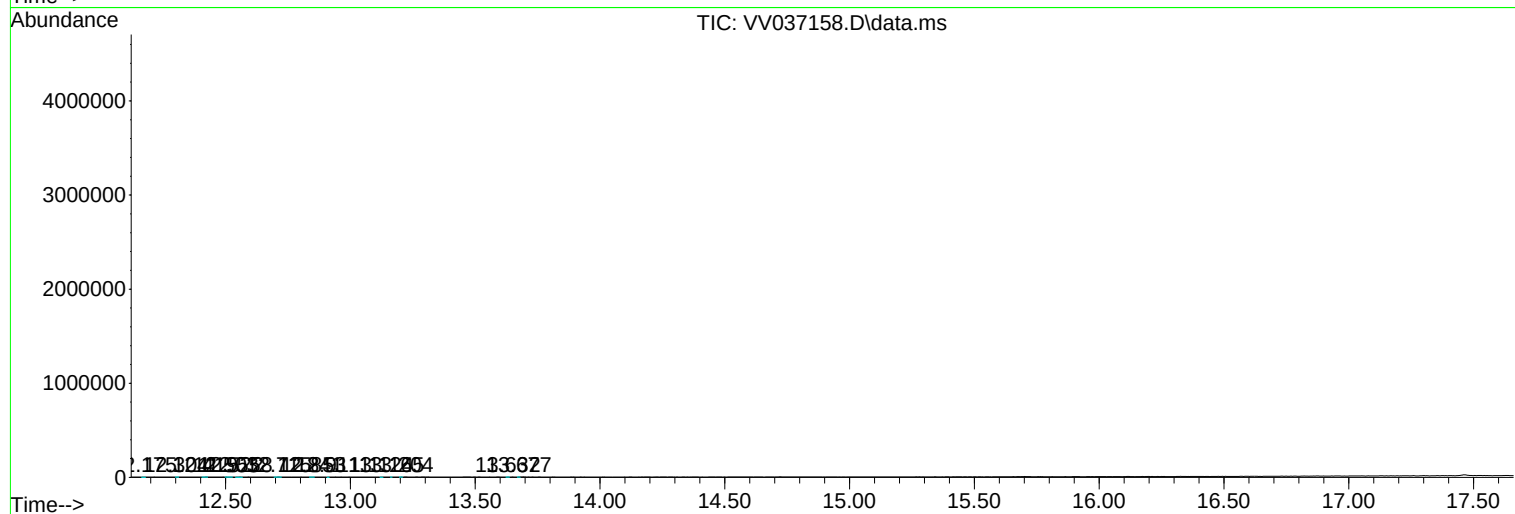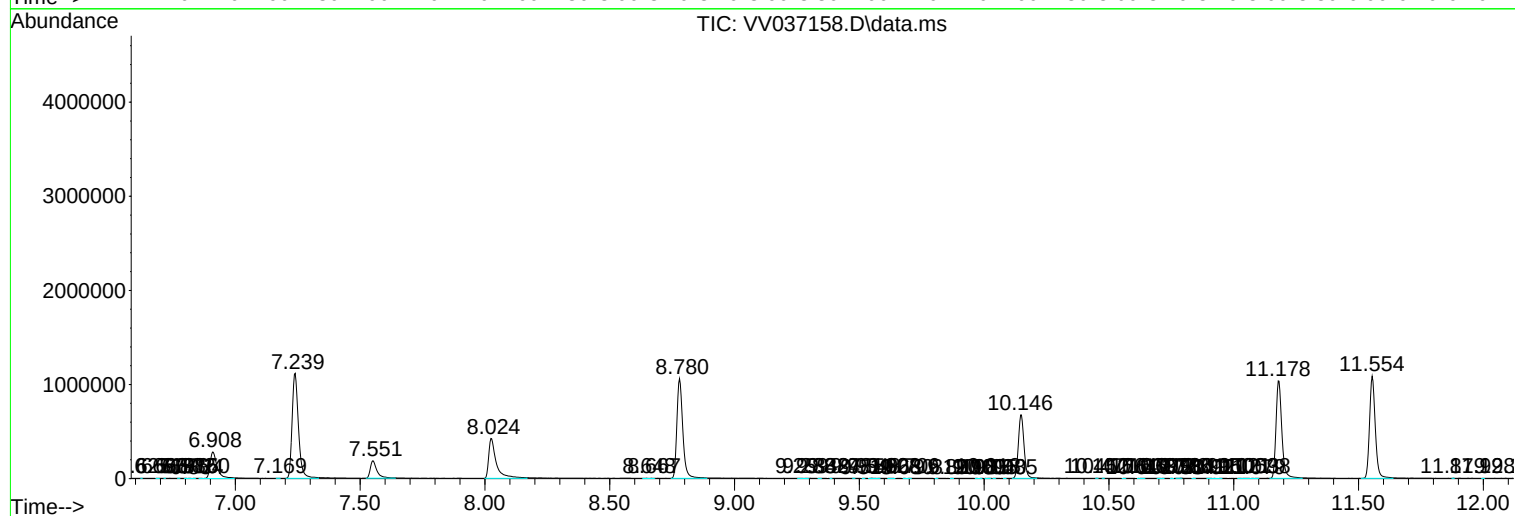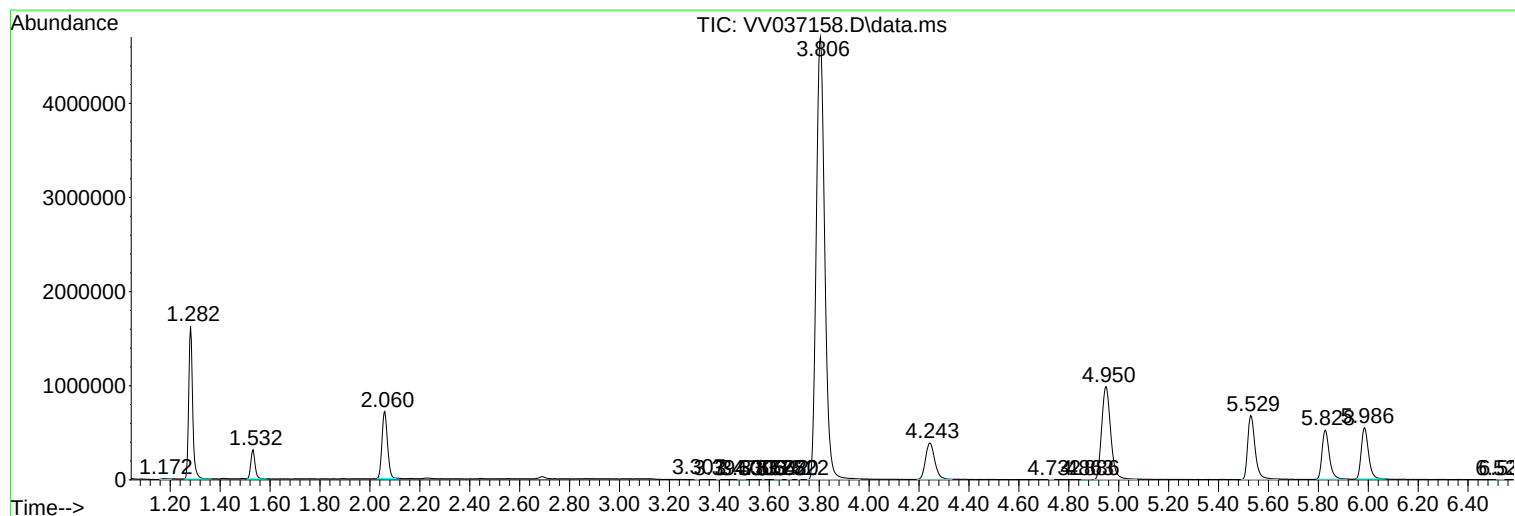

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037158.D
Acq On : 29 Aug 2024 15:28
Operator : SY/MD
Sample : P3692-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037158.D
Acq On : 29 Aug 2024 15:28
Operator : SY/MD
Sample : P3692-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------