

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037172.D
 Acq On : 29 Aug 2024 21:26
 Operator : SY/MD
 Sample : P3785-04 100X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	343694	363885	2.37%	0.748%
2	1.529	145	152	166	rVB	288306	338779	2.21%	0.697%
3	2.056	307	316	332	rBV	583874	832037	5.43%	1.711%
4	3.371	723	725	727	rBV2	986	572	0.00%	0.001%
5	3.420	738	740	742	rBV3	1033	599	0.00%	0.001%
6	3.510	767	768	773	rBV5	891	481	0.00%	0.001%
7	3.535	773	776	779	rBV4	686	399	0.00%	0.001%
8	3.548	779	780	781	rBV	581	190	0.00%	0.000%
9	3.738	835	839	841	rBV3	1349	1182	0.01%	0.002%
10	3.796	848	857	884	rBV	124097	343461	2.24%	0.706%
11	4.124	955	959	961	rBV4	952	802	0.01%	0.002%
12	4.140	962	964	965	rBV2	988	364	0.00%	0.001%
13	4.243	981	996	1024	rBV	378300	977295	6.38%	2.009%
14	4.686	1131	1134	1136	rBV4	1124	817	0.01%	0.002%
15	4.796	1164	1168	1171	rBV6	936	597	0.00%	0.001%
16	4.815	1171	1174	1178	rBV4	972	835	0.01%	0.002%
17	4.860	1186	1188	1190	rBV3	628	423	0.00%	0.001%
18	4.950	1200	1216	1225	rBV2	976285	2395061	15.63%	4.924%
19	5.471	1376	1378	1379	rBV2	1110	360	0.00%	0.001%
20	5.529	1385	1396	1430	rBV	696416	1431834	9.34%	2.944%
21	5.834	1480	1491	1505	rBV	9701	25786	0.17%	0.053%
22	5.985	1526	1538	1563	rBV	532135	1101504	7.19%	2.265%
23	6.358	1652	1654	1656	rBV3	1256	846	0.01%	0.002%
24	6.416	1670	1672	1674	rBV3	858	268	0.00%	0.001%
25	6.516	1700	1703	1705	rBV4	1060	740	0.00%	0.002%
26	6.542	1709	1711	1714	rBV3	1275	722	0.00%	0.001%
27	6.574	1719	1721	1725	rBV4	1143	582	0.00%	0.001%
28	6.600	1725	1729	1731	rBV4	994	651	0.00%	0.001%
29	6.651	1741	1745	1746	rVB3	641	445	0.00%	0.001%
30	6.657	1746	1747	1749	rVB2	883	263	0.00%	0.001%
31	6.673	1749	1752	1755	rBV3	991	920	0.01%	0.002%
32	6.696	1755	1759	1763	rVV7	1368	1051	0.01%	0.002%
33	6.731	1768	1770	1772	rBV2	793	358	0.00%	0.001%
34	6.747	1772	1775	1779	rVV6	1190	973	0.01%	0.002%
35	6.767	1779	1781	1785	rVB5	1726	1096	0.01%	0.002%
36	6.792	1785	1789	1791	rBV6	1291	1034	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037172.D
 Acq On : 29 Aug 2024 21:26
 Operator : SY/MD
 Sample : P3785-04 100X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.850	1804	1807	1809	rBV4	1228	601	0.00%	0.001%
38	6.911	1814	1826	1859	rBV	260609	515051	3.36%	1.059%
39	7.239	1916	1928	1956	rBV	1085774	1911106	12.47%	3.929%
40	7.551	2016	2025	2053	rBV	168356	320766	2.09%	0.660%
41	7.751	2085	2087	2093	rVB7	1454	898	0.01%	0.002%
42	7.982	2157	2159	2162	rBV5	1365	931	0.01%	0.002%
43	8.024	2164	2172	2208	rBV	389745	791810	5.17%	1.628%
44	8.484	2313	2315	2318	rBV3	1593	958	0.01%	0.002%
45	8.616	2354	2356	2358	rVB3	1039	353	0.00%	0.001%
46	8.635	2360	2362	2363	rBV2	541	167	0.00%	0.000%
47	8.673	2371	2374	2376	rBV3	1235	818	0.01%	0.002%
48	8.709	2383	2385	2387	rBV3	875	484	0.00%	0.001%
49	8.808	2396	2416	2460	rBV2	8475358	15326463	100.00%	31.512%
50	9.477	2622	2624	2625	rBV2	1089	439	0.00%	0.001%
51	9.519	2635	2637	2641	rBV5	882	571	0.00%	0.001%
52	9.574	2652	2654	2659	rBV6	840	668	0.00%	0.001%
53	9.689	2688	2690	2691	rBV2	977	466	0.00%	0.001%
54	9.718	2697	2699	2701	rBV2	936	489	0.00%	0.001%
55	9.821	2727	2731	2733	rVB5	953	602	0.00%	0.001%
56	9.844	2733	2738	2741	rBV5	1532	1205	0.01%	0.002%
57	9.876	2745	2748	2754	rVB5	1648	1294	0.01%	0.003%
58	9.911	2754	2759	2765	rBV7	1222	1187	0.01%	0.002%
59	9.937	2765	2767	2769	rBV3	789	471	0.00%	0.001%
60	9.988	2780	2783	2785	rBV4	1318	764	0.00%	0.002%
61	10.011	2787	2790	2794	rVB4	1965	1657	0.01%	0.003%
62	10.033	2794	2797	2798	rBV2	1311	607	0.00%	0.001%
63	10.085	2810	2813	2815	rBV3	729	406	0.00%	0.001%
64	10.149	2821	2833	2863	rBV	628114	1016931	6.64%	2.091%
65	10.323	2885	2887	2889	rBV3	749	381	0.00%	0.001%
66	10.358	2895	2898	2900	rBV4	1791	1213	0.01%	0.002%
67	10.423	2917	2918	2921	rBV2	837	423	0.00%	0.001%
68	10.522	2945	2949	2950	rBV2	1197	695	0.00%	0.001%
69	10.593	2968	2971	2974	rVB4	1245	727	0.00%	0.001%
70	10.609	2974	2976	2977	rBV2	1060	528	0.00%	0.001%
71	10.654	2988	2990	2995	rBV4	841	528	0.00%	0.001%
72	10.673	2995	2996	2999	rVB2	447	205	0.00%	0.000%
73	10.686	2999	3000	3005	rVB5	839	383	0.00%	0.001%
74	10.705	3005	3006	3008	rVB2	656	130	0.00%	0.000%
75	10.725	3008	3012	3013	rBV3	450	292	0.00%	0.001%
76	10.844	3041	3049	3050	rBV5	1205	1226	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037172.D
 Acq On : 29 Aug 2024 21:26
 Operator : SY/MD
 Sample : P3785-04 100X
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	10.889	3061	3063	3066	rBV3	1070	582	0.00%	0.001%
78	10.908	3067	3069	3073	rVB4	1555	742	0.00%	0.002%
79	10.940	3075	3079	3083	rVB5	934	805	0.01%	0.002%
80	10.959	3083	3085	3086	rBV2	659	308	0.00%	0.001%
81	11.017	3100	3103	3105	rBV5	918	598	0.00%	0.001%
82	11.053	3112	3114	3116	rVB2	861	231	0.00%	0.000%
83	11.066	3116	3118	3120	rBV3	835	315	0.00%	0.001%
84	11.114	3122	3133	3144	rBV	496555	784425	5.12%	1.613%
85	11.201	3145	3160	3193	rVB2	4455386	8377243	54.66%	17.224%
86	11.570	3259	3275	3303	rBV2	5567770	9986281	65.16%	20.532%
87	12.136	3449	3451	3453	rBV2	1044	429	0.00%	0.001%
88	12.197	3467	3470	3473	rBV6	1452	869	0.01%	0.002%
89	12.448	3545	3548	3551	rBV5	1652	1230	0.01%	0.003%
90	12.625	3599	3603	3607	rBV6	1591	1726	0.01%	0.004%
91	12.840	3668	3670	3672	rBV2	927	585	0.00%	0.001%
92	12.885	3682	3684	3685	rBV	1106	410	0.00%	0.001%
93	12.927	3694	3697	3703	rBV7	1225	1153	0.01%	0.002%
94	12.985	3712	3715	3718	rBV5	1147	980	0.01%	0.002%
95	13.069	3739	3741	3744	rVB4	798	376	0.00%	0.001%
96	13.152	3765	3767	3768	rBV2	651	283	0.00%	0.001%
97	13.191	3768	3779	3800	rBV	894393	1435232	9.36%	2.951%
98	13.676	3918	3930	3948	rBV	188710	310393	2.03%	0.638%




Sum of corrected areas: 48637302

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037172.D
Acq On : 29 Aug 2024 21:26
Operator : SY/MD
Sample : P3785-04 100X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

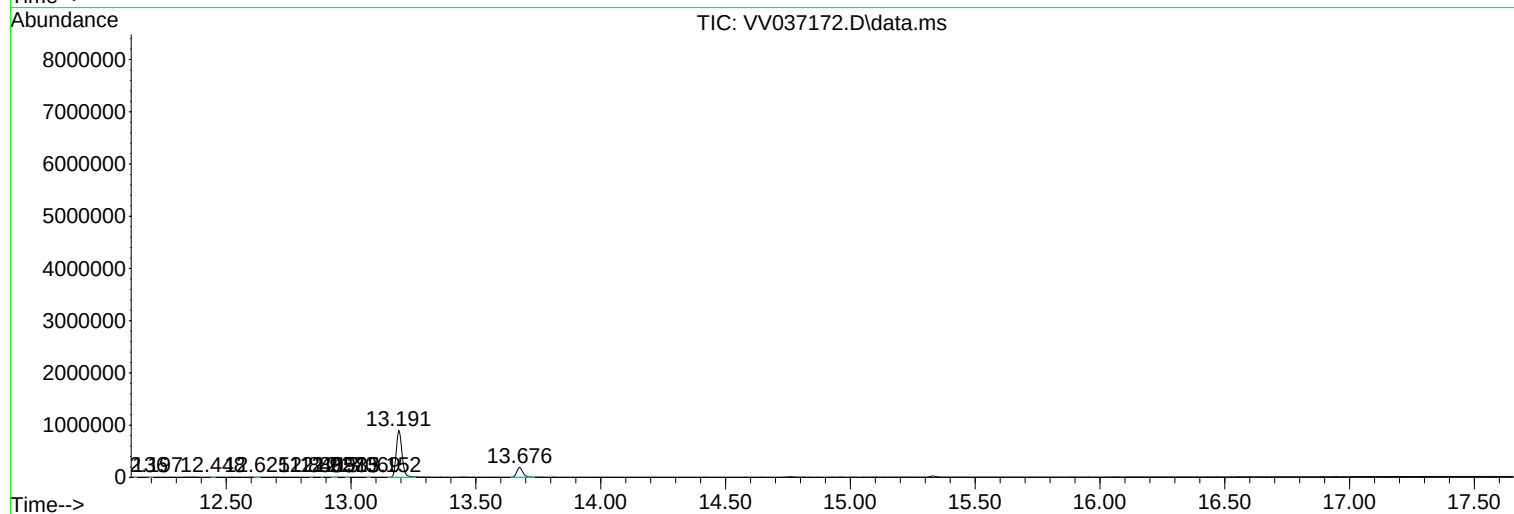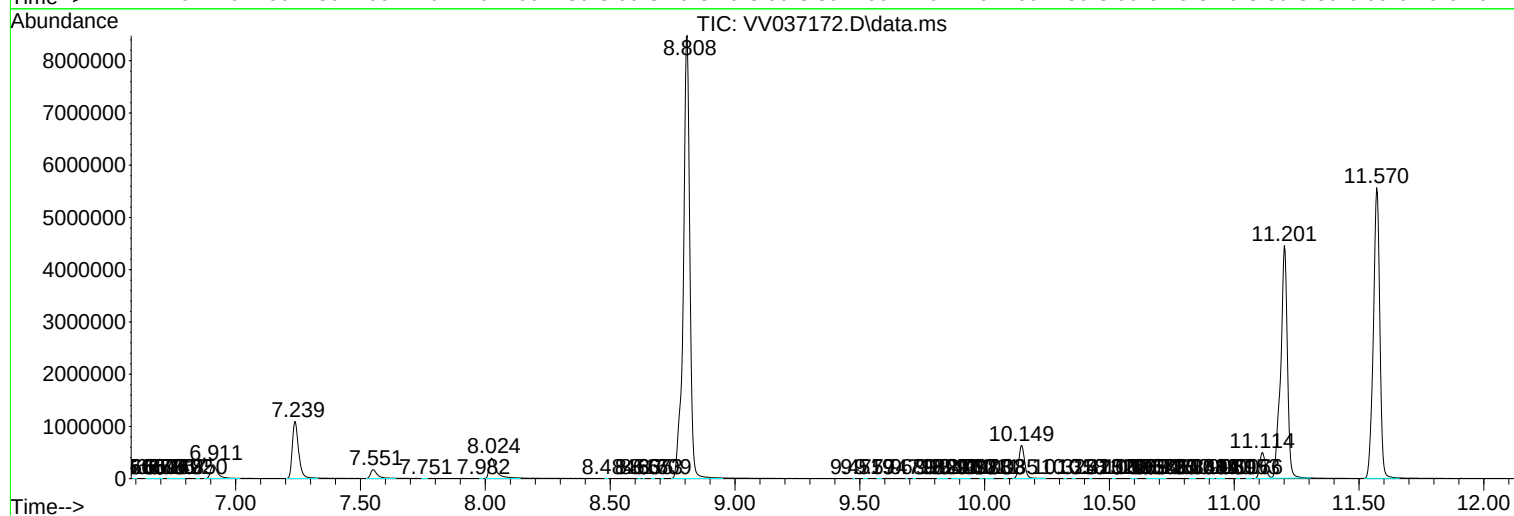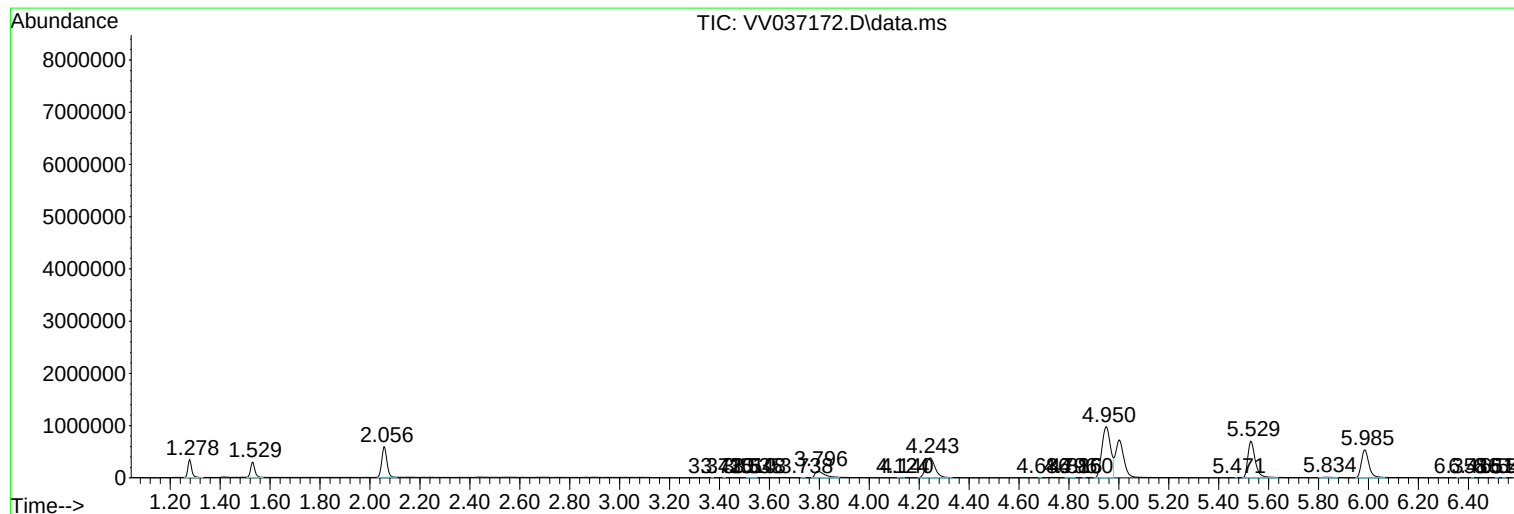

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037172.D
Acq On : 29 Aug 2024 21:26
Operator : SY/MD
Sample : P3785-04 100X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037172.D
Acq On : 29 Aug 2024 21:26
Operator : SY/MD
Sample : P3785-04 100X
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc