

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037174.D
 Acq On : 29 Aug 2024 22:09
 Operator : SY/MD
 Sample : P3785-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	334942	344869	4.88%	1.343%
2	1.532	146	153	167	rVB	277688	326983	4.63%	1.273%
3	2.060	307	317	328	rBV	573020	831471	11.76%	3.237%
4	3.503	762	766	768	rBV5	948	529	0.01%	0.002%
5	3.641	807	809	810	rBV2	1068	493	0.01%	0.002%
6	3.670	816	818	819	rBV2	535	163	0.00%	0.001%
7	3.703	823	828	829	rBV4	1026	772	0.01%	0.003%
8	3.738	838	839	841	rVB2	959	287	0.00%	0.001%
9	3.796	848	857	890	rBV3	118669	392855	5.56%	1.529%
10	4.137	961	963	970	rVB7	1399	1078	0.02%	0.004%
11	4.243	983	996	1023	rVB	373593	928674	13.14%	3.615%
12	4.612	1110	1111	1114	rBV3	988	452	0.01%	0.002%
13	4.658	1123	1125	1127	rBV2	1116	546	0.01%	0.002%
14	4.703	1134	1139	1143	rBV6	1373	1444	0.02%	0.006%
15	4.738	1148	1150	1152	rBV	903	400	0.01%	0.002%
16	4.805	1168	1171	1173	rBV4	1328	952	0.01%	0.004%
17	4.834	1177	1180	1183	rVB4	1250	813	0.01%	0.003%
18	4.950	1200	1216	1248	rBV2	931885	2405173	34.02%	9.363%
19	5.529	1384	1396	1428	rBV	667785	1382254	19.55%	5.381%
20	5.985	1526	1538	1565	rBV	522092	1066990	15.09%	4.154%
21	6.349	1649	1651	1656	rVB6	1243	843	0.01%	0.003%
22	6.468	1685	1688	1690	rVB3	1189	634	0.01%	0.002%
23	6.529	1706	1707	1712	rVB4	1420	781	0.01%	0.003%
24	6.555	1712	1715	1718	rBV4	1453	1224	0.02%	0.005%
25	6.625	1735	1737	1740	rBV4	1391	824	0.01%	0.003%
26	6.667	1746	1750	1754	rBV7	1387	1240	0.02%	0.005%
27	6.693	1756	1758	1761	rVB3	1204	790	0.01%	0.003%
28	6.719	1761	1766	1767	rBV4	1356	844	0.01%	0.003%
29	6.792	1786	1789	1794	rVB7	1380	1171	0.02%	0.005%
30	6.837	1802	1803	1807	rBV3	770	395	0.01%	0.002%
31	6.860	1807	1810	1811	rBV2	847	532	0.01%	0.002%
32	6.911	1816	1826	1850	rBV2	255287	492279	6.96%	1.916%
33	7.239	1917	1928	1955	rBV	1046037	1855907	26.25%	7.225%
34	7.551	2016	2025	2052	rBV	163693	310201	4.39%	1.208%
35	7.889	2127	2130	2133	rBV4	1665	1081	0.02%	0.004%
36	7.927	2139	2142	2143	rBV3	1413	828	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037174.D
 Acq On : 29 Aug 2024 22:09
 Operator : SY/MD
 Sample : P3785-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.024	2164	2172	2207	rBV2	353849	749120	10.60%	2.916%
38	8.683	2372	2377	2378	rBV4	1020	844	0.01%	0.003%
39	8.780	2396	2407	2414	rBV	1070359	1822740	25.78%	7.096%
40	9.329	2573	2578	2581	rBV6	1257	1446	0.02%	0.006%
41	9.358	2585	2587	2591	rVB4	1153	730	0.01%	0.003%
42	9.384	2591	2595	2598	rBV6	1672	1508	0.02%	0.006%
43	9.403	2598	2601	2603	rBV4	1022	581	0.01%	0.002%
44	9.439	2610	2612	2614	rBV3	922	424	0.01%	0.002%
45	9.548	2645	2646	2647	rBV3	558	117	0.00%	0.000%
46	9.580	2654	2656	2658	rBV2	590	243	0.00%	0.001%
47	9.612	2662	2666	2667	rBV4	938	778	0.01%	0.003%
48	9.706	2692	2695	2699	rBV6	1413	1307	0.02%	0.005%
49	9.728	2699	2702	2705	rVV4	1380	902	0.01%	0.004%
50	9.741	2705	2706	2709	rVV3	610	358	0.01%	0.001%
51	9.776	2715	2717	2720	rBV3	855	458	0.01%	0.002%
52	9.815	2727	2729	2731	rBV3	822	329	0.00%	0.001%
53	9.995	2779	2785	2787	rBV6	1463	1296	0.02%	0.005%
54	10.008	2787	2789	2790	rVV	1225	547	0.01%	0.002%
55	10.034	2794	2797	2802	rBV7	900	729	0.01%	0.003%
56	10.146	2821	2832	2854	rBV	606775	973067	13.76%	3.788%
57	10.471	2932	2933	2936	rVB2	1228	407	0.01%	0.002%
58	10.484	2936	2937	2938	rBV	457	100	0.00%	0.000%
59	10.509	2943	2945	2946	rBV	821	392	0.01%	0.002%
60	10.551	2956	2958	2962	rVB6	1090	749	0.01%	0.003%
61	10.577	2962	2966	2967	rBV4	844	523	0.01%	0.002%
62	10.587	2967	2969	2972	rBV4	644	293	0.00%	0.001%
63	10.609	2972	2976	2980	rBV6	777	735	0.01%	0.003%
64	10.702	3002	3005	3008	rBV5	1512	1110	0.02%	0.004%
65	10.799	3033	3035	3040	rVB5	1508	993	0.01%	0.004%
66	10.834	3045	3046	3048	rBV	345	187	0.00%	0.001%
67	10.869	3053	3057	3061	rBV4	1786	1594	0.02%	0.006%
68	10.911	3068	3070	3072	rBV4	813	324	0.00%	0.001%
69	10.976	3086	3090	3093	rBV5	1274	953	0.01%	0.004%
70	10.992	3093	3095	3096	rBV2	448	196	0.00%	0.001%
71	11.011	3097	3101	3105	rVB4	1201	1215	0.02%	0.005%
72	11.027	3105	3106	3107	rBV	977	352	0.00%	0.001%
73	11.114	3124	3133	3143	rBV	126830	204683	2.90%	0.797%
74	11.178	3144	3153	3194	rVB2	1081858	2141350	30.29%	8.336%
75	11.570	3259	3275	3303	rBV2	3728099	7069330	100.00%	27.520%
76	11.959	3394	3396	3397	rBV3	957	264	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037174.D
Acq On : 29 Aug 2024 22:09
Operator : SY/MD
Sample : P3785-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	12.223	3475	3478	3481	rBV5	1451	1278	0.02%	0.005%
78	12.429	3539	3542	3545	rBV4	1657	1177	0.02%	0.005%
79	12.580	3580	3589	3608	rBV2	20489	49715	0.70%	0.194%
80	12.914	3690	3693	3697	rBV6	1347	1261	0.02%	0.005%
81	12.988	3714	3716	3717	rBV2	1042	404	0.01%	0.002%
82	13.191	3768	3779	3804	rBV	873514	1370091	19.38%	5.334%
83	13.554	3888	3892	3894	rBV4	1031	924	0.01%	0.004%
84	13.673	3918	3929	3943	rBV	429142	691930	9.79%	2.694%
85	14.098	4053	4061	4075	rVB8	11700	21518	0.30%	0.084%
86	15.326	4434	4443	4459	rBV	126451	209955	2.97%	0.817%




Sum of corrected areas: 25688299

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037174.D
Acq On : 29 Aug 2024 22:09
Operator : SY/MD
Sample : P3785-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

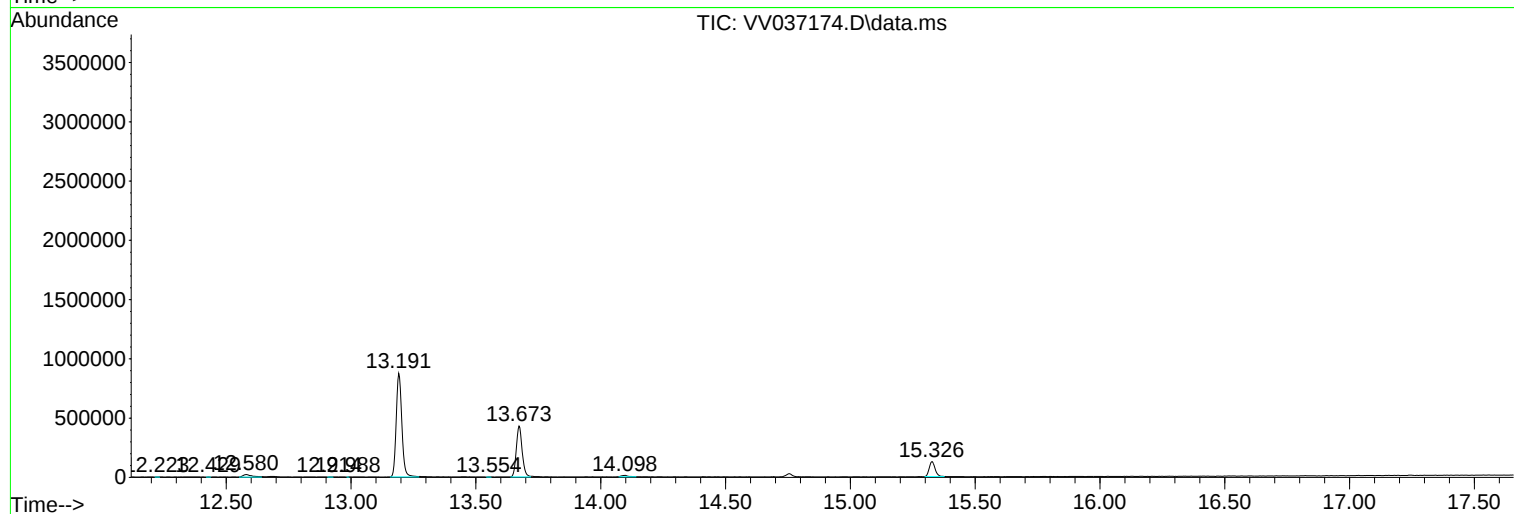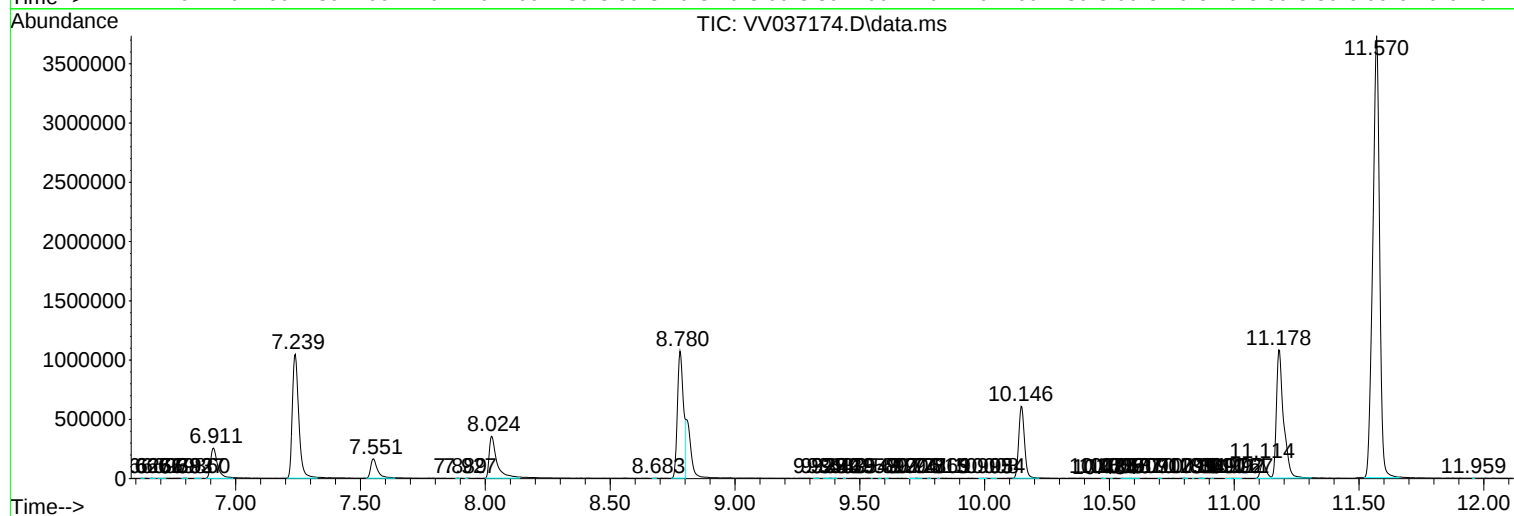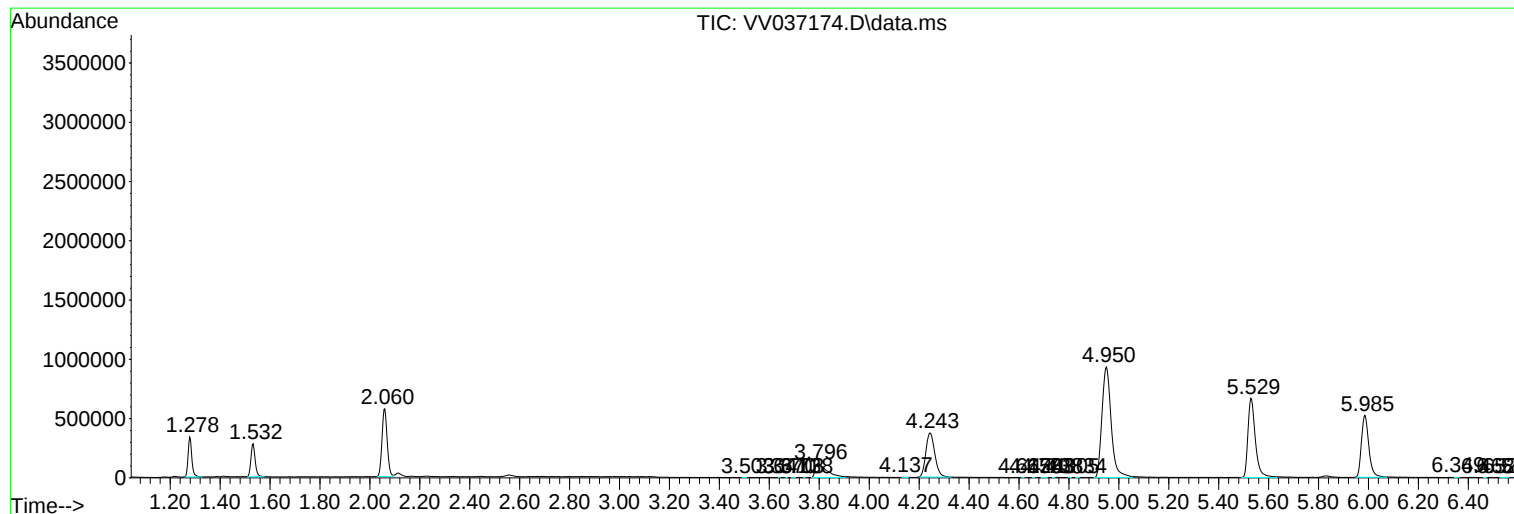

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037174.D
Acq On : 29 Aug 2024 22:09
Operator : SY/MD
Sample : P3785-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037174.D
Acq On : 29 Aug 2024 22:09
Operator : SY/MD
Sample : P3785-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc