

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037178.D
 Acq On : 29 Aug 2024 23:36
 Operator : SY/MD
 Sample : P3692-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	337268	352360	15.26%	2.125%
2	1.532	146	153	170	rVB	283199	332511	14.40%	2.005%
3	2.059	308	317	331	rVB	557288	804370	34.83%	4.850%
4	3.323	708	710	715	rBV5	1372	1030	0.04%	0.006%
5	3.516	768	770	775	rBV6	743	611	0.03%	0.004%
6	3.625	801	804	807	rBV4	1731	1006	0.04%	0.006%
7	3.661	812	815	817	rVV4	1262	632	0.03%	0.004%
8	3.670	817	818	821	rVB2	986	285	0.01%	0.002%
9	3.764	846	847	848	rBV	724	269	0.01%	0.002%
10	3.796	849	857	883	rVV	107292	293855	12.72%	1.772%
11	4.243	981	996	1030	rBV	361876	932100	40.36%	5.621%
12	4.558	1092	1094	1097	rVB3	933	399	0.02%	0.002%
13	4.574	1097	1099	1103	rVB4	1129	578	0.03%	0.003%
14	4.596	1103	1106	1109	rVB3	826	549	0.02%	0.003%
15	4.619	1109	1113	1115	rBV4	1239	816	0.04%	0.005%
16	4.860	1186	1188	1191	rVB3	781	225	0.01%	0.001%
17	4.950	1199	1216	1242	rBV2	919034	2309275	100.00%	13.925%
18	5.448	1368	1371	1372	rBV3	1197	581	0.03%	0.004%
19	5.529	1385	1396	1423	rBV	645750	1326028	57.42%	7.996%
20	5.934	1520	1522	1524	rBV3	1175	433	0.02%	0.003%
21	5.985	1525	1538	1568	rBV	516139	1068397	46.27%	6.442%
22	6.374	1654	1659	1660	rBV4	1048	819	0.04%	0.005%
23	6.400	1665	1667	1670	rBV3	1102	593	0.03%	0.004%
24	6.419	1670	1673	1675	rBV3	1169	688	0.03%	0.004%
25	6.455	1682	1684	1685	rBV	757	272	0.01%	0.002%
26	6.481	1690	1692	1697	rBV6	1794	1656	0.07%	0.010%
27	6.590	1725	1726	1732	rBV5	1015	913	0.04%	0.006%
28	6.619	1734	1735	1736	rBV	1051	328	0.01%	0.002%
29	6.712	1762	1764	1770	rBV6	1195	811	0.04%	0.005%
30	6.751	1774	1776	1777	rBV2	963	366	0.02%	0.002%
31	6.770	1781	1782	1786	rVB4	1184	758	0.03%	0.005%
32	6.911	1816	1826	1852	rBV	245909	472742	20.47%	2.851%
33	7.136	1892	1896	1897	rBV4	1161	1007	0.04%	0.006%
34	7.239	1917	1928	1967	rBV	1031719	1828688	79.19%	11.027%
35	7.551	2016	2025	2049	rBV	162474	298177	12.91%	1.798%
36	7.956	2146	2151	2154	rBV6	1771	1480	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037178.D
 Acq On : 29 Aug 2024 23:36
 Operator : SY/MD
 Sample : P3692-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.027	2164	2173	2207	rBV	327146	712261	30.84%	4.295%
38	8.654	2366	2368	2372	rVB5	1431	700	0.03%	0.004%
39	8.677	2372	2375	2378	rBV4	1404	1082	0.05%	0.007%
40	8.779	2394	2407	2434	rBV	992259	1668206	72.24%	10.059%
41	9.403	2599	2601	2604	rBV3	1246	667	0.03%	0.004%
42	9.458	2616	2618	2622	rVB3	1624	1143	0.05%	0.007%
43	9.487	2622	2627	2629	rBV6	1940	1671	0.07%	0.010%
44	9.619	2666	2668	2671	rBV4	1073	453	0.02%	0.003%
45	9.664	2680	2682	2683	rBV	1061	477	0.02%	0.003%
46	9.741	2704	2706	2707	rBV	576	156	0.01%	0.001%
47	9.750	2707	2709	2714	rVB5	1246	832	0.04%	0.005%
48	9.776	2714	2717	2720	rBV4	1236	1081	0.05%	0.007%
49	9.815	2726	2729	2732	rBV5	1152	853	0.04%	0.005%
50	9.828	2732	2733	2734	rVV	767	164	0.01%	0.001%
51	9.876	2746	2748	2750	rBV2	1257	820	0.04%	0.005%
52	9.905	2753	2757	2760	rVB5	1831	1485	0.06%	0.009%
53	9.921	2760	2762	2764	rBV3	1292	606	0.03%	0.004%
54	9.937	2764	2767	2769	rBV3	1165	737	0.03%	0.004%
55	10.066	2805	2807	2810	rVB2	1313	528	0.02%	0.003%
56	10.149	2821	2833	2851	rBV	579807	933328	40.42%	5.628%
57	10.313	2881	2884	2888	rBV6	1501	1240	0.05%	0.007%
58	10.445	2923	2925	2927	rVB4	1029	415	0.02%	0.003%
59	10.480	2934	2936	2943	rVB7	1404	995	0.04%	0.006%
60	10.603	2970	2974	2980	rBV7	1464	1616	0.07%	0.010%
61	10.660	2990	2992	2998	rVB5	1196	1223	0.05%	0.007%
62	10.686	2998	3000	3009	rVB9	1153	800	0.03%	0.005%
63	10.850	3049	3051	3052	rBV	725	281	0.01%	0.002%
64	10.860	3052	3054	3056	rVV3	993	503	0.02%	0.003%
65	10.882	3059	3061	3064	rVB3	986	590	0.03%	0.004%
66	10.898	3064	3066	3069	rBV3	556	400	0.02%	0.002%
67	10.943	3077	3080	3082	rBV4	907	603	0.03%	0.004%
68	10.956	3082	3084	3085	rBV	1234	479	0.02%	0.003%
69	11.059	3114	3116	3118	rBV3	828	438	0.02%	0.003%
70	11.085	3121	3124	3127	rBV4	989	571	0.02%	0.003%
71	11.178	3142	3153	3173	rBV	993908	1574337	68.17%	9.493%
72	11.554	3259	3270	3299	rBV	1016403	1618003	70.07%	9.757%
73	11.824	3352	3354	3361	rVB7	1843	1650	0.07%	0.010%
74	11.956	3391	3395	3399	rBV7	998	1006	0.04%	0.006%
75	12.146	3453	3454	3457	rVB2	1125	471	0.02%	0.003%
76	12.181	3457	3465	3470	rBV8	2119	3091	0.13%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
 Data File : VV037178.D
 Acq On : 29 Aug 2024 23:36
 Operator : SY/MD
 Sample : P3692-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	12.635	3604	3606	3608	rBV3	1693	804	0.03%	0.005%
78	12.738	3635	3638	3644	rBV8	1043	812	0.04%	0.005%
79	12.799	3655	3657	3659	rBV3	1012	616	0.03%	0.004%
80	12.850	3672	3673	3675	rBV	1046	353	0.02%	0.002%
81	12.866	3675	3678	3681	rBV2	1484	857	0.04%	0.005%
82	12.892	3684	3686	3688	rBV3	978	565	0.02%	0.003%
83	12.943	3698	3702	3704	rBV5	1440	1141	0.05%	0.007%
84	13.017	3724	3725	3731	rVB5	1145	896	0.04%	0.005%
85	13.204	3780	3783	3785	rBV4	2809	1566	0.07%	0.009%
86	13.442	3855	3857	3860	rBV4	1639	856	0.04%	0.005%
87	13.564	3893	3895	3898	rBV4	1275	651	0.03%	0.004%
88	13.744	3947	3951	3953	rBV4	1022	753	0.03%	0.005%
89	13.966	4017	4020	4021	rBV3	1006	630	0.03%	0.004%
90	14.120	4064	4068	4073	rBV6	1550	1454	0.06%	0.009%
91	14.143	4073	4075	4076	rBV2	839	311	0.01%	0.002%




Sum of corrected areas: 16583835

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037178.D
Acq On : 29 Aug 2024 23:36
Operator : SY/MD
Sample : P3692-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

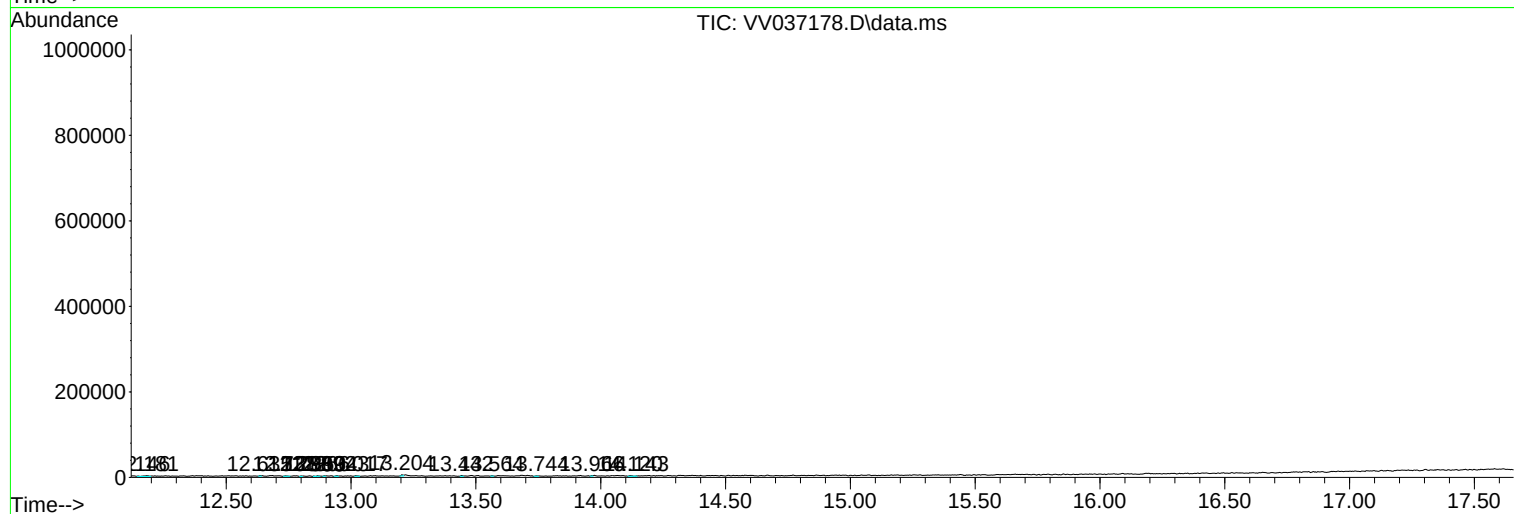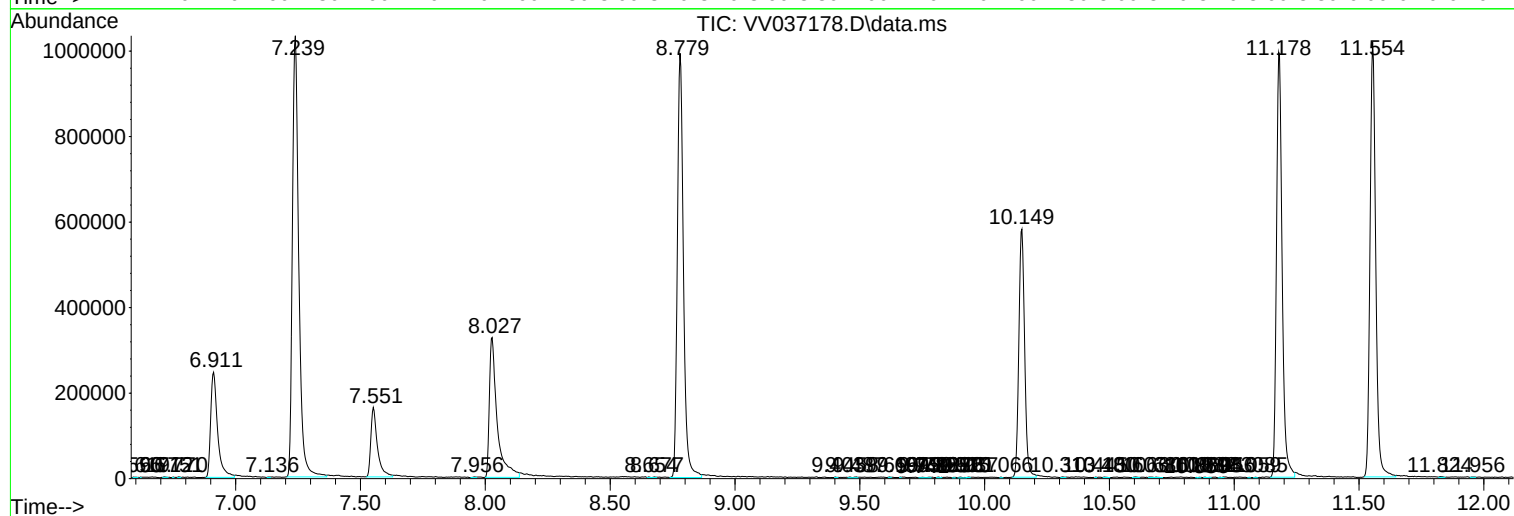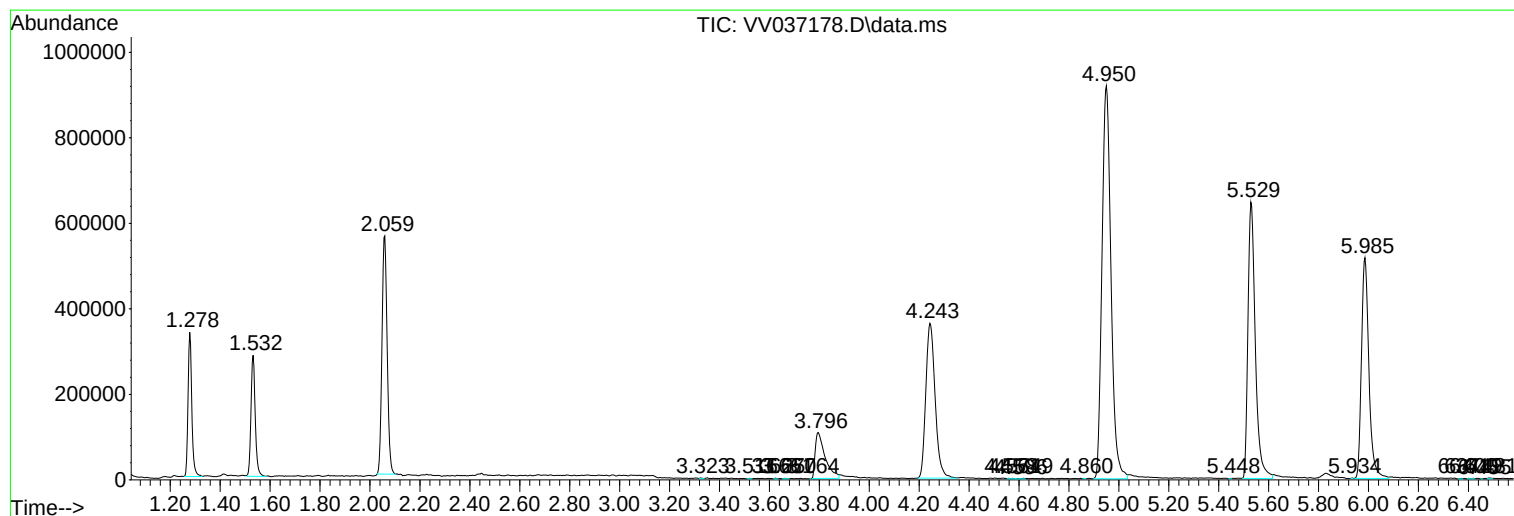

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037178.D
Acq On : 29 Aug 2024 23:36
Operator : SY/MD
Sample : P3692-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037178.D
Acq On : 29 Aug 2024 23:36
Operator : SY/MD
Sample : P3692-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc