
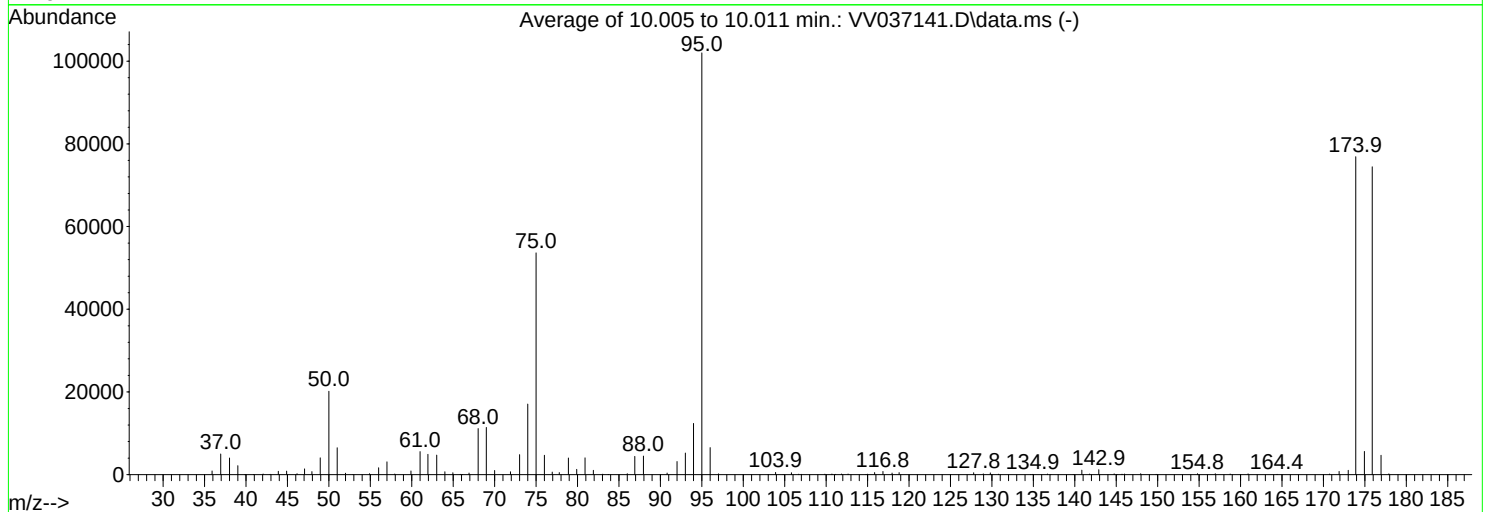


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082924\
Data File : VV037141.D
Acq On : 29 Aug 2024 08:17
Operator : SY/MD
Sample : BFB371
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB371

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis
Last Update : Fri Aug 30 01:20:16 2024

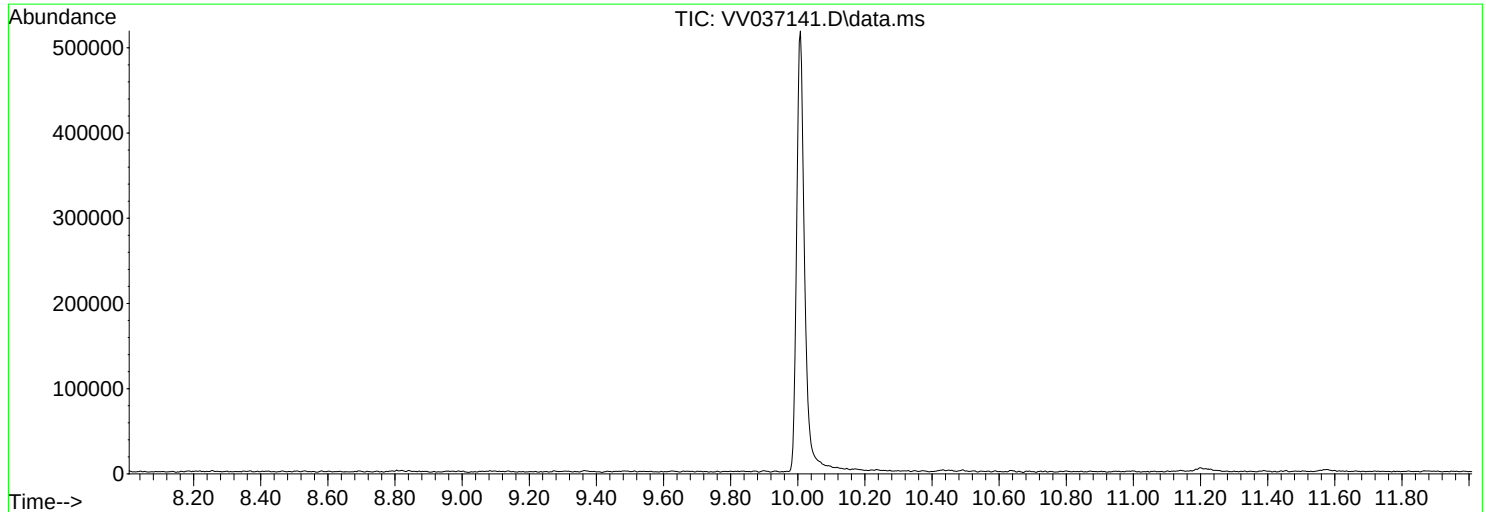

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	20173	PASS
75	95	30	80	52.6	53629	PASS
95	95	100	100	100.0	102005	PASS
96	95	5	9	6.4	6541	PASS
173	174	0.00	2	1.4	1066	PASS
174	95	50	120	75.4	76893	PASS
175	174	5	9	7.3	5619	PASS
176	174	95	105	96.8	74445	PASS
177	176	5	10	6.3	4702	PASS

m/z	Abundance
36.10	176.0
36.90	116.0
38.10	139.0
39.80	385.0
40.90	166.0
42.40	107.0
43.80	766.0
45.00	158.0
47.30	135.0
48.90	104.0
52.80	128.0
55.00	165.0
55.30	133.0
59.90	104.0
68.80	124.0
207.00	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB371

m/z	Abundance
35.90	1093.0
37.00	5120.0
38.00	4318.0
39.00	2111.0
39.90	430.0
41.00	174.0
42.10	175.0
44.00	1600.0
44.90	1086.0
46.10	209.0
47.00	1436.0
47.90	728.0
49.00	4460.0
50.00	21016.0
51.00	6630.0
52.00	397.0
53.00	167.0
54.90	437.0
56.00	1634.0
57.00	3348.0
58.00	163.0
59.90	1059.0
61.00	5644.0
62.00	5214.0
63.00	4891.0
64.00	826.0
65.00	512.0
65.80	144.0
66.90	380.0
68.00	11373.0
69.00	11416.0
70.00	1081.0
71.90	569.0
73.00	4816.0
74.00	17488.0
75.00	54536.0
76.00	4829.0
76.90	718.0
77.80	501.0
78.90	4148.0
79.90	1375.0
80.90	4233.0
81.90	897.0
83.10	144.0
86.00	171.0
86.90	4680.0
87.90	4597.0
90.80	463.0
92.00	3174.0
93.00	5510.0
94.00	12583.0
95.00	103840.0
96.00	6794.0
97.00	241.0
103.90	568.0
105.80	573.0
106.70	122.0
109.90	130.0
110.70	136.0
111.90	133.0
112.60	135.0
114.80	146.0
115.90	519.0
116.90	745.0
118.00	431.0
118.80	493.0
127.80	469.0
128.90	243.0
129.90	373.0
131.00	128.0
134.70	154.0
136.70	270.0
140.80	1083.0
141.80	188.0
142.90	1228.0
144.80	252.0
145.70	195.0
146.10	161.0
147.90	269.0
149.80	140.0
154.80	229.0
157.00	217.0
158.90	140.0
160.90	149.0
170.70	155.0
172.00	724.0
173.00	1093.0
173.90	75832.0
174.90	5794.0
175.90	72880.0
176.90	4778.0
177.90	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB371

m/z	Abundance
35.90	1112.0
37.00	5222.0
38.00	4280.0
39.00	2227.0
39.90	420.0
41.00	186.0
42.10	161.0
42.90	118.0
44.00	1612.0
44.90	1040.0
46.20	236.0
47.10	1469.0
48.00	776.0
49.00	4302.0
50.00	21024.0
51.00	6714.0
52.00	362.0
53.00	156.0
54.90	432.0
56.00	1727.0
57.00	3205.0
57.90	155.0
59.90	1025.0
61.00	5791.0
62.00	5047.0
63.00	4945.0
64.00	735.0
65.00	497.0
65.90	126.0
66.90	413.0
68.00	11602.0
69.00	11814.0
70.00	1061.0
71.90	714.0
73.00	4976.0
74.00	17512.0
75.00	55640.0
76.00	4854.0
76.90	636.0
77.80	535.0
78.90	4168.0
79.90	1345.0
80.90	4200.0
81.90	1058.0
83.10	144.0
83.70	112.0
86.00	259.0
86.90	4522.0
87.90	4605.0
90.80	396.0
92.00	3305.0
93.00	5501.0
94.00	12777.0
95.00	105464.0
96.00	6678.0
97.00	201.0
103.90	546.0
105.80	470.0
106.70	133.0
107.00	138.0
109.80	144.0
110.70	147.0
111.10	142.0
111.90	163.0
112.60	156.0
115.00	152.0
115.80	529.0
116.80	797.0
118.00	407.0
118.80	519.0
127.80	486.0
128.90	211.0
129.80	410.0
130.80	123.0
134.90	135.0
136.70	214.0
140.90	1129.0
141.80	169.0
142.90	1245.0
144.70	180.0
145.70	190.0
146.00	181.0
147.90	256.0
149.80	124.0
154.80	272.0
157.00	235.0
158.70	179.0
160.90	220.0
164.40	128.0
170.80	158.0
171.90	784.0
173.00	1074.0

Instrument :
MSVOA_V
ClientSampleId :
BFB371

173.90	79592.0
174.90	5779.0
175.90	77152.0
177.00	4915.0
177.90	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB371

m/z	Abundance
35.90	977.0
37.00	4964.0
38.00	3953.0
39.00	2131.0
39.90	370.0
40.90	210.0
42.00	152.0
42.90	118.0
44.00	1523.0
44.90	957.0
46.20	268.0
47.10	1267.0
48.00	760.0
49.00	3740.0
50.00	18480.0
51.00	6145.0
52.00	341.0
53.00	155.0
54.90	366.0
56.00	1670.0
57.00	2734.0
57.90	192.0
59.90	930.0
61.00	5260.0
61.90	4539.0
63.00	4361.0
64.00	533.0
64.80	432.0
66.10	108.0
66.90	365.0
68.00	10461.0
69.00	10998.0
70.00	847.0
71.90	766.0
73.00	4702.0
74.00	16243.0
75.00	50712.0
76.00	4309.0
77.00	541.0
77.80	499.0
78.90	3783.0
79.90	1172.0
80.90	3725.0
81.90	1155.0
83.00	125.0
86.00	258.0
86.90	3992.0
88.00	4249.0
90.80	356.0
92.00	3035.0
93.00	4717.0
94.00	11801.0
95.00	96712.0
96.00	6151.0
97.00	179.0
103.00	112.0
103.90	527.0
104.80	108.0
105.80	373.0
106.70	133.0
107.00	144.0
109.80	123.0
110.70	140.0
111.10	113.0
111.80	174.0
112.70	142.0
115.00	163.0
115.80	486.0
116.80	754.0
117.90	356.0
118.80	490.0
127.80	472.0
129.00	154.0
129.70	450.0
130.70	163.0
135.00	147.0
137.10	153.0
139.80	110.0
140.90	1060.0
141.80	138.0
142.90	1190.0
144.70	148.0
145.10	163.0
145.90	171.0
148.00	222.0
154.80	248.0
156.90	211.0
158.70	182.0
160.90	225.0
164.40	113.0
170.70	135.0
171.80	774.0

Instrument :
MSVOA_V
ClientSampleId :
BFB371

173.00	1032.0
173.90	75256.0
175.00	5284.0
175.90	73304.0
177.00	4412.0
177.90	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB371