

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
 Data File : VV037190.D
 Acq On : 30 Aug 2024 11:48
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 31 00:28:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 31 00:26:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	549571	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	538641	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	240662	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	171775	34.169	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	68.340%
7) Chloroethane-d5	1.532	69	156071	40.169	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.340%
11) 1,1-Dichloroethene-d2	2.060	65	78302	37.058	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.120%
21) 2-Butanone-d5	3.796	46	188377	96.762	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.760%
24) Chloroform-d	4.246	84	366204	46.543	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.080%
26) 1,2-Dichloroethane-d4	4.937	65	243833	49.210	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.420%
32) Benzene-d6	4.953	84	719712	44.238	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.480%
36) 1,2-Dichloropropane-d6	5.986	67	243406	47.767	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.540%
41) Toluene-d8	7.240	98	609161	41.488	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.980%
43) trans-1,3-Dichloroprop...	7.551	79	99511	42.211	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.420%
47) 2-Hexanone-d5	8.024	63	117340	84.374	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.370%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	289963	46.919	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.840%
66) 1,2-Dichlorobenzene-d4	11.554	152	235620	48.884	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.760%
Target Compounds						
39) cis-1,3-Dichloropropene	6.912	75	6526	0.992	ug/L	Qvalue # 47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037190.D
Acq On : 30 Aug 2024 11:48
Operator : SY/MD
Sample : VIBLK
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 31 00:28:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 31 00:26:21 2024
Response via : Initial Calibration

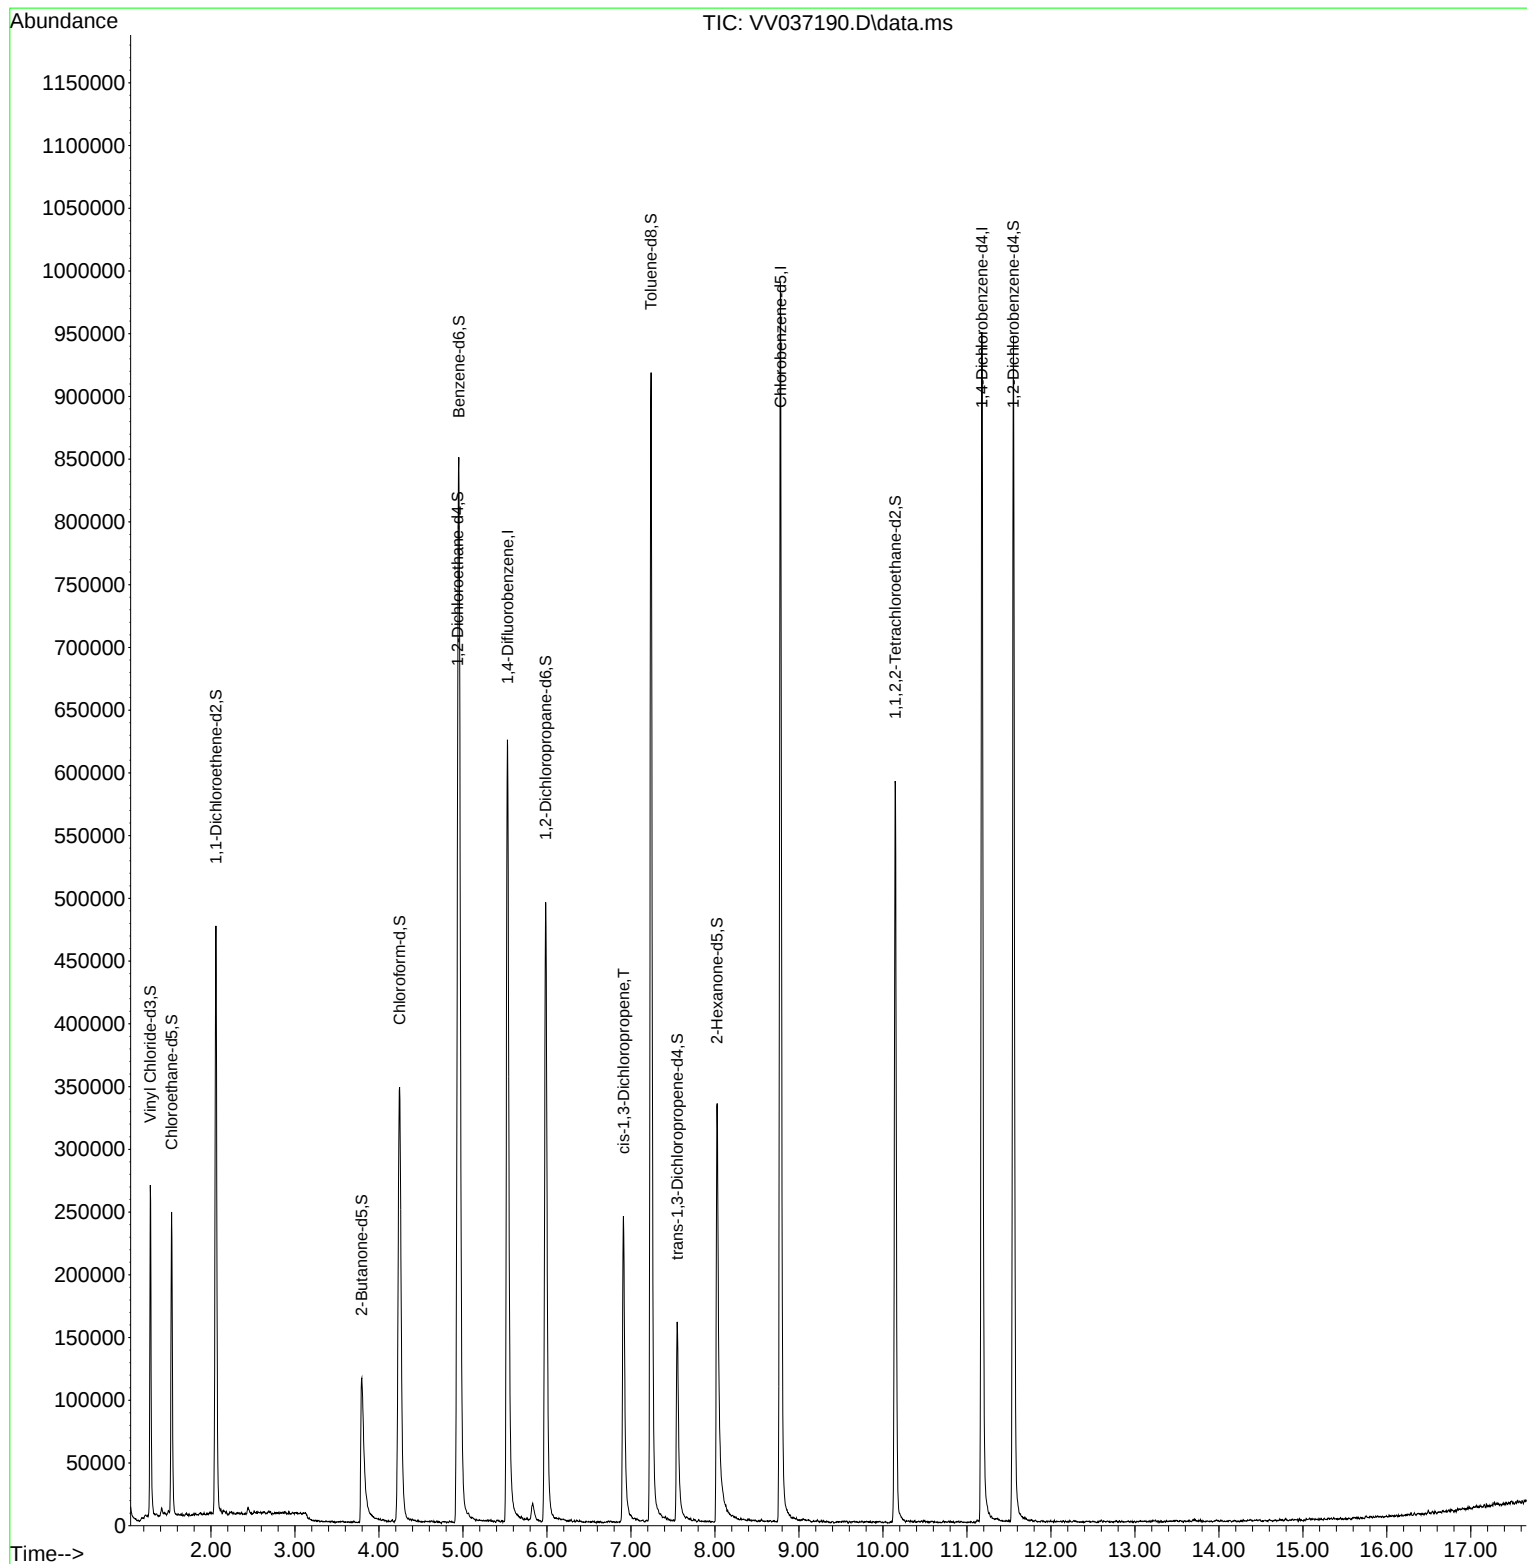

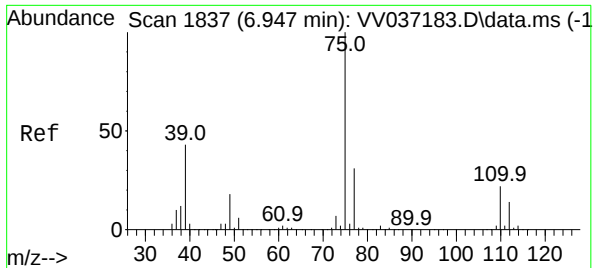

#39
 cis-1,3-Dichloropropene
 Concen: 0.992 ug/L
 RT: 6.912 min Scan# 11
 Delta R.T. -0.035 min
 Lab File: VV037190.D
 Acq: 30 Aug 2024 11:48

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 6526
 Ion Ratio Lower Upper
 75 100
 77 60.1 21.7 40.3#

