

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
 Data File : VV037187.D
 Acq On : 30 Aug 2024 10:44
 Operator : SY/MD
 Sample : VIBLK373
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK373

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	91	rVB	293379	309585	13.83%	1.874%
2	1.535	146	154	167	rVB	257394	295128	13.19%	1.787%
3	2.060	308	317	332	rBV	505657	731096	32.67%	4.426%
4	3.397	731	733	740	rBV6	1177	1187	0.05%	0.007%
5	3.545	776	779	780	rBV2	801	469	0.02%	0.003%
6	3.638	805	808	811	rBV3	1105	648	0.03%	0.004%
7	3.651	811	812	814	rBV2	486	220	0.01%	0.001%
8	3.687	818	823	826	rBV4	697	551	0.02%	0.003%
9	3.706	826	829	831	rBV3	849	542	0.02%	0.003%
10	3.799	849	858	881	rBV	110464	296220	13.24%	1.793%
11	4.246	980	997	1024	rBV2	353843	910480	40.68%	5.512%
12	4.439	1054	1057	1061	rBV5	1482	1452	0.06%	0.009%
13	4.551	1090	1092	1094	rBV3	1041	707	0.03%	0.004%
14	4.748	1150	1153	1156	rBV5	932	653	0.03%	0.004%
15	4.953	1200	1217	1255	rBV2	868106	2237960	100.00%	13.550%
16	5.368	1344	1346	1347	rBV2	1158	350	0.02%	0.002%
17	5.532	1385	1397	1432	rBV	669438	1384548	61.87%	8.383%
18	5.985	1526	1538	1568	rBV2	498737	1031482	46.09%	6.245%
19	6.252	1620	1621	1626	rVB6	1187	576	0.03%	0.003%
20	6.532	1706	1708	1710	rBV2	748	510	0.02%	0.003%
21	6.593	1725	1727	1728	rBV2	891	302	0.01%	0.002%
22	6.706	1759	1762	1764	rBV3	1141	735	0.03%	0.004%
23	6.744	1772	1774	1777	rBV4	1088	634	0.03%	0.004%
24	6.783	1783	1786	1789	rBV4	1351	917	0.04%	0.006%
25	6.802	1789	1792	1796	rBV7	1311	1039	0.05%	0.006%
26	6.834	1800	1802	1803	rBV2	491	170	0.01%	0.001%
27	6.873	1811	1814	1815	rBV	545	192	0.01%	0.001%
28	6.911	1815	1826	1853	rBV	255270	497152	22.21%	3.010%
29	7.239	1917	1928	1962	rBV	977810	1720441	76.88%	10.416%
30	7.551	2017	2025	2055	rBV	164685	313980	14.03%	1.901%
31	7.902	2132	2134	2136	rBV3	1115	623	0.03%	0.004%
32	7.947	2143	2148	2150	rBV6	1503	1459	0.07%	0.009%
33	7.982	2156	2159	2164	rBV6	1154	948	0.04%	0.006%
34	8.027	2164	2173	2225	rBV2	322800	727530	32.51%	4.405%
35	8.780	2396	2407	2435	rBV	1056612	1752423	78.30%	10.610%
36	9.204	2537	2539	2540	rBV2	1310	615	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
 Data File : VV037187.D
 Acq On : 30 Aug 2024 10:44
 Operator : SY/MD
 Sample : VIBLK373
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK373

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.455	2615	2617	2619	rBV3	807	510	0.02%	0.003%
38	9.513	2631	2635	2637	rBV4	900	764	0.03%	0.005%
39	9.625	2667	2670	2675	rBV4	1507	1577	0.07%	0.010%
40	9.648	2675	2677	2678	rBV	665	295	0.01%	0.002%
41	9.725	2699	2701	2706	rVB4	801	662	0.03%	0.004%
42	9.760	2710	2712	2714	rBV2	550	307	0.01%	0.002%
43	9.808	2723	2727	2729	rBV4	1135	866	0.04%	0.005%
44	9.844	2736	2738	2740	rBV2	1006	424	0.02%	0.003%
45	9.863	2740	2744	2748	rVV7	1164	917	0.04%	0.006%
46	9.992	2782	2784	2789	rBV6	1084	707	0.03%	0.004%
47	10.066	2805	2807	2810	rBV4	809	604	0.03%	0.004%
48	10.149	2821	2833	2857	rBV	587089	942942	42.13%	5.709%
49	10.390	2905	2908	2909	rBV3	936	533	0.02%	0.003%
50	10.468	2930	2932	2934	rBV3	1298	806	0.04%	0.005%
51	10.484	2934	2937	2939	rVV4	1293	801	0.04%	0.005%
52	10.570	2963	2964	2965	rBV	686	170	0.01%	0.001%
53	10.635	2980	2984	2987	rBV5	1289	1069	0.05%	0.006%
54	10.654	2988	2990	2995	rVB5	1310	927	0.04%	0.006%
55	10.689	2999	3001	3002	rBV2	498	226	0.01%	0.001%
56	11.005	3096	3099	3101	rBB3	910	442	0.02%	0.003%
57	11.069	3115	3119	3123	rVB4	1044	840	0.04%	0.005%
58	11.088	3123	3125	3126	rBV2	979	532	0.02%	0.003%
59	11.178	3143	3153	3187	rBV	1054815	1697599	75.85%	10.278%
60	11.554	3259	3270	3296	rBV	1001627	1616441	72.23%	9.787%
61	11.728	3320	3324	3329	rBV7	1845	2205	0.10%	0.013%
62	11.866	3364	3367	3368	rBV3	1682	1052	0.05%	0.006%
63	12.030	3413	3418	3421	rBV6	1520	1311	0.06%	0.008%
64	12.165	3458	3460	3461	rBV	913	274	0.01%	0.002%
65	12.236	3480	3482	3486	rBV4	1326	794	0.04%	0.005%
66	12.763	3642	3646	3649	rBV5	1709	1616	0.07%	0.010%
67	12.828	3664	3666	3670	rBV3	1504	797	0.04%	0.005%
68	12.988	3710	3716	3717	rBV6	1226	1202	0.05%	0.007%
69	13.156	3765	3768	3770	rBV4	1070	826	0.04%	0.005%
70	13.204	3775	3783	3793	rBV4	5349	11080	0.50%	0.067%
71	13.448	3856	3859	3861	rBV4	1330	1013	0.05%	0.006%




Sum of corrected areas: 16516655

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037187.D
Acq On : 30 Aug 2024 10:44
Operator : SY/MD
Sample : VIBLK373
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK373

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

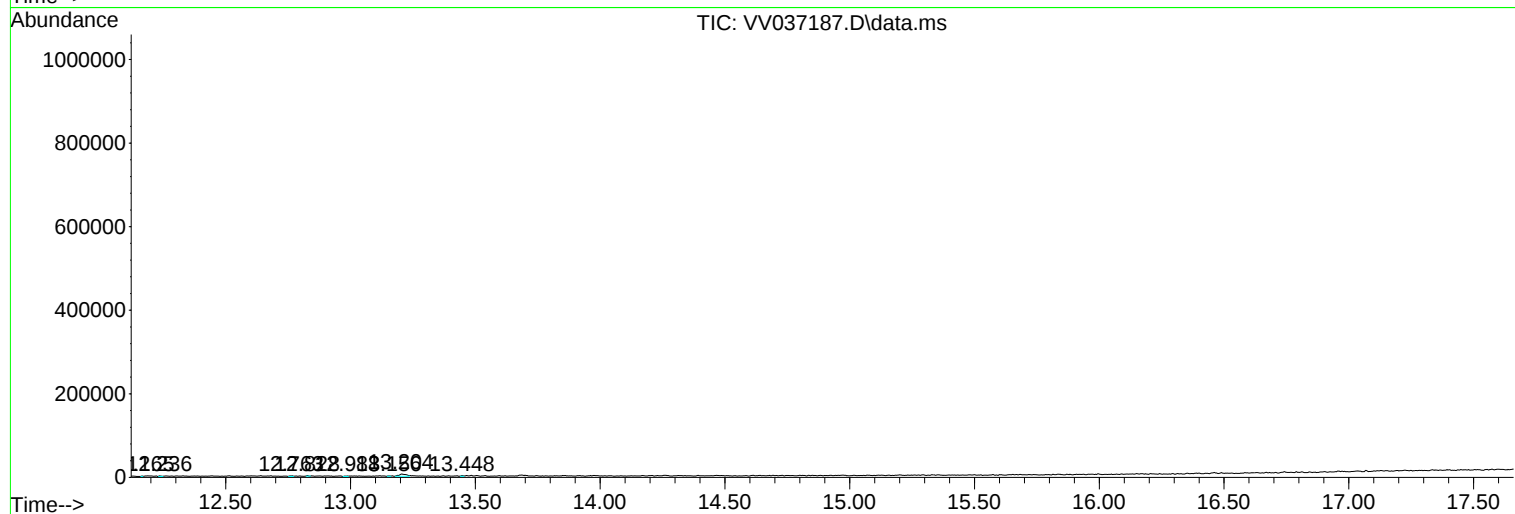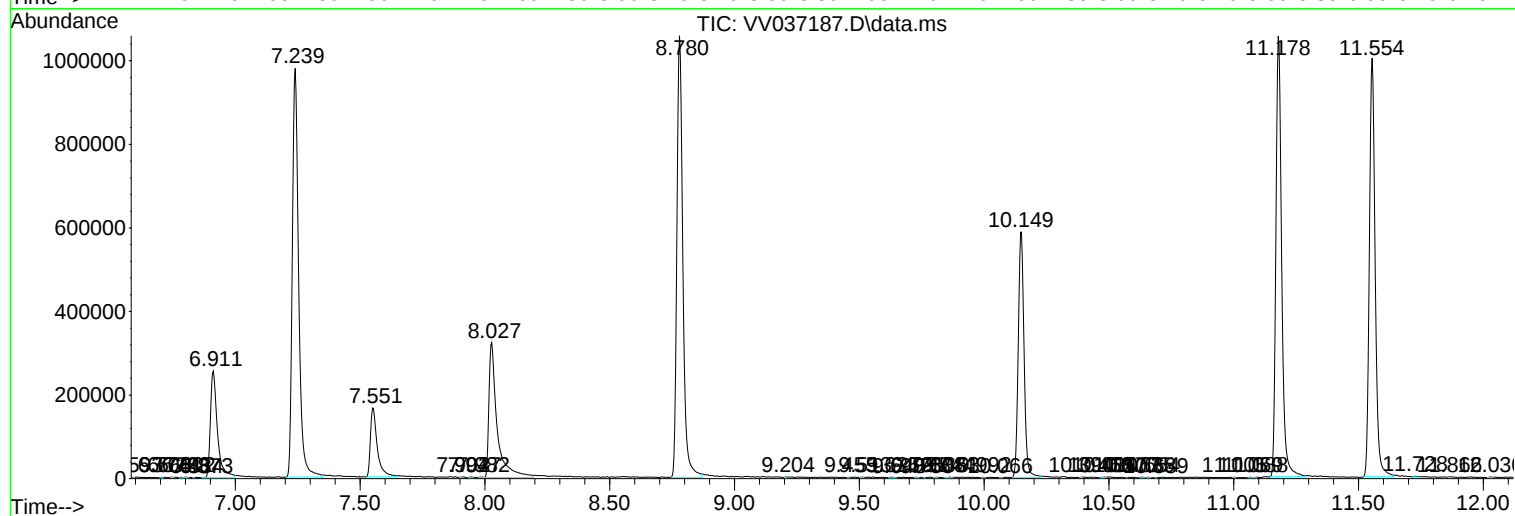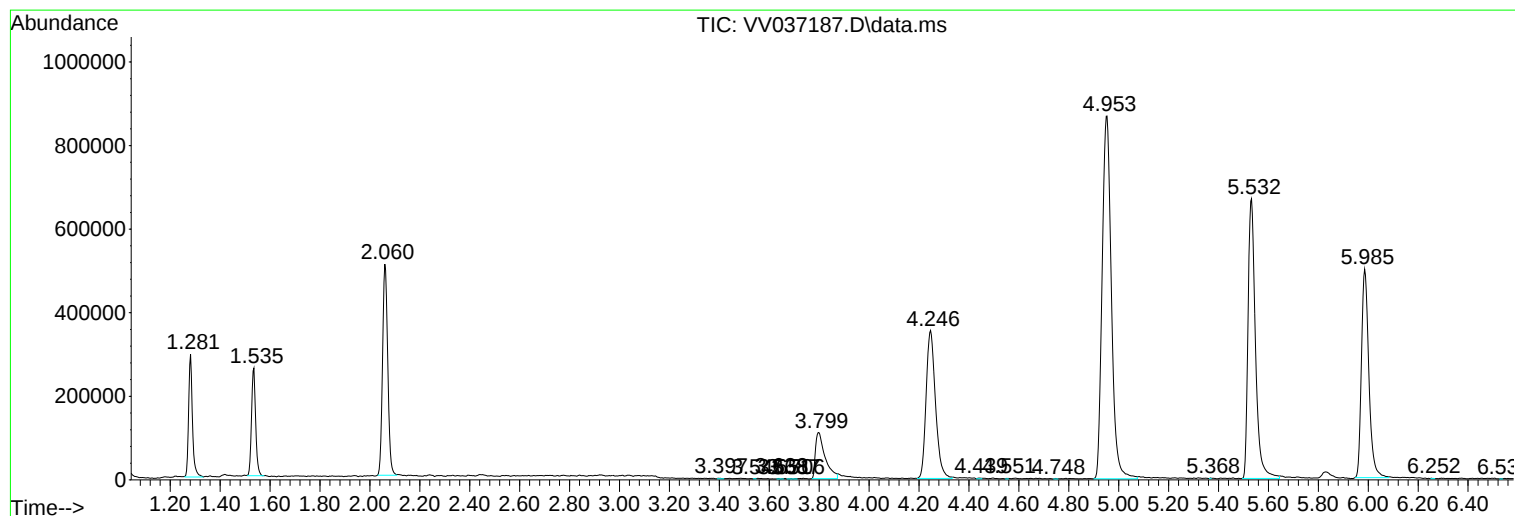

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037187.D
Acq On : 30 Aug 2024 10:44
Operator : SY/MD
Sample : VIBLK373
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK373

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037187.D
Acq On : 30 Aug 2024 10:44
Operator : SY/MD
Sample : VIBLK373
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK373

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc