

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
 Data File : VV037188.D
 Acq On : 30 Aug 2024 11:05
 Operator : SY/MD
 Sample : P3785-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	93	rBV	331447	348938	15.07%	2.044%
2	1.535	146	154	168	rBV	274273	326654	14.10%	1.914%
3	2.059	308	317	333	rBV	567388	820415	35.42%	4.806%
4	3.278	693	696	700	rVB6	1465	1222	0.05%	0.007%
5	3.391	728	731	732	rBV3	791	485	0.02%	0.003%
6	3.564	783	785	788	rVB4	1192	527	0.02%	0.003%
7	3.584	789	791	794	rVV3	798	352	0.02%	0.002%
8	3.799	849	858	894	rBV2	103626	305379	13.19%	1.789%
9	4.246	982	997	1029	rBV	363786	931099	40.20%	5.455%
10	4.503	1075	1077	1080	rBV3	872	448	0.02%	0.003%
11	4.600	1105	1107	1110	rBV4	789	483	0.02%	0.003%
12	4.616	1110	1112	1114	rVV	863	376	0.02%	0.002%
13	4.648	1114	1122	1124	rVB6	1196	1022	0.04%	0.006%
14	4.741	1147	1151	1152	rBV3	830	568	0.02%	0.003%
15	4.847	1183	1184	1185	rBV	632	124	0.01%	0.001%
16	4.953	1201	1217	1259	rBV2	916099	2316097	100.00%	13.569%
17	5.413	1358	1360	1363	rBV4	1354	862	0.04%	0.005%
18	5.532	1385	1397	1431	rBV	715850	1483215	64.04%	8.689%
19	5.985	1526	1538	1559	rBV	508812	1058215	45.69%	6.199%
20	6.384	1660	1662	1664	rBV3	766	388	0.02%	0.002%
21	6.545	1709	1712	1714	rBV5	802	496	0.02%	0.003%
22	6.606	1729	1731	1733	rVB3	909	314	0.01%	0.002%
23	6.728	1763	1769	1771	rBV7	2683	2303	0.10%	0.013%
24	6.760	1776	1779	1787	rVB9	1902	2094	0.09%	0.012%
25	6.831	1798	1801	1804	rVB3	1420	647	0.03%	0.004%
26	6.850	1804	1807	1810	rBV4	839	589	0.03%	0.003%
27	6.911	1816	1826	1846	rBV	259968	489241	21.12%	2.866%
28	7.149	1897	1900	1903	rBV4	1218	1054	0.05%	0.006%
29	7.239	1917	1928	1955	rBV	1048685	1820272	78.59%	10.664%
30	7.551	2017	2025	2053	rBV	168531	304776	13.16%	1.786%
31	7.828	2110	2111	2113	rBV2	1154	453	0.02%	0.003%
32	7.969	2152	2155	2157	rBV4	761	354	0.02%	0.002%
33	7.982	2157	2159	2162	rBV4	1077	623	0.03%	0.004%
34	8.027	2164	2173	2207	rBV2	312899	676896	29.23%	3.966%
35	8.696	2379	2381	2385	rVB3	1475	969	0.04%	0.006%
36	8.715	2385	2387	2389	rVB3	659	194	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
 Data File : VV037188.D
 Acq On : 30 Aug 2024 11:05
 Operator : SY/MD
 Sample : P3785-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.731	2389	2392	2396	rBV5	1050	830	0.04%	0.005%
38	8.779	2396	2407	2434	rBV	1119456	1836292	79.28%	10.758%
39	9.239	2546	2550	2552	rBV5	1648	1363	0.06%	0.008%
40	9.368	2588	2590	2592	rBV3	560	155	0.01%	0.001%
41	9.416	2601	2605	2607	rBV5	932	738	0.03%	0.004%
42	9.493	2627	2629	2631	rBV3	1473	652	0.03%	0.004%
43	9.532	2637	2641	2642	rBV3	1338	962	0.04%	0.006%
44	9.603	2660	2663	2664	rBV3	680	453	0.02%	0.003%
45	9.664	2680	2682	2684	rBV3	430	244	0.01%	0.001%
46	9.677	2684	2686	2690	rVB4	687	285	0.01%	0.002%
47	9.763	2707	2713	2714	rBV4	1878	1472	0.06%	0.009%
48	9.879	2744	2749	2753	rVB8	1758	1771	0.08%	0.010%
49	9.898	2753	2755	2761	rBV6	904	905	0.04%	0.005%
50	9.950	2768	2771	2774	rVB3	1135	770	0.03%	0.005%
51	9.966	2774	2776	2777	rBV2	827	254	0.01%	0.001%
52	9.979	2777	2780	2783	rBV4	1229	803	0.03%	0.005%
53	10.017	2788	2792	2794	rBV3	1094	749	0.03%	0.004%
54	10.149	2821	2833	2856	rBV	570973	915256	39.52%	5.362%
55	10.355	2894	2897	2900	rBV5	1026	612	0.03%	0.004%
56	10.419	2916	2917	2919	rVB	893	190	0.01%	0.001%
57	10.439	2919	2923	2927	rBV7	1303	1079	0.05%	0.006%
58	10.625	2976	2981	2983	rBV2	1290	1142	0.05%	0.007%
59	10.686	2997	3000	3004	rBV6	1364	941	0.04%	0.006%
60	10.840	3046	3048	3050	rVB3	1373	505	0.02%	0.003%
61	10.853	3050	3052	3053	rBV2	450	166	0.01%	0.001%
62	10.866	3055	3056	3059	rVB2	772	428	0.02%	0.003%
63	11.037	3104	3109	3111	rBV7	1282	1312	0.06%	0.008%
64	11.066	3115	3118	3120	rBV2	1057	646	0.03%	0.004%
65	11.101	3125	3129	3131	rBV3	1213	770	0.03%	0.005%
66	11.123	3131	3136	3139	rBV5	2261	2174	0.09%	0.013%
67	11.181	3143	3154	3183	rBV	1092546	1757417	75.88%	10.296%
68	11.506	3254	3255	3258	rBV3	1210	923	0.04%	0.005%
69	11.554	3259	3270	3292	rVV	1019951	1625806	70.20%	9.525%
70	11.988	3404	3405	3408	rBV3	924	510	0.02%	0.003%
71	12.297	3498	3501	3503	rBV3	1135	729	0.03%	0.004%
72	12.377	3521	3526	3531	rBV8	1826	2324	0.10%	0.014%
73	12.529	3572	3573	3574	rBV	477	113	0.00%	0.001%
74	12.590	3589	3592	3594	rBV3	1309	752	0.03%	0.004%
75	12.676	3616	3619	3621	rBV4	1655	817	0.04%	0.005%
76	12.799	3653	3657	3658	rBV3	1197	666	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037188.D
Acq On : 30 Aug 2024 11:05
Operator : SY/MD
Sample : P3785-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	12.882	3679	3683	3684	rBV2	913	635	0.03%	0.004%
78	13.004	3720	3721	3725	rBV3	978	582	0.03%	0.003%
79	13.101	3747	3751	3754	rBV5	1221	1180	0.05%	0.007%
80	13.291	3808	3810	3811	rBV3	461	197	0.01%	0.001%
81	13.384	3837	3839	3840	rBV2	771	255	0.01%	0.001%
82	13.551	3889	3891	3892	rBV2	857	244	0.01%	0.001%
83	13.892	3994	3997	4000	rBV5	1222	957	0.04%	0.006%
84	14.114	4064	4066	4068	rBV3	921	438	0.02%	0.003%
85	14.130	4069	4071	4077	rVV7	1630	1420	0.06%	0.008%
86	14.612	4219	4221	4225	rBV3	1553	1456	0.06%	0.009%




Sum of corrected areas: 17069484

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037188.D
Acq On : 30 Aug 2024 11:05
Operator : SY/MD
Sample : P3785-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

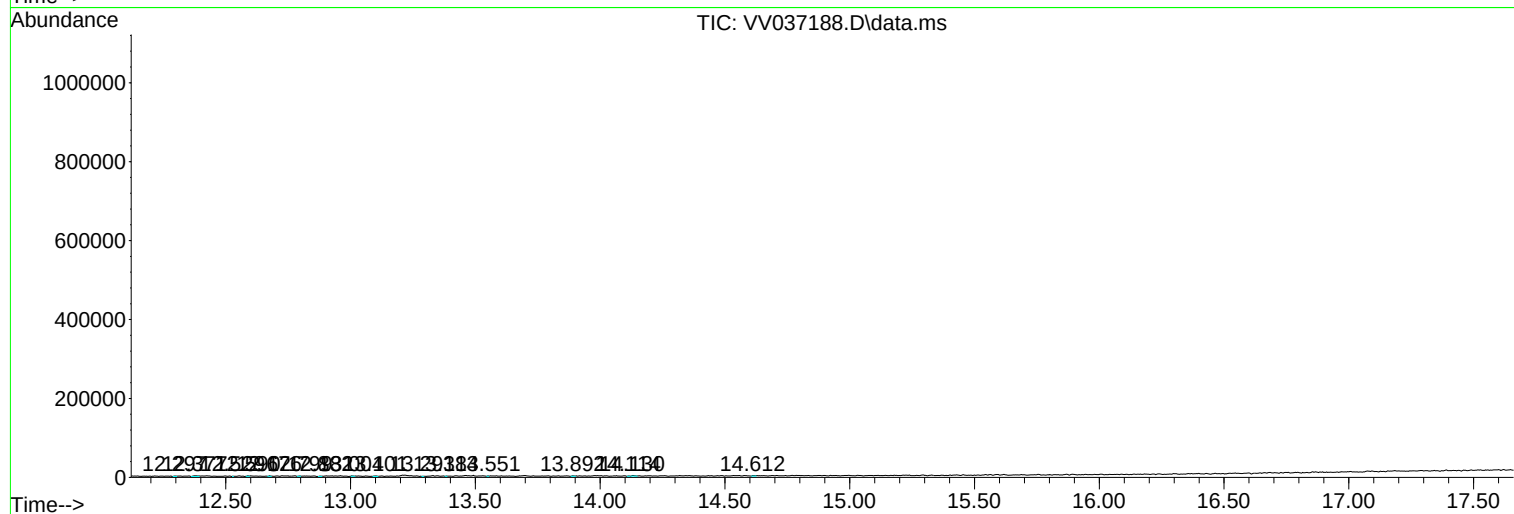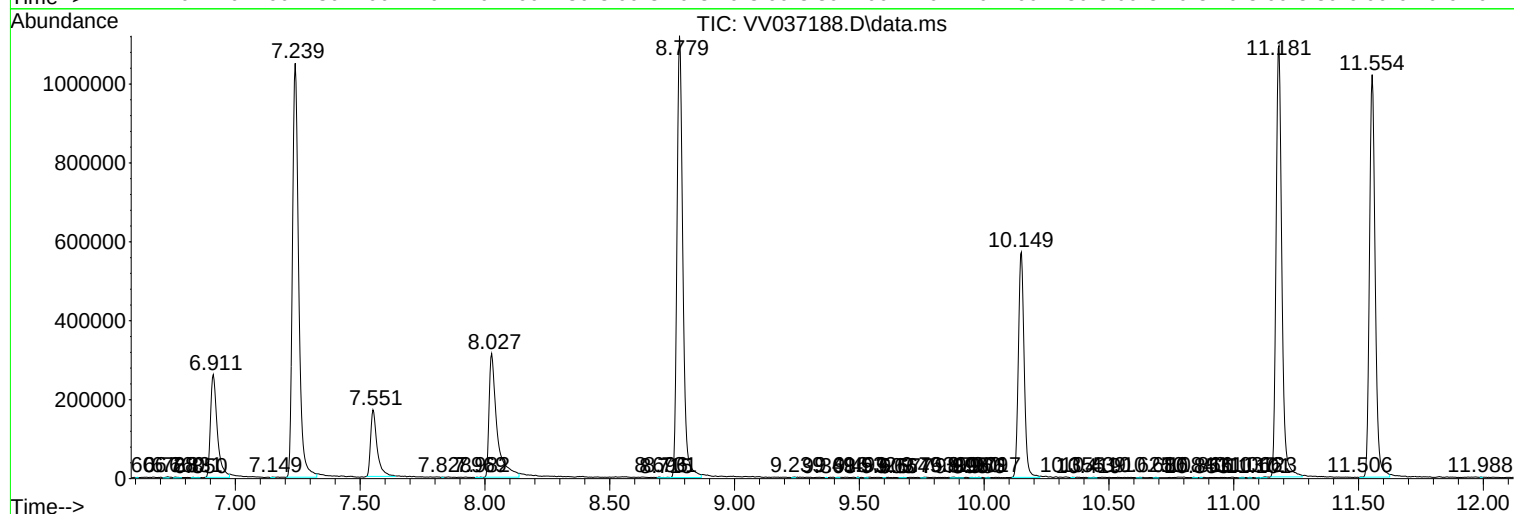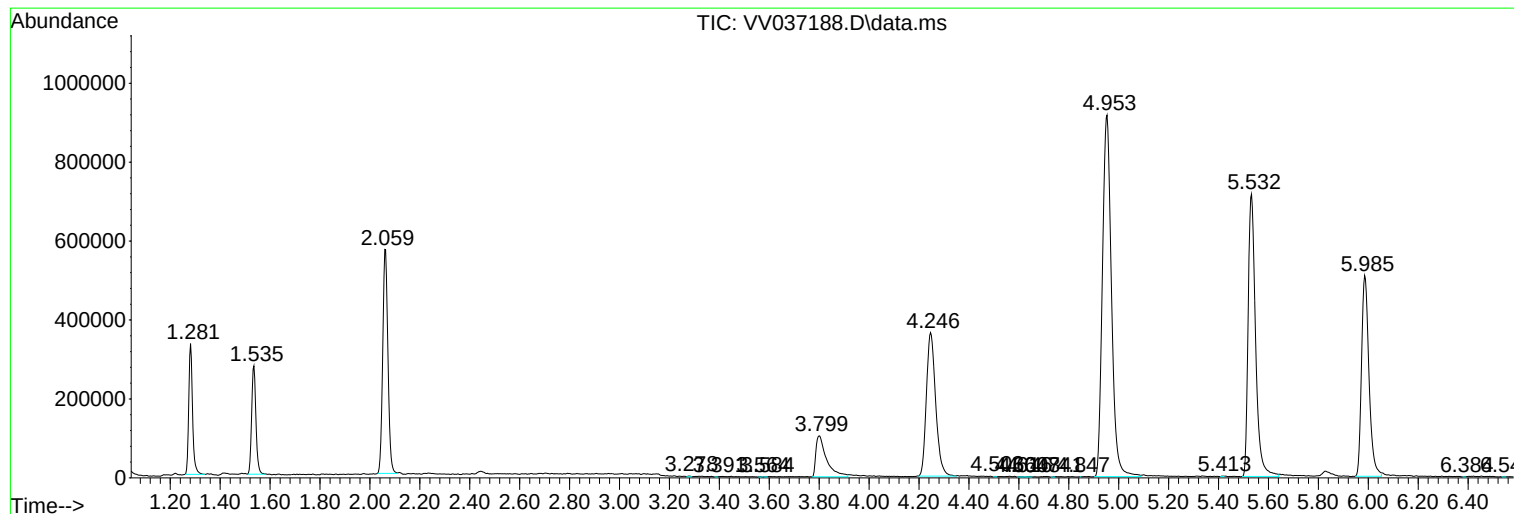

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037188.D
Acq On : 30 Aug 2024 11:05
Operator : SY/MD
Sample : P3785-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037188.D
Acq On : 30 Aug 2024 11:05
Operator : SY/MD
Sample : P3785-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------