

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
 Data File : VV037190.D
 Acq On : 30 Aug 2024 11:48
 Operator : SY/MD
 Sample : VIBLK374
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	262052	273449	12.52%	1.741%
2	1.532	146	153	170	rVB	241259	286848	13.13%	1.826%
3	2.060	308	317	330	rBV	465582	665687	30.47%	4.238%
4	3.487	759	761	762	rBV	771	278	0.01%	0.002%
5	3.593	792	794	795	rBV2	575	259	0.01%	0.002%
6	3.664	814	816	820	rBV5	756	480	0.02%	0.003%
7	3.696	823	826	828	rBV4	1110	628	0.03%	0.004%
8	3.796	848	857	889	rBV	115380	330633	15.13%	2.105%
9	4.246	982	997	1024	rBV	345031	882148	40.38%	5.616%
10	4.510	1077	1079	1082	rBV4	947	503	0.02%	0.003%
11	4.548	1089	1091	1093	rBV3	1050	483	0.02%	0.003%
12	4.722	1143	1145	1149	rVB4	1225	780	0.04%	0.005%
13	4.751	1152	1154	1155	rBV	1274	652	0.03%	0.004%
14	4.818	1171	1175	1179	rBV4	872	785	0.04%	0.005%
15	4.841	1179	1182	1188	rBV6	1351	1340	0.06%	0.009%
16	4.950	1200	1216	1248	rBV2	849296	2184665	100.00%	13.908%
17	5.159	1279	1281	1286	rBV6	1539	1243	0.06%	0.008%
18	5.404	1353	1357	1358	rBV4	1906	1297	0.06%	0.008%
19	5.458	1372	1374	1376	rBV2	946	428	0.02%	0.003%
20	5.529	1385	1396	1432	rBV	622971	1300438	59.53%	8.279%
21	5.941	1522	1524	1525	rBV2	866	363	0.02%	0.002%
22	5.986	1525	1538	1563	rVV	493410	1019603	46.67%	6.491%
23	6.529	1705	1707	1709	rBV4	597	272	0.01%	0.002%
24	6.564	1715	1718	1719	rBV3	904	363	0.02%	0.002%
25	6.603	1727	1730	1735	rBV7	1258	1337	0.06%	0.009%
26	6.635	1738	1740	1743	rVB4	993	586	0.03%	0.004%
27	6.683	1751	1755	1757	rBV5	796	598	0.03%	0.004%
28	6.793	1788	1789	1791	rBV2	602	302	0.01%	0.002%
29	6.825	1798	1799	1801	rBV2	781	353	0.02%	0.002%
30	6.912	1817	1826	1848	rBV	242149	456394	20.89%	2.906%
31	7.240	1917	1928	1959	rBV	915231	1624714	74.37%	10.344%
32	7.551	2016	2025	2053	rBV	158406	304391	13.93%	1.938%
33	8.027	2164	2173	2204	rBV2	333194	704767	32.26%	4.487%
34	8.780	2396	2407	2440	rBV	986719	1635696	74.87%	10.414%
35	9.265	2557	2558	2563	rVB3	1224	600	0.03%	0.004%
36	9.288	2563	2565	2569	rVB4	1301	887	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
 Data File : VV037190.D
 Acq On : 30 Aug 2024 11:48
 Operator : SY/MD
 Sample : VIBLK374
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.378	2591	2593	2595	rBV2	587	320	0.01%	0.002%
38	9.391	2595	2597	2599	rBV3	923	547	0.03%	0.003%
39	9.423	2605	2607	2608	rBV2	317	141	0.01%	0.001%
40	9.455	2614	2617	2618	rBV3	923	517	0.02%	0.003%
41	9.516	2634	2636	2639	rBV3	1026	625	0.03%	0.004%
42	9.600	2658	2662	2665	rBV4	1679	1360	0.06%	0.009%
43	9.625	2668	2670	2671	rBV2	871	421	0.02%	0.003%
44	9.783	2717	2719	2721	rBV3	675	260	0.01%	0.002%
45	9.850	2738	2740	2741	rBV2	1034	417	0.02%	0.003%
46	9.879	2746	2749	2750	rBV	1203	636	0.03%	0.004%
47	9.918	2758	2761	2762	rBV3	1119	577	0.03%	0.004%
48	10.059	2803	2805	2809	rVB4	448	335	0.02%	0.002%
49	10.088	2809	2814	2817	rBV6	1206	1089	0.05%	0.007%
50	10.104	2817	2819	2820	rBV2	713	197	0.01%	0.001%
51	10.146	2820	2832	2855	rBV	590567	946047	43.30%	6.023%
52	10.329	2887	2889	2892	rBV4	1333	848	0.04%	0.005%
53	10.381	2901	2905	2910	rVB5	1802	1376	0.06%	0.009%
54	10.413	2910	2915	2916	rBV5	685	625	0.03%	0.004%
55	10.484	2935	2937	2941	rBV5	1257	899	0.04%	0.006%
56	10.548	2954	2957	2960	rBV4	1112	910	0.04%	0.006%
57	10.616	2976	2978	2982	rBV3	1007	619	0.03%	0.004%
58	10.654	2989	2990	2992	rVB2	756	185	0.01%	0.001%
59	10.670	2992	2995	2996	rBV4	498	229	0.01%	0.001%
60	10.709	3003	3007	3008	rBV4	738	442	0.02%	0.003%
61	10.719	3008	3010	3014	rVB4	1419	797	0.04%	0.005%
62	10.735	3014	3015	3018	rBV2	868	535	0.02%	0.003%
63	10.802	3033	3036	3038	rBV3	1222	539	0.02%	0.003%
64	10.841	3046	3048	3051	rVB2	1530	772	0.04%	0.005%
65	10.873	3051	3058	3061	rBV8	1374	1502	0.07%	0.010%
66	10.918	3070	3072	3075	rBV4	1011	610	0.03%	0.004%
67	10.963	3084	3086	3089	rBV3	626	310	0.01%	0.002%
68	11.011	3099	3101	3104	rBV4	848	566	0.03%	0.004%
69	11.082	3121	3123	3127	rVB3	1454	850	0.04%	0.005%
70	11.114	3128	3133	3134	rBV5	1575	1074	0.05%	0.007%
71	11.178	3143	3153	3179	rBV	947840	1525620	69.83%	9.713%
72	11.554	3258	3270	3294	rBV	944386	1515866	69.39%	9.651%
73	11.953	3389	3394	3397	rBV5	1392	1171	0.05%	0.007%
74	12.040	3418	3421	3424	rBV5	1875	1061	0.05%	0.007%
75	12.194	3467	3469	3472	rVB3	891	434	0.02%	0.003%
76	12.210	3472	3474	3477	rBV3	846	421	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
 Data File : VV037190.D
 Acq On : 30 Aug 2024 11:48
 Operator : SY/MD
 Sample : VIBLK374
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	12.226	3477	3479	3482	rBV4	1284	609	0.03%	0.004%
78	12.548	3577	3579	3580	rBV	303	84	0.00%	0.001%
79	12.561	3581	3583	3584	rBV2	1034	330	0.02%	0.002%
80	12.622	3600	3602	3604	rBV3	1011	435	0.02%	0.003%
81	12.715	3629	3631	3635	rBV2	911	564	0.03%	0.004%
82	12.751	3640	3642	3645	rBV3	824	600	0.03%	0.004%
83	12.802	3657	3658	3660	rBV	644	340	0.02%	0.002%
84	12.995	3713	3718	3721	rBV4	1251	1240	0.06%	0.008%
85	13.021	3725	3726	3728	rBV2	782	343	0.02%	0.002%
86	13.291	3809	3810	3814	rBV3	1033	628	0.03%	0.004%
87	13.310	3814	3816	3819	rVB3	1575	954	0.04%	0.006%
88	13.374	3833	3836	3839	rBV5	1655	1100	0.05%	0.007%
89	13.596	3899	3905	3907	rBV6	1512	1707	0.08%	0.011%
90	14.255	4107	4110	4111	rBV2	1217	571	0.03%	0.004%
91	14.956	4324	4328	4331	rBV7	2360	1933	0.09%	0.012%




Sum of corrected areas: 15707438

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037190.D
Acq On : 30 Aug 2024 11:48
Operator : SY/MD
Sample : VIBLK374
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK374

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

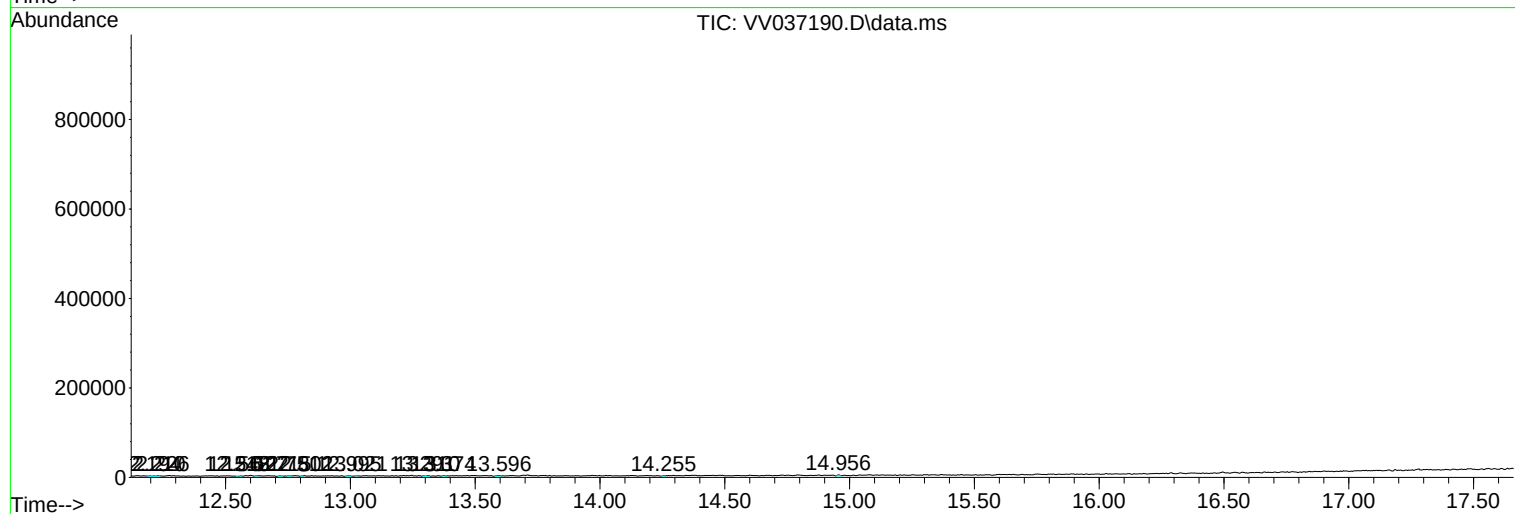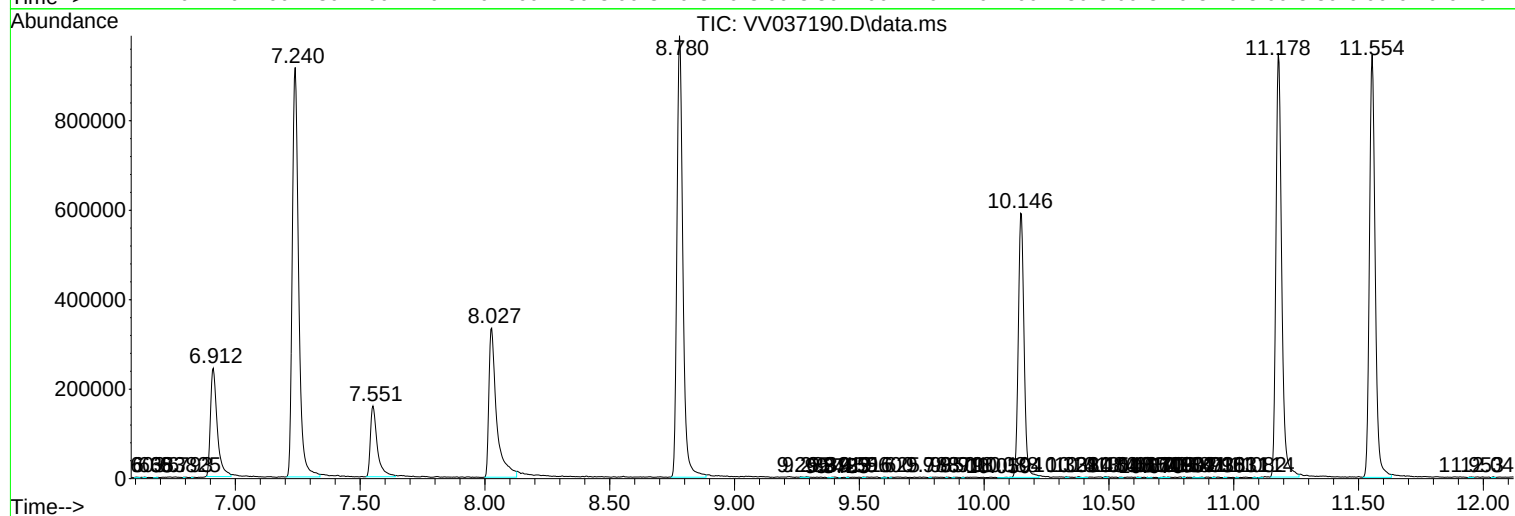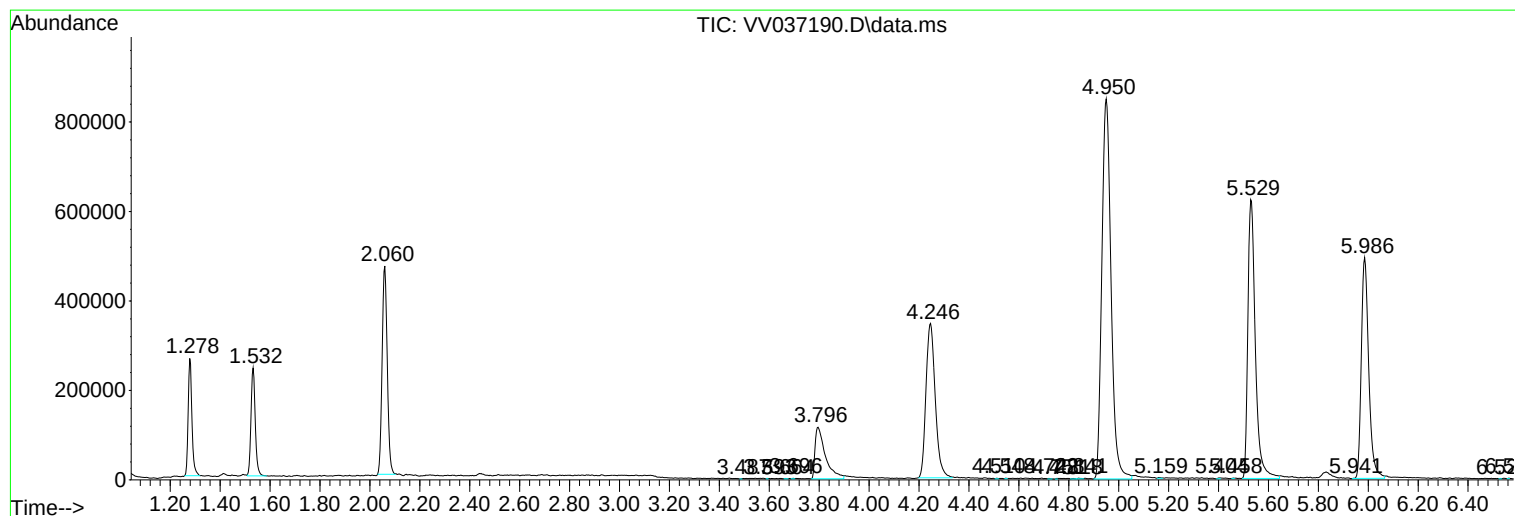

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037190.D
Acq On : 30 Aug 2024 11:48
Operator : SY/MD
Sample : VIBLK374
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK374

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037190.D
Acq On : 30 Aug 2024 11:48
Operator : SY/MD
Sample : VIBLK374
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK374

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc