
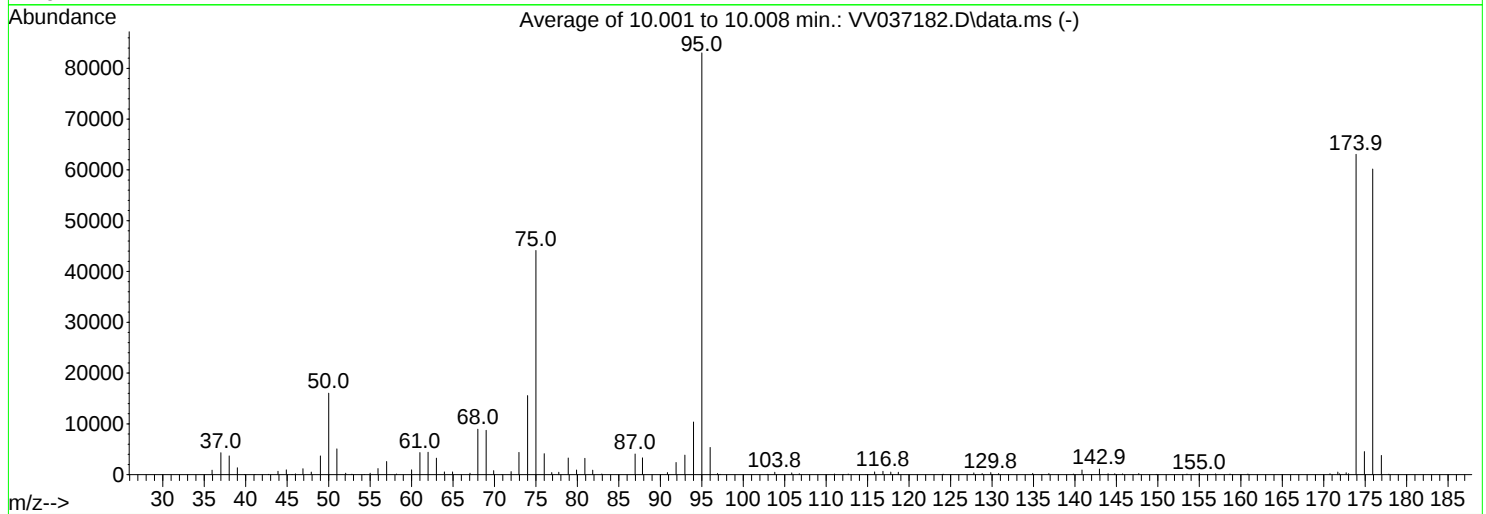


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083024\
Data File : VV037182.D
Acq On : 30 Aug 2024 08:00
Operator : SY/MD
Sample : BFB372
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB372

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis
Last Update : Sat Aug 31 00:26:21 2024

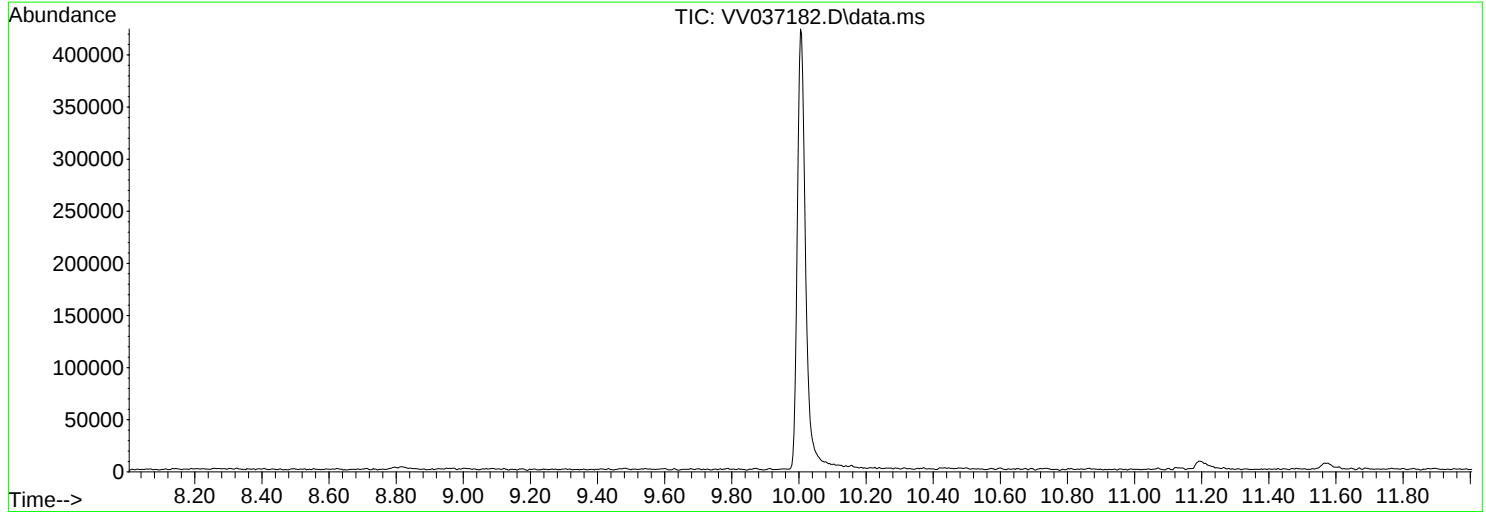

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2777

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	16047	PASS
75	95	30	80	53.1	44133	PASS
95	95	100	100	100.0	83048	PASS
96	95	5	9	6.5	5364	PASS
173	174	0.00	2	0.6	378	PASS
174	95	50	120	75.9	63064	PASS
175	174	5	9	7.2	4536	PASS
176	174	95	105	95.4	60181	PASS
177	176	5	10	6.3	3779	PASS

m/z	Abundance
35.20	146.0
38.40	166.0
39.10	194.0
39.80	334.0
40.90	152.0
41.70	170.0
43.00	143.0
44.00	595.0
47.80	116.0
50.20	122.0
51.30	100.0
56.10	118.0
57.70	114.0
77.10	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

m/z	Abundance
36.00	894.0
37.00	4221.0
38.00	3417.0
39.00	1515.0
39.90	371.0
41.10	103.0
41.80	132.0
42.70	123.0
43.10	106.0
43.90	1180.0
44.90	865.0
46.00	171.0
46.90	994.0
47.90	547.0
49.00	3607.0
50.00	16066.0
51.00	4775.0
52.10	287.0
52.80	150.0
55.00	277.0
56.00	1194.0
57.00	2698.0
60.00	832.0
61.00	4397.0
62.00	4485.0
63.00	3154.0
64.00	529.0
64.90	513.0
67.10	306.0
68.00	8488.0
69.00	8290.0
69.90	749.0
70.90	128.0
72.00	613.0
72.90	4422.0
74.00	14873.0
75.00	41600.0
76.00	3851.0
76.90	554.0
77.70	477.0
78.90	3085.0
79.90	864.0
80.90	3092.0
81.80	751.0
83.00	105.0
86.90	3804.0
87.90	3335.0
90.80	392.0
91.90	2332.0
93.00	3708.0
94.00	9975.0
95.00	77776.0
96.00	5274.0
96.90	222.0
103.80	429.0
105.80	321.0
106.70	173.0
111.00	116.0
112.10	110.0
112.60	122.0
115.90	543.0
116.80	655.0
117.80	491.0
118.70	428.0
124.10	129.0
127.80	368.0
128.80	191.0
129.90	395.0
130.80	188.0
134.80	208.0
136.80	155.0
139.80	120.0
140.80	765.0
143.00	1005.0
144.00	168.0
144.90	143.0
145.80	120.0
147.70	185.0
153.50	127.0
155.00	234.0
156.90	199.0
158.80	144.0
170.70	185.0
171.80	442.0
171.90	441.0
173.00	610.0
173.90	58936.0
174.90	4089.0
175.90	56008.0
177.00	3533.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

m/z	Abundance
35.90	947.0
37.00	4506.0
38.00	3812.0
39.00	1625.0
39.90	396.0
41.80	126.0
43.20	130.0
43.90	1304.0
44.90	1025.0
45.60	140.0
46.00	152.0
46.90	1226.0
48.00	670.0
49.00	3730.0
50.00	16560.0
51.00	5234.0
52.00	265.0
52.80	129.0
55.00	277.0
55.90	1367.0
57.00	2627.0
58.20	164.0
60.00	996.0
61.00	4502.0
62.00	4605.0
63.00	3318.0
63.90	591.0
64.90	555.0
67.10	300.0
68.00	9298.0
69.00	8984.0
69.90	871.0
72.00	602.0
72.90	4500.0
74.00	16042.0
75.00	45704.0
76.00	4285.0
76.90	554.0
77.70	485.0
78.90	3371.0
79.90	985.0
80.90	3310.0
81.90	692.0
83.00	130.0
87.00	4276.0
87.90	3388.0
90.80	426.0
91.90	2437.0
93.00	3940.0
94.00	10770.0
95.00	85792.0
96.00	5579.0
96.90	231.0
102.90	118.0
103.80	510.0
105.80	339.0
106.70	194.0
111.00	135.0
112.70	120.0
115.80	573.0
116.90	646.0
117.80	508.0
118.70	500.0
124.10	119.0
127.80	344.0
128.80	235.0
129.80	441.0
130.80	232.0
134.90	234.0
136.80	219.0
139.80	142.0
140.80	959.0
143.00	1147.0
144.00	218.0
144.80	187.0
145.70	155.0
147.70	269.0
149.80	113.0
153.50	148.0
155.00	249.0
157.00	181.0
158.70	140.0
160.90	130.0
170.70	238.0
171.70	517.0
172.70	587.0
173.90	65216.0
174.90	4675.0
175.90	62208.0
176.90	3872.0
177.90	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

m/z	Abundance
36.00	838.0
37.00	4200.0
38.00	3807.0
39.00	1513.0
40.00	388.0
40.80	188.0
41.80	141.0
42.80	102.0
43.20	136.0
43.90	1324.0
44.90	968.0
46.00	144.0
46.90	1326.0
47.90	669.0
49.00	3718.0
50.00	15880.0
51.00	5253.0
52.00	263.0
54.30	102.0
55.00	279.0
55.90	1435.0
57.00	2405.0
58.20	189.0
60.00	985.0
61.00	4118.0
62.00	4166.0
63.00	3236.0
63.90	516.0
65.00	553.0
66.90	253.0
68.00	9036.0
69.00	8924.0
69.90	794.0
72.00	570.0
73.00	4211.0
74.00	15768.0
75.00	45096.0
76.00	4255.0
76.90	598.0
77.80	479.0
78.90	3344.0
79.90	923.0
80.90	3239.0
81.80	584.0
82.00	581.0
82.90	152.0
87.00	4148.0
87.80	3185.0
90.90	396.0
91.90	2441.0
92.90	3912.0
94.00	10339.0
95.00	85576.0
96.00	5239.0
96.90	191.0
97.20	188.0
102.90	117.0
103.80	512.0
105.90	421.0
106.80	165.0
111.00	108.0
112.70	107.0
114.80	110.0
115.80	503.0
116.90	646.0
117.80	508.0
118.70	522.0
127.80	304.0
128.80	243.0
129.90	378.0
130.80	243.0
135.00	281.0
136.90	314.0
139.80	167.0
140.90	1001.0
142.90	1111.0
144.00	179.0
144.70	233.0
145.70	158.0
147.70	241.0
149.80	107.0
153.50	115.0
155.00	206.0
157.00	142.0
158.60	132.0
160.80	205.0
170.80	192.0
171.60	536.0
172.70	547.0
173.90	65040.0
174.90	4844.0
175.90	62328.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

176.903932.0

177.80157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372