

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037225.D
 Acq On : 06 Sep 2024 14:55
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 06 23:25:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 06 23:21:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	662634	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	641839	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	299962	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	188809	31.149	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	62.300%		
7) Chloroethane-d5	1.532	69	165989	35.432	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	70.860%		
11) 1,1-Dichloroethene-d2	2.060	65	88378	34.690	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.380%		
21) 2-Butanone-d5	3.796	46	184464	78.585	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	78.590%		
24) Chloroform-d	4.246	84	376035	39.638	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.280%		
26) 1,2-Dichloroethane-d4	4.937	65	245316	41.062	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.120%		
32) Benzene-d6	4.953	84	762559	39.335	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.680%		
36) 1,2-Dichloropropane-d6	5.985	67	253049	41.675	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	83.360%		
41) Toluene-d8	7.239	98	647028	36.981	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.960%#		
43) trans-1,3-Dichloroprop...	7.551	79	100553	35.795	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.580%		
47) 2-Hexanone-d5	8.024	63	111419	67.235	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	67.240%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	289431	39.303	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	78.600%		
66) 1,2-Dichlorobenzene-d4	11.554	152	255985	42.610	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.220%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.915	75	6526	0.833	ug/L	# 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037225.D
Acq On : 06 Sep 2024 14:55
Operator : SY/MD
Sample : VIBLK
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 06 23:25:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 06 23:21:35 2024
Response via : Initial Calibration

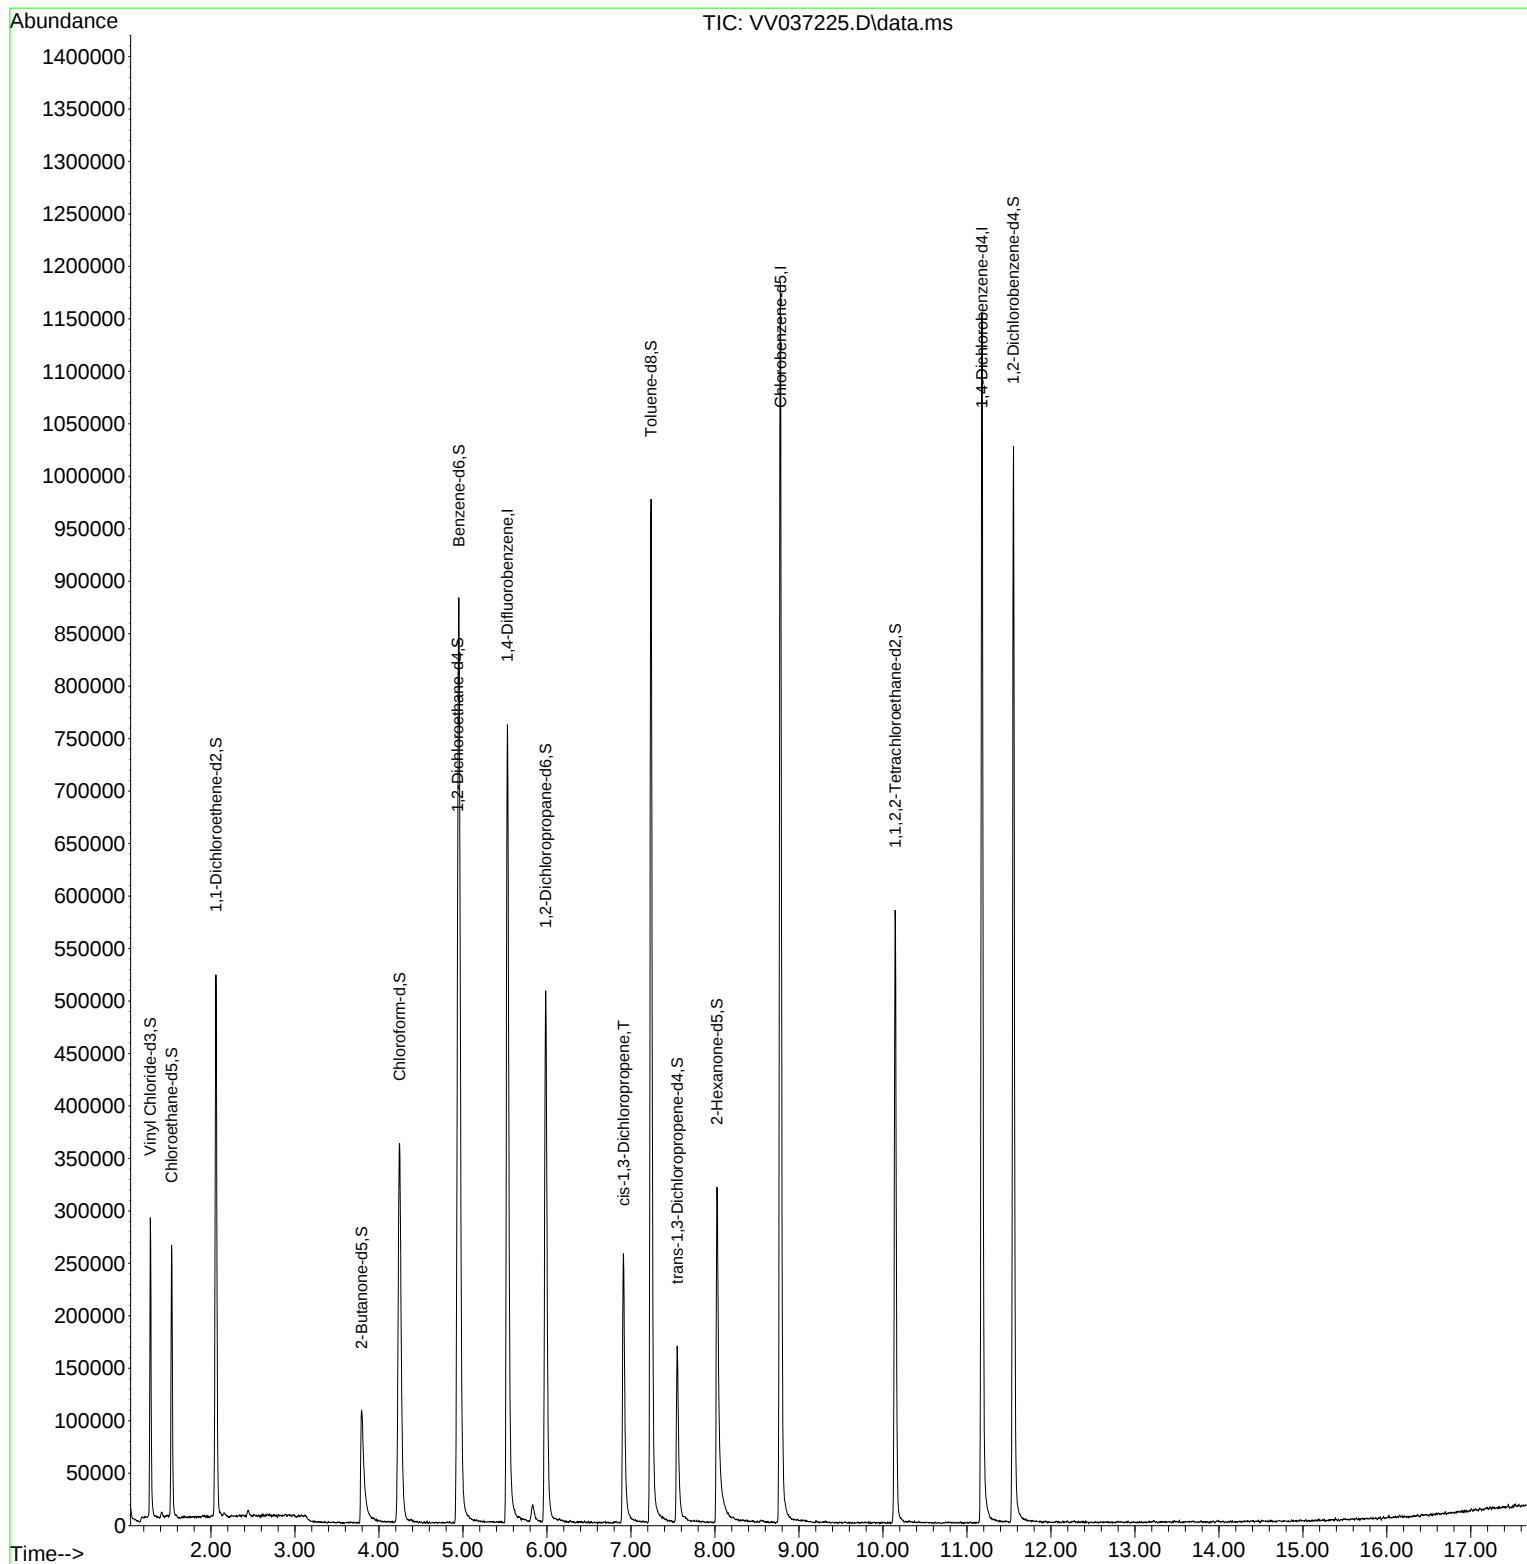

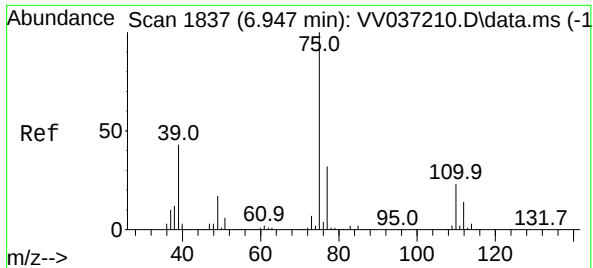

#39
 cis-1,3-Dichloropropene
 Concen: 0.833 ug/L
 RT: 6.915 min Scan# 11
 Delta R.T. -0.032 min
 Lab File: VV037225.D
 Acq: 06 Sep 2024 14:55

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 6526
 Ion Ratio Lower Upper
 75 100
 77 52.7 21.7 40.3#

