

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037215.D
 Acq On : 06 Sep 2024 11:20
 Operator : SY/MD
 Sample : P3843-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM6

Quant Time: Sep 06 23:23:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 06 23:21:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	669601	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	653167	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	297931	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	219358	35.812	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	71.620%		
7) Chloroethane-d5	1.532	69	193450	40.864	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.720%		
11) 1,1-Dichloroethene-d2	2.060	65	102439	39.791	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.580%		
21) 2-Butanone-d5	3.796	46	194711	82.087	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.090%		
24) Chloroform-d	4.246	84	431854	45.048	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.100%		
26) 1,2-Dichloroethane-d4	4.937	65	270482	44.803	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.600%		
32) Benzene-d6	4.953	84	864659	43.829	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.660%		
36) 1,2-Dichloropropane-d6	5.982	67	287541	46.534	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.060%		
41) Toluene-d8	7.239	98	750758	42.166	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.340%		
43) trans-1,3-Dichloroprop...	7.548	79	117969	41.266	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.540%		
47) 2-Hexanone-d5	8.024	63	113241	67.150	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	67.150%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	304006	40.566	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	81.140%		
66) 1,2-Dichlorobenzene-d4	11.554	152	284949	47.754	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.500%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	68532	26.940	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037215.D
Acq On : 06 Sep 2024 11:20
Operator : SY/MD
Sample : P3843-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM6

Quant Time: Sep 06 23:23:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 06 23:21:35 2024
Response via : Initial Calibration

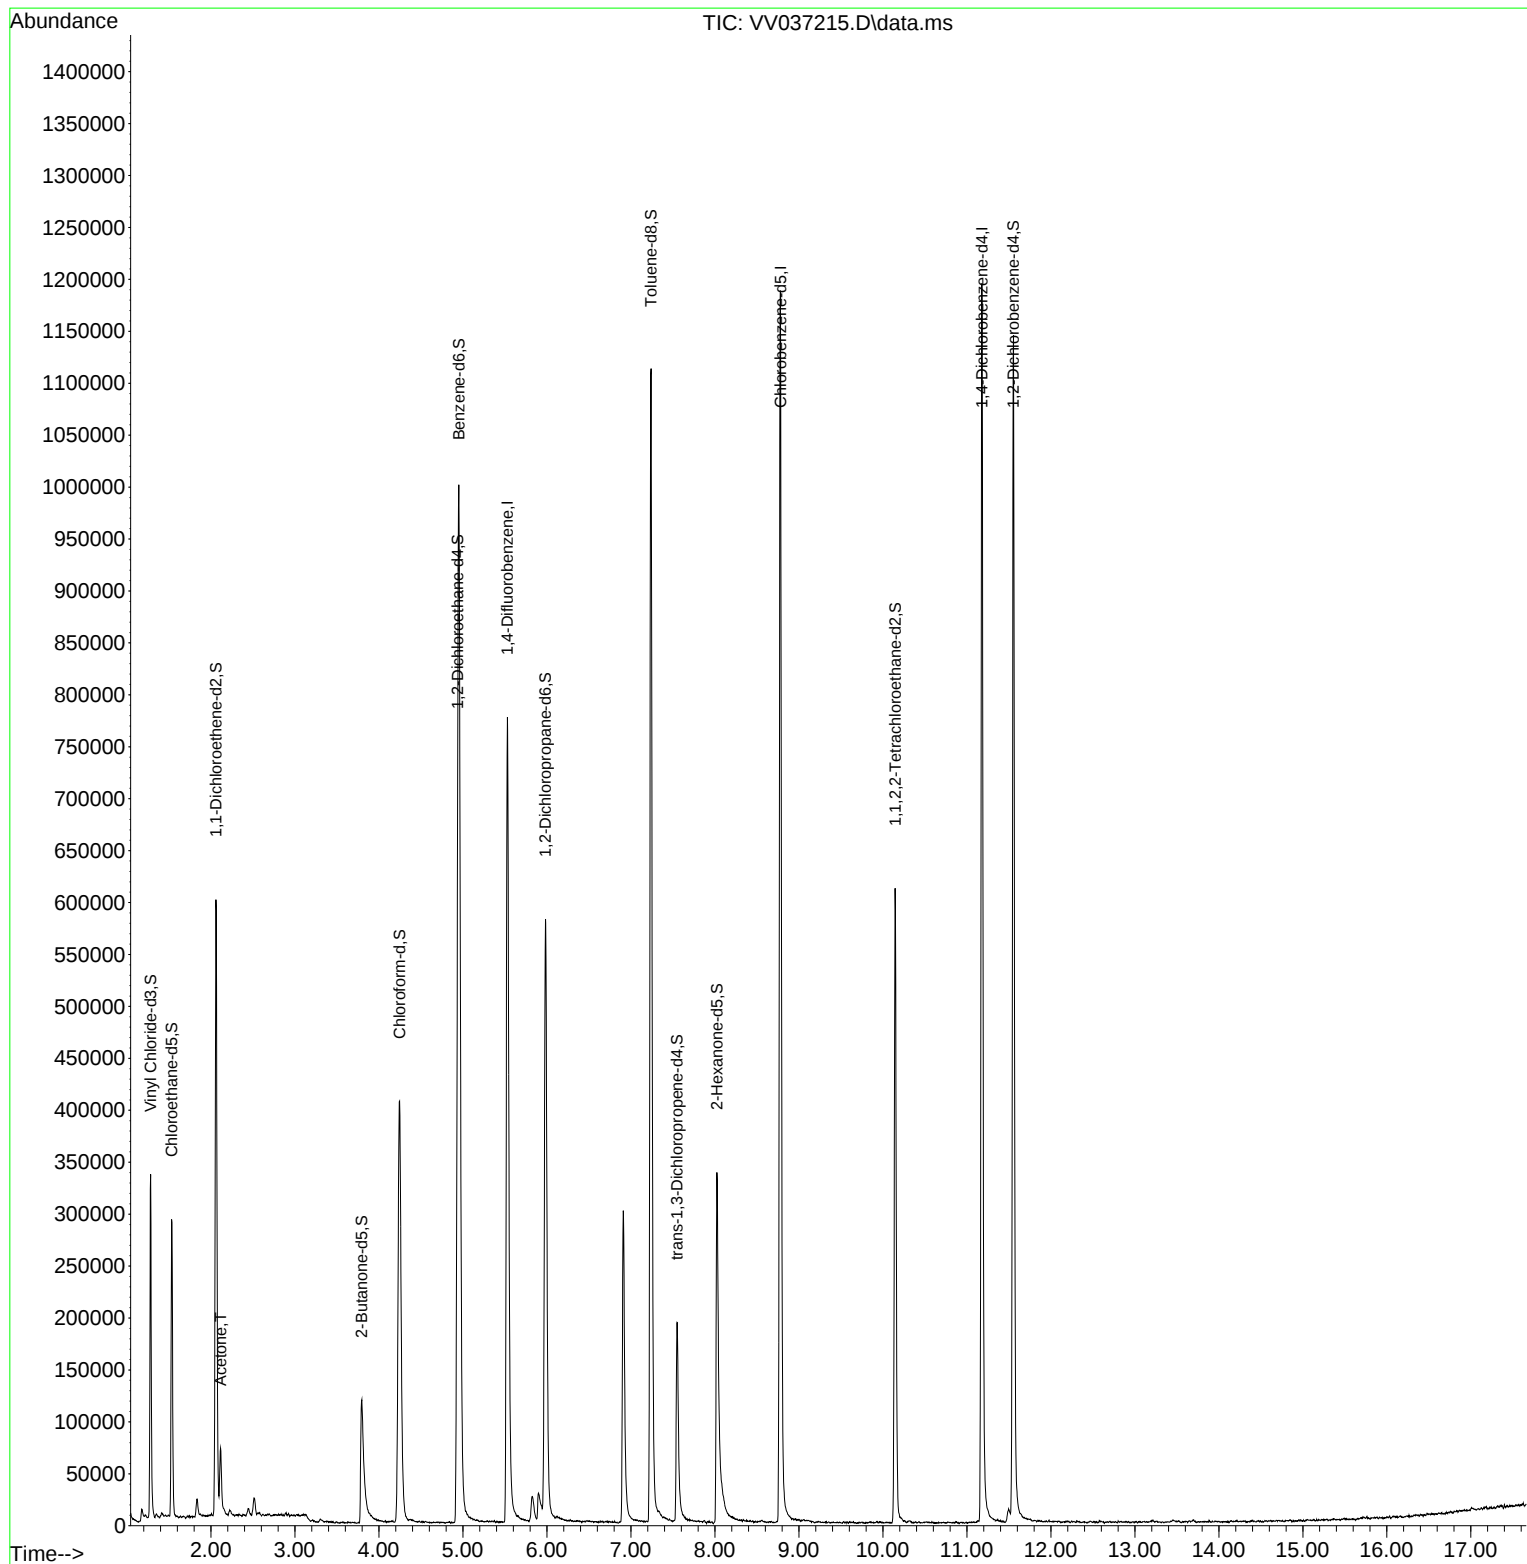

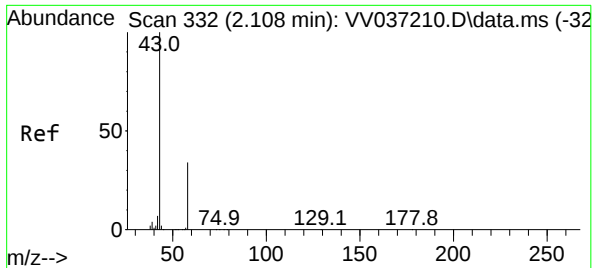

#13
 Acetone
 Concen: 26.940 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.007 min
 Lab File: VV037215.D
 Acq: 06 Sep 2024 11:20

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM6

Tgt Ion: 43 Resp: 68532
 Ion Ratio Lower Upper
 43 100
 58 31.4 0.0 64.8

