

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037221.D
 Acq On : 06 Sep 2024 13:29
 Operator : SY/MD
 Sample : P3843-07
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJL8

Quant Time: Sep 06 23:24:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 06 23:21:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	560803	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	548655	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	253482	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	189136	36.869	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	73.740%	
7) Chloroethane-d5	1.532	69	167968	42.365	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	84.740%	
11) 1,1-Dichloroethene-d2	2.060	65	88740	41.157	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	82.320%	
21) 2-Butanone-d5	3.796	46	170738	85.945	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	85.950%	
24) Chloroform-d	4.246	84	379772	47.301	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.600%	
26) 1,2-Dichloroethane-d4	4.937	65	244989	48.453	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.900%	
32) Benzene-d6	4.953	84	765717	46.207	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.420%	
36) 1,2-Dichloropropane-d6	5.985	67	255006	49.130	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	98.260%	
41) Toluene-d8	7.239	98	648078	43.333	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	86.660%	
43) trans-1,3-Dichloroprop...	7.551	79	104188	43.388	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	86.780%	
47) 2-Hexanone-d5	8.024	63	105904	74.761	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	74.760%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	279802	44.448	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	88.900%	
66) 1,2-Dichlorobenzene-d4	11.554	152	254383	50.108	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.220%	
Target Compounds					Qvalue	
13) Acetone	2.114	43	14345	6.733	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037221.D
Acq On : 06 Sep 2024 13:29
Operator : SY/MD
Sample : P3843-07
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJL8

Quant Time: Sep 06 23:24:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 06 23:21:35 2024
Response via : Initial Calibration

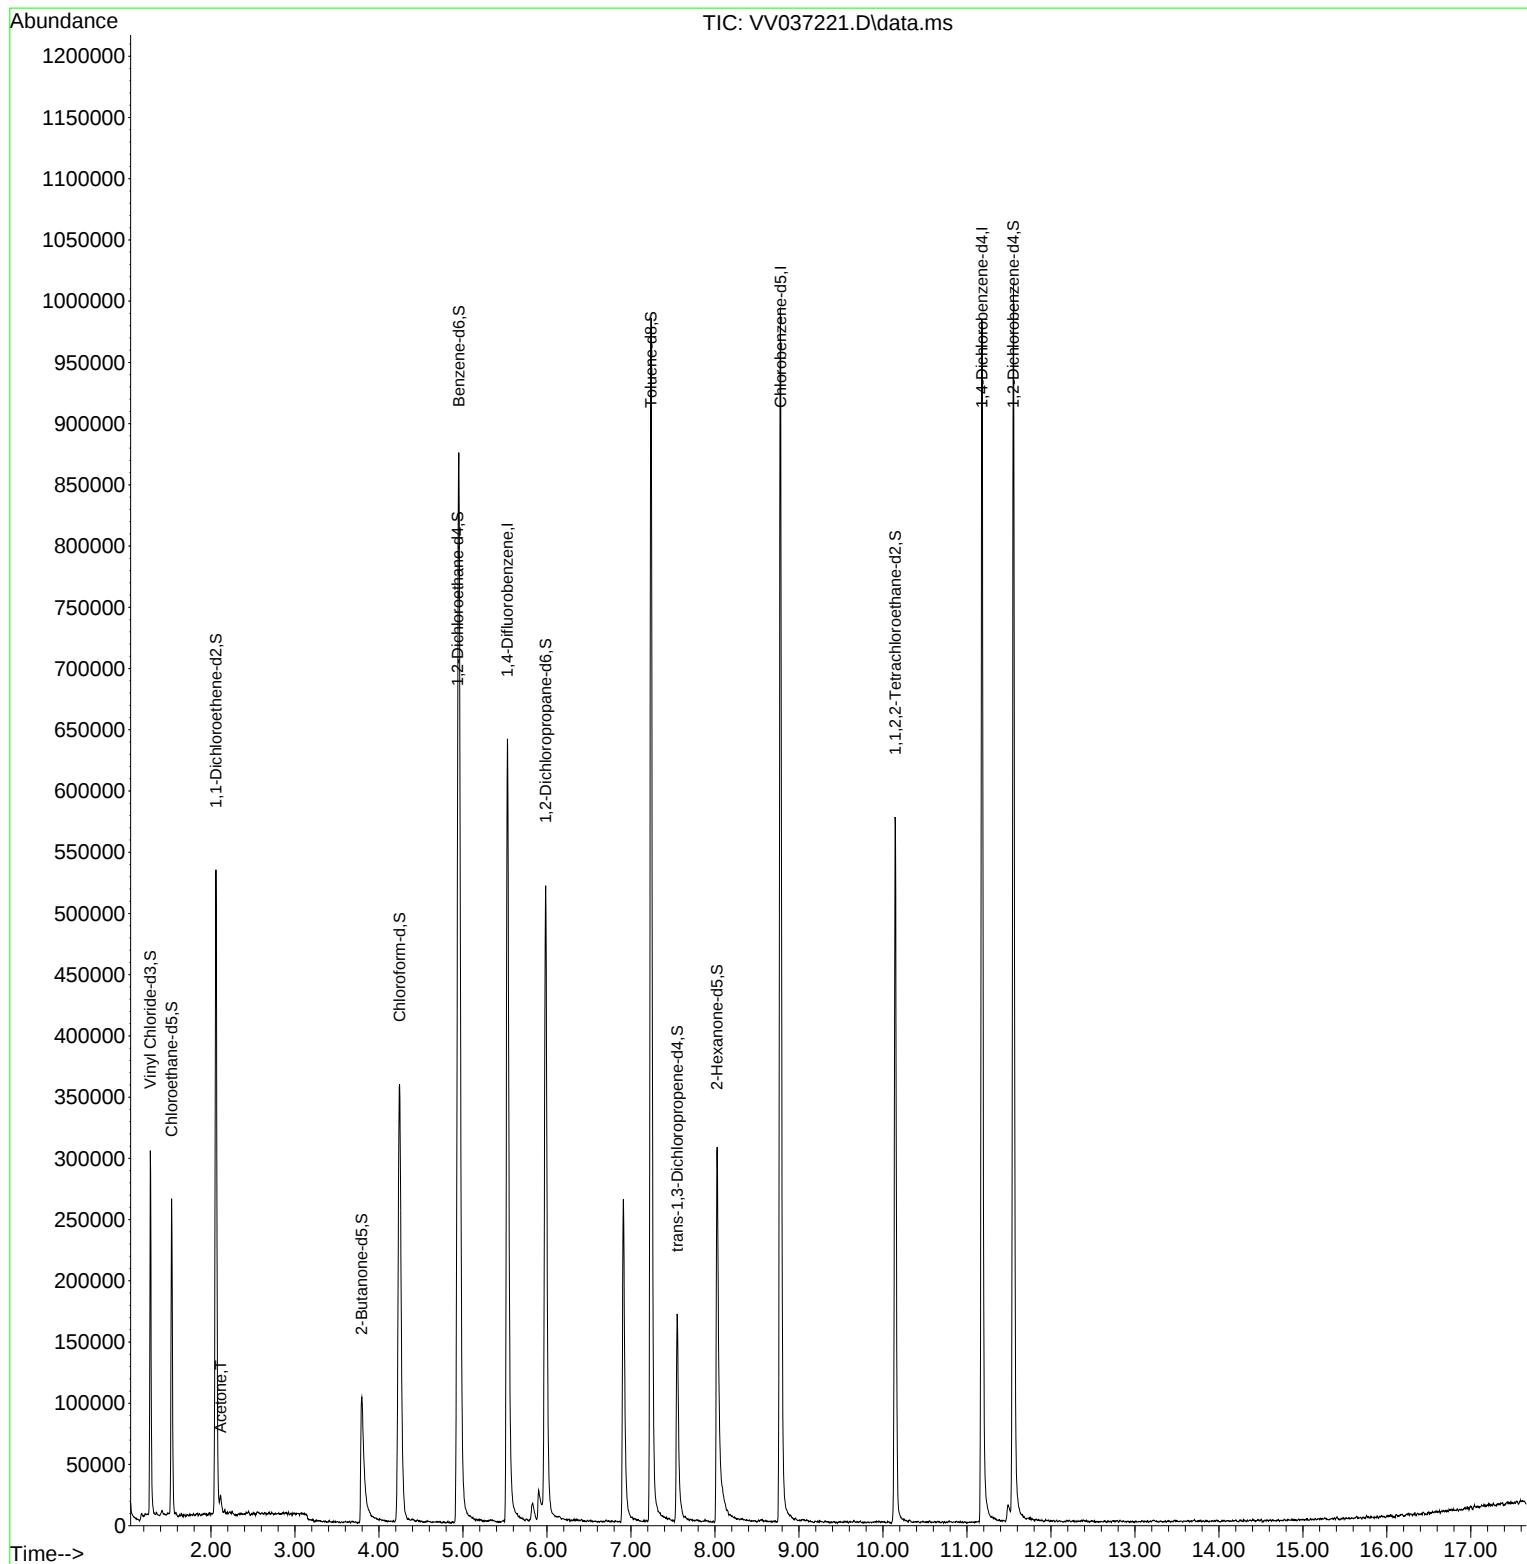

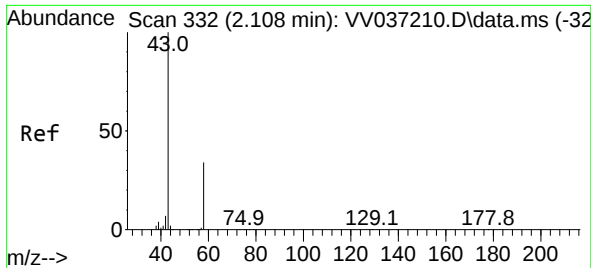

#13
 Acetone
 Concen: 6.733 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV037221.D
 Acq: 06 Sep 2024 13:29

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJL8

Tgt Ion: 43 Resp: 14345
 Ion Ratio Lower Upper
 43 100
 58 32.6 0.0 64.8

