

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037211.D
 Acq On : 06 Sep 2024 09:17
 Operator : SY/MD
 Sample : VV0906MBL01
 Misc : 5.00G/5 mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037211.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	36	41	50	rBV	15423	24076	0.88%	0.124%
2	1.278	68	74	90	rVB	428121	455221	16.63%	2.338%
3	1.532	146	153	167	rVB	334339	392914	14.36%	2.018%
4	2.056	307	316	341	rVB	697367	1021130	37.31%	5.244%
5	3.600	793	796	799	rBV4	1392	996	0.04%	0.005%
6	3.635	805	807	809	rVB	911	353	0.01%	0.002%
7	3.754	842	844	845	rBV	761	335	0.01%	0.002%
8	3.789	846	855	894	rVV	105853	311595	11.39%	1.600%
9	4.240	979	995	1027	rBV	421685	1092632	39.93%	5.611%
10	4.612	1107	1111	1112	rBV3	865	410	0.01%	0.002%
11	4.625	1112	1115	1117	rBV3	1278	899	0.03%	0.005%
12	4.805	1168	1171	1173	rBV3	958	612	0.02%	0.003%
13	4.838	1179	1181	1182	rBV	772	314	0.01%	0.002%
14	4.947	1196	1215	1251	rBV2	1060113	2736528	100.00%	14.052%
15	5.526	1383	1395	1430	rBV	742485	1549596	56.63%	7.957%
16	5.979	1521	1536	1570	rBV	599829	1249095	45.65%	6.414%
17	6.397	1663	1666	1667	rBV3	1287	618	0.02%	0.003%
18	6.500	1696	1698	1699	rBV2	994	280	0.01%	0.001%
19	6.532	1706	1708	1709	rBV2	917	348	0.01%	0.002%
20	6.696	1755	1759	1761	rBV5	1602	1332	0.05%	0.007%
21	6.709	1761	1763	1769	rVB5	2164	1581	0.06%	0.008%
22	6.735	1769	1771	1776	rBV5	1315	1014	0.04%	0.005%
23	6.796	1788	1790	1791	rBV2	1166	525	0.02%	0.003%
24	6.834	1800	1802	1804	rVB2	978	344	0.01%	0.002%
25	6.857	1806	1809	1810	rBV2	1218	516	0.02%	0.003%
26	6.905	1813	1824	1858	rBV	323446	622018	22.73%	3.194%
27	7.236	1915	1927	1973	rBV	1237580	2198364	80.33%	11.289%
28	7.548	2015	2024	2045	rBV	201824	375006	13.70%	1.926%
29	8.024	2163	2172	2205	rBV2	317014	705740	25.79%	3.624%
30	8.513	2322	2324	2329	rBV4	1475	1096	0.04%	0.006%
31	8.622	2356	2358	2360	rBV3	864	459	0.02%	0.002%
32	8.670	2367	2373	2375	rBV6	1497	1459	0.05%	0.007%
33	8.776	2394	2406	2443	rBV	1141667	1904747	69.60%	9.781%
34	9.204	2537	2539	2544	rVB5	1392	1207	0.04%	0.006%
35	9.230	2544	2547	2548	rBV2	845	494	0.02%	0.003%
36	9.329	2576	2578	2579	rBV2	794	311	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037211.D
 Acq On : 06 Sep 2024 09:17
 Operator : SY/MD
 Sample : VV0906MBL01
 Misc : 5.00G/5 mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.378	2589	2593	2597	rBV5	1470	1675	0.06%	0.009%
38	9.776	2715	2717	2721	rVB5	928	544	0.02%	0.003%
39	9.995	2780	2785	2787	rBV4	1000	1050	0.04%	0.005%
40	10.146	2820	2832	2848	rBV	605529	951618	34.77%	4.887%
41	10.378	2903	2904	2906	rBV	1071	511	0.02%	0.003%
42	10.445	2924	2925	2928	rVB2	1009	381	0.01%	0.002%
43	10.535	2950	2953	2954	rBV3	877	443	0.02%	0.002%
44	10.606	2972	2975	2978	rBV5	1043	815	0.03%	0.004%
45	10.712	3005	3008	3009	rBV3	784	433	0.02%	0.002%
46	10.818	3039	3041	3042	rBV2	233	51	0.00%	0.000%
47	10.857	3044	3053	3065	rVB8	4941	8528	0.31%	0.044%
48	10.911	3065	3070	3074	rBV6	1342	1467	0.05%	0.008%
49	10.953	3080	3083	3085	rBV4	1314	819	0.03%	0.004%
50	10.979	3087	3091	3094	rVV6	1302	1018	0.04%	0.005%
51	11.030	3103	3107	3110	rBV4	1005	859	0.03%	0.004%
52	11.123	3128	3136	3142	rBV7	7149	12734	0.47%	0.065%
53	11.178	3143	3153	3181	rVV	1171060	1847943	67.53%	9.489%
54	11.554	3258	3270	3294	rBV	1159426	1888884	69.02%	9.700%
55	12.049	3421	3424	3425	rBV3	1392	741	0.03%	0.004%
56	12.059	3425	3427	3429	rVV3	1135	482	0.02%	0.002%
57	12.104	3439	3441	3443	rBV2	1155	557	0.02%	0.003%
58	12.432	3540	3543	3545	rBV3	1310	835	0.03%	0.004%
59	12.654	3610	3612	3614	rBV2	1000	421	0.02%	0.002%
60	12.773	3647	3649	3651	rBV2	1088	552	0.02%	0.003%
61	12.802	3656	3658	3660	rBV3	1068	565	0.02%	0.003%
62	13.024	3724	3727	3730	rBV3	1406	1180	0.04%	0.006%
63	13.107	3752	3753	3755	rBV2	1255	510	0.02%	0.003%
64	13.204	3776	3783	3796	rVB5	14964	24013	0.88%	0.123%
65	13.442	3848	3857	3873	rBV	33501	66685	2.44%	0.342%
66	13.905	3998	4001	4002	rBV2	1157	762	0.03%	0.004%
67	14.731	4255	4258	4264	rBV5	2338	2388	0.09%	0.012%




Sum of corrected areas: 19473629

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037211.D
Acq On : 06 Sep 2024 09:17
Operator : SY/MD
Sample : VV0906MBL01
Misc : 5.00G/5 mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

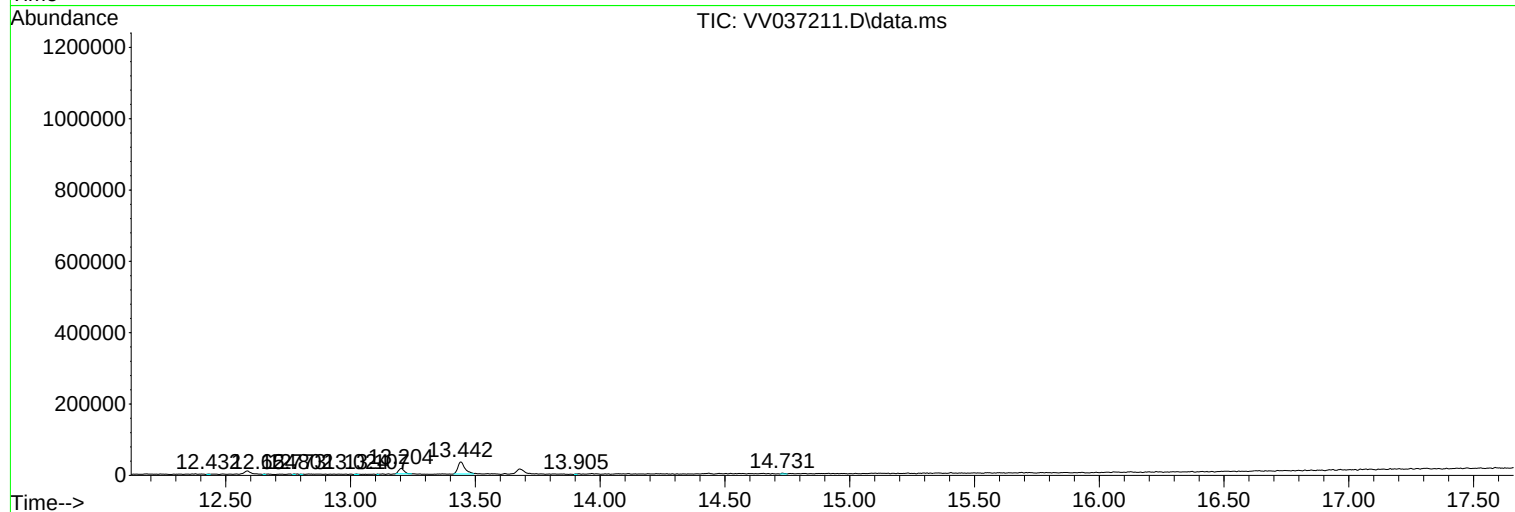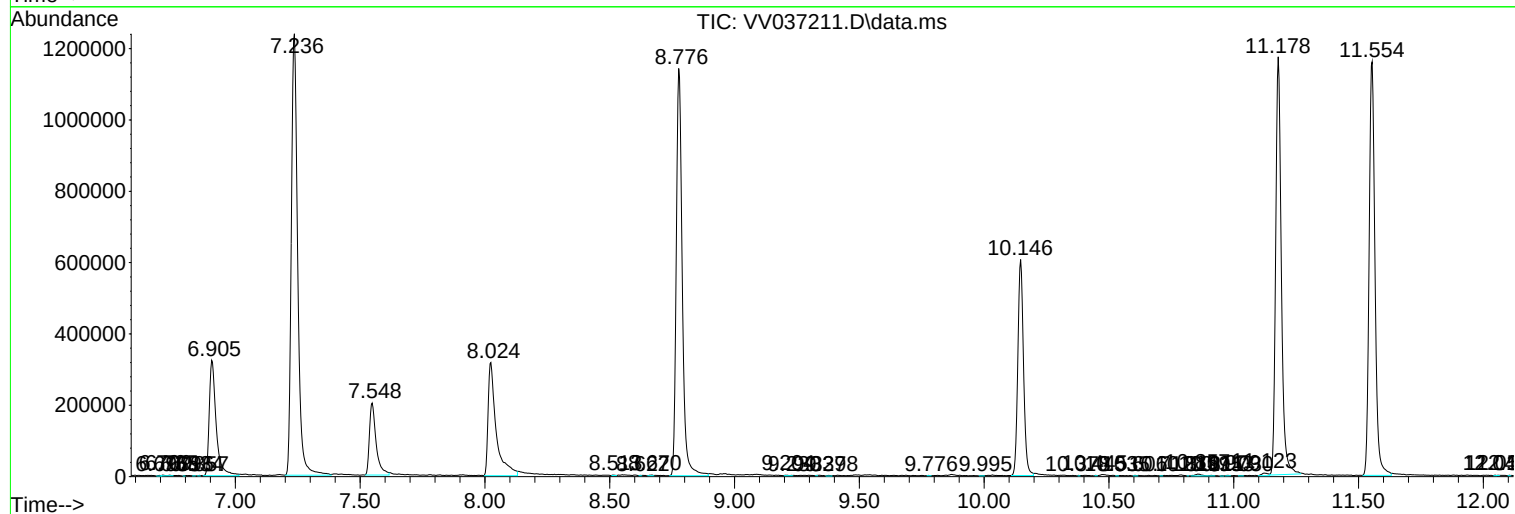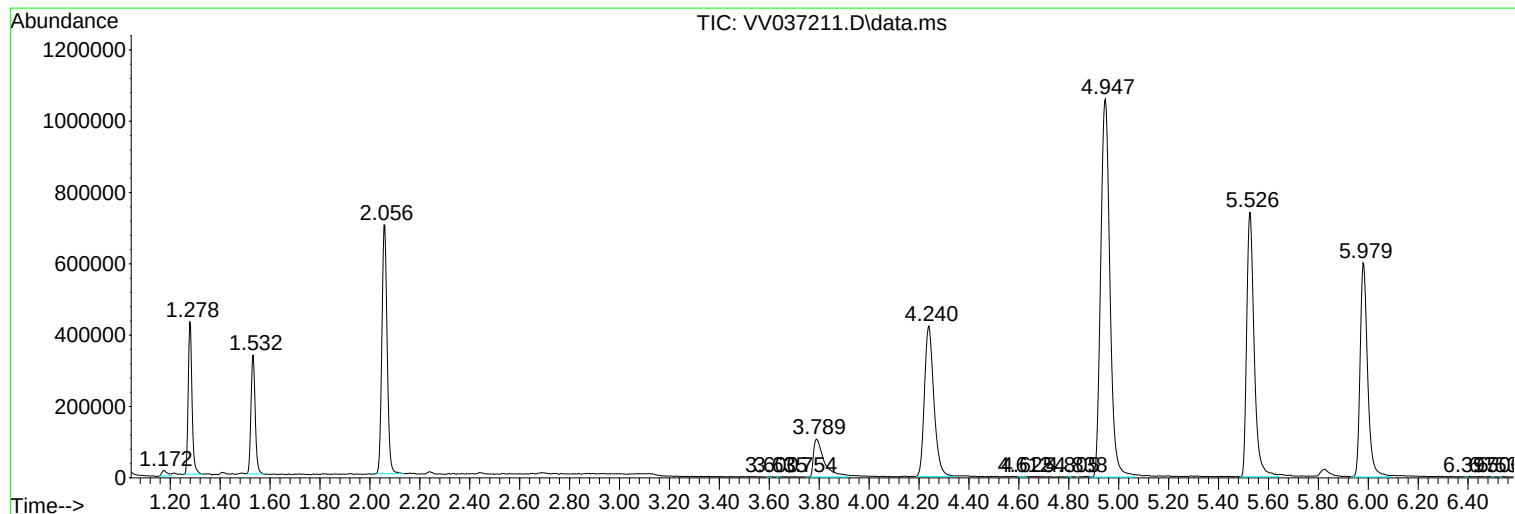

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037211.D
Acq On : 06 Sep 2024 09:17
Operator : SY/MD
Sample : VV0906MBL01
Misc : 5.00G/5 mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037211.D
Acq On : 06 Sep 2024 09:17
Operator : SY/MD
Sample : VV0906MBL01
Misc : 5.00G/5 mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc